

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111321\
 Data File : BP007971.D
 Acq On : 13 Nov 2021 17:22
 Operator : CG/JU
 Sample : PB140688BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB140688BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111321.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP007971.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.428	357	364	376	rBV	2474765	3620853	35.38%	8.975%
2	7.022	626	635	649	rBV	2255205	3718234	36.33%	9.217%
3	7.840	766	774	783	rBV	443312	696690	6.81%	1.727%
4	8.999	963	971	983	rBV	1290252	2154132	21.05%	5.340%
5	10.640	1240	1250	1264	rBV	538432	916067	8.95%	2.271%
6	13.104	1660	1669	1685	rBV	3731205	5506985	53.80%	13.651%
7	14.481	1896	1903	1912	rBV	913778	1353920	13.23%	3.356%
8	15.975	2149	2157	2180	rBV	3509303	5142844	50.25%	12.748%
9	17.234	2365	2371	2385	rBV	1200820	1806019	17.64%	4.477%
10	19.804	2802	2808	2821	rBV	8435506	10235488	100.00%	25.372%
11	21.328	3062	3067	3074	rBV	1909306	2473613	24.17%	6.132%
12	23.739	3470	3477	3490	rVB2	1323788	2717383	26.55%	6.736%




Sum of corrected areas: 40342228

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111321\
Data File : BP007971.D
Acq On : 13 Nov 2021 17:22
Operator : CG/JU
Sample : PB140688BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB140688BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

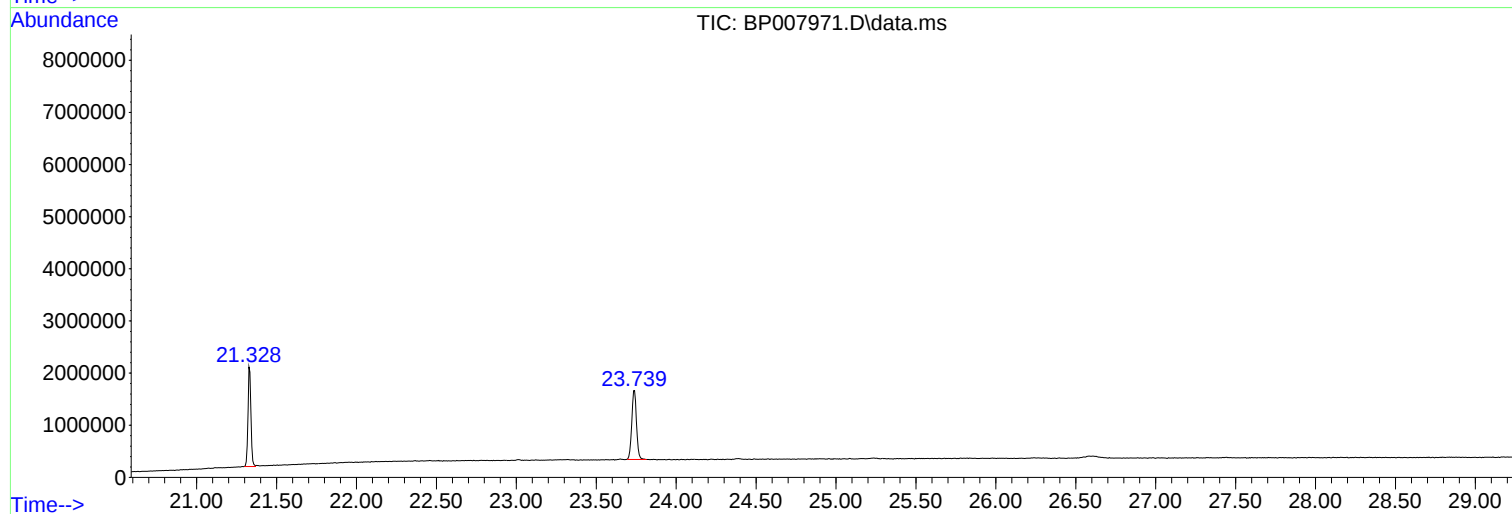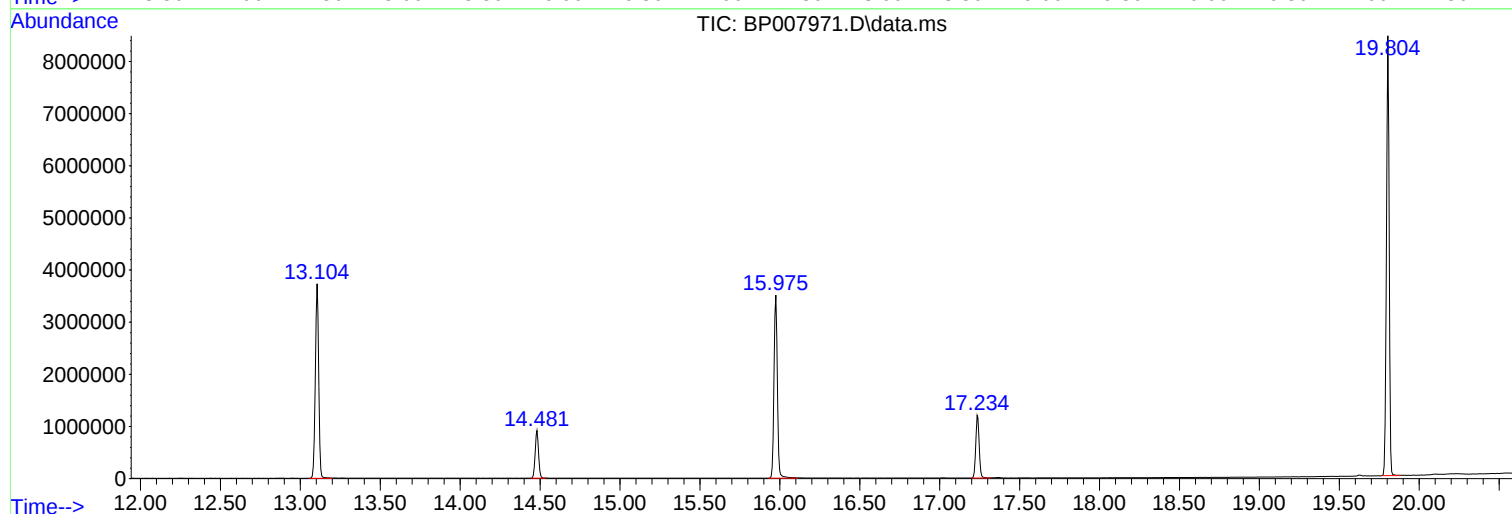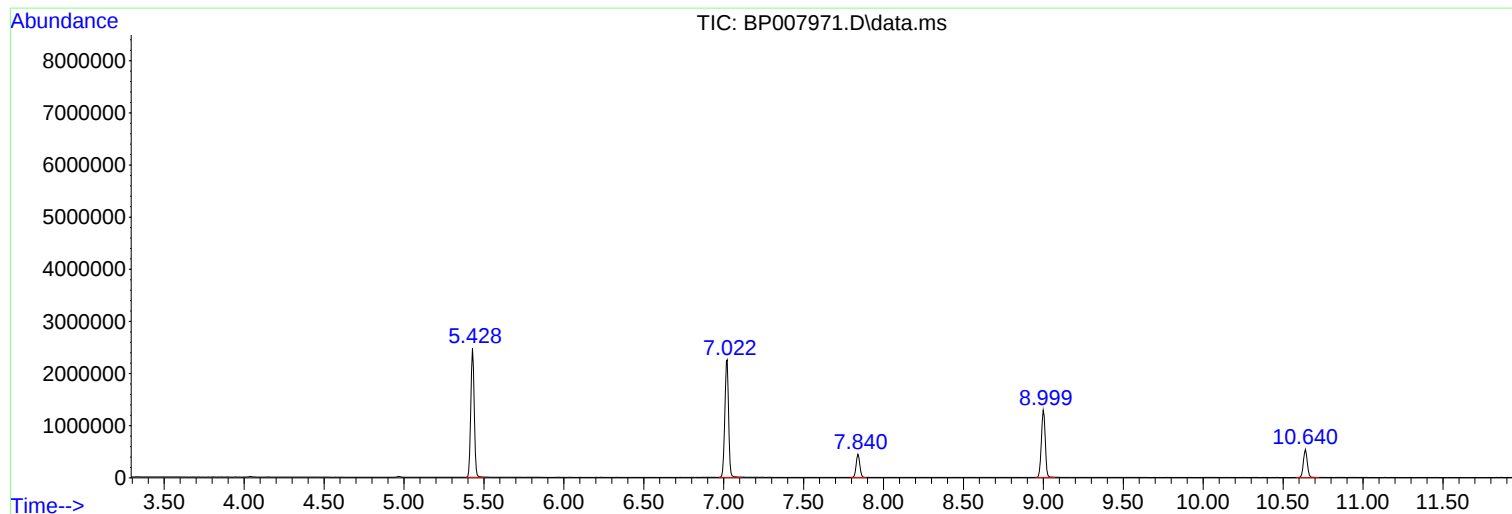

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111321\
Data File : BP007971.D
Acq On : 13 Nov 2021 17:22
Operator : CG/JU
Sample : PB140688BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB140688BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111321\
Data File : BP007971.D
Acq On : 13 Nov 2021 17:22
Operator : CG/JU
Sample : PB140688BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB140688BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------