

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111321\
 Data File : BP007972.D
 Acq On : 13 Nov 2021 17:55
 Operator : CG/JU
 Sample : PB140690BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB140690BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP007972.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.428	357	364	379	rBV	2406208	3560409	36.48%	9.189%
2	7.016	626	634	651	rBV	2227544	3633247	37.23%	9.377%
3	7.840	767	774	785	rVB	424124	674941	6.92%	1.742%
4	8.999	963	971	987	rBV	1247957	2109113	21.61%	5.444%
5	10.640	1242	1250	1260	rBV	521081	895222	9.17%	2.311%
6	13.104	1661	1669	1685	rBV	3487362	5271735	54.01%	13.606%
7	14.481	1895	1903	1917	rBV	879634	1298058	13.30%	3.350%
8	15.975	2148	2157	2182	rBV	3313749	4830308	49.49%	12.467%
9	17.234	2365	2371	2386	rBV	1122610	1708844	17.51%	4.410%
10	19.804	2802	2808	2818	rBV	7953846	9759916	100.00%	25.190%
11	21.328	3062	3067	3074	rBV	1804867	2345518	24.03%	6.054%
12	23.739	3470	3477	3488	rVB2	1275946	2657853	27.23%	6.860%




Sum of corrected areas: 38745164

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111321\
Data File : BP007972.D
Acq On : 13 Nov 2021 17:55
Operator : CG/JU
Sample : PB140690BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB140690BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

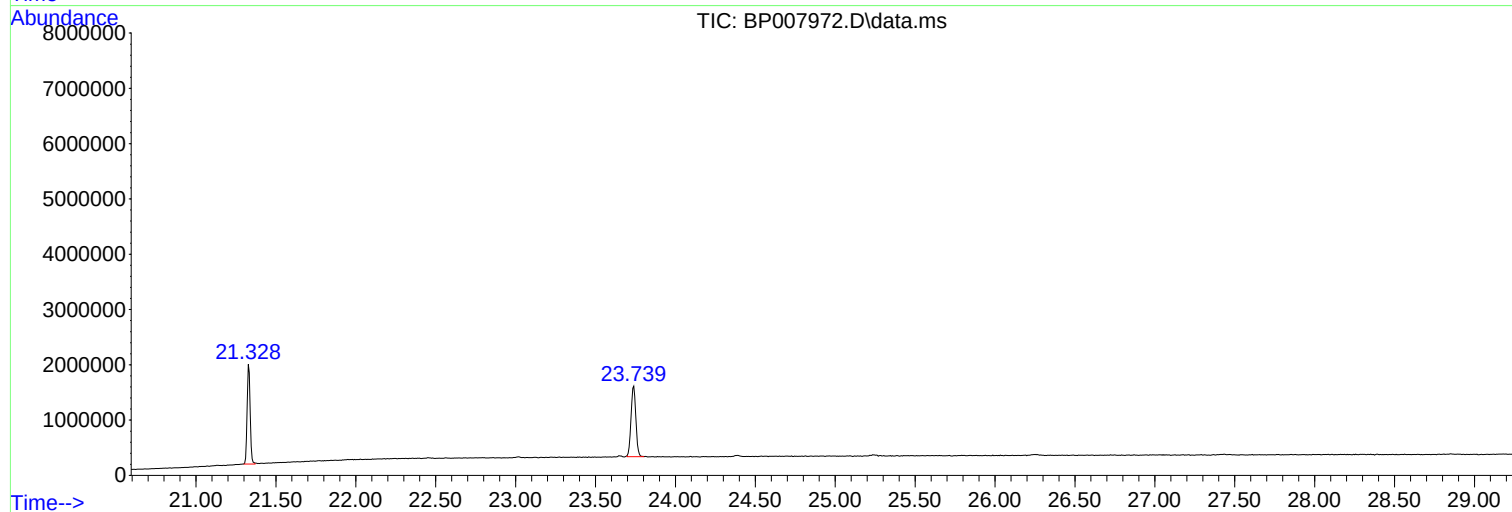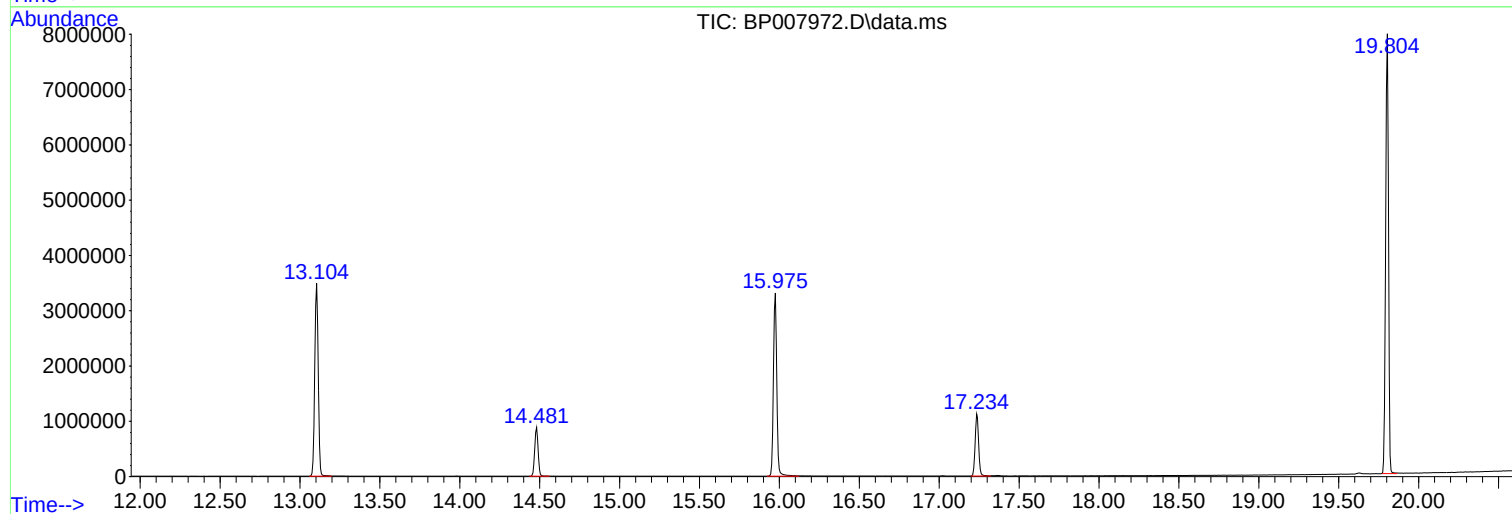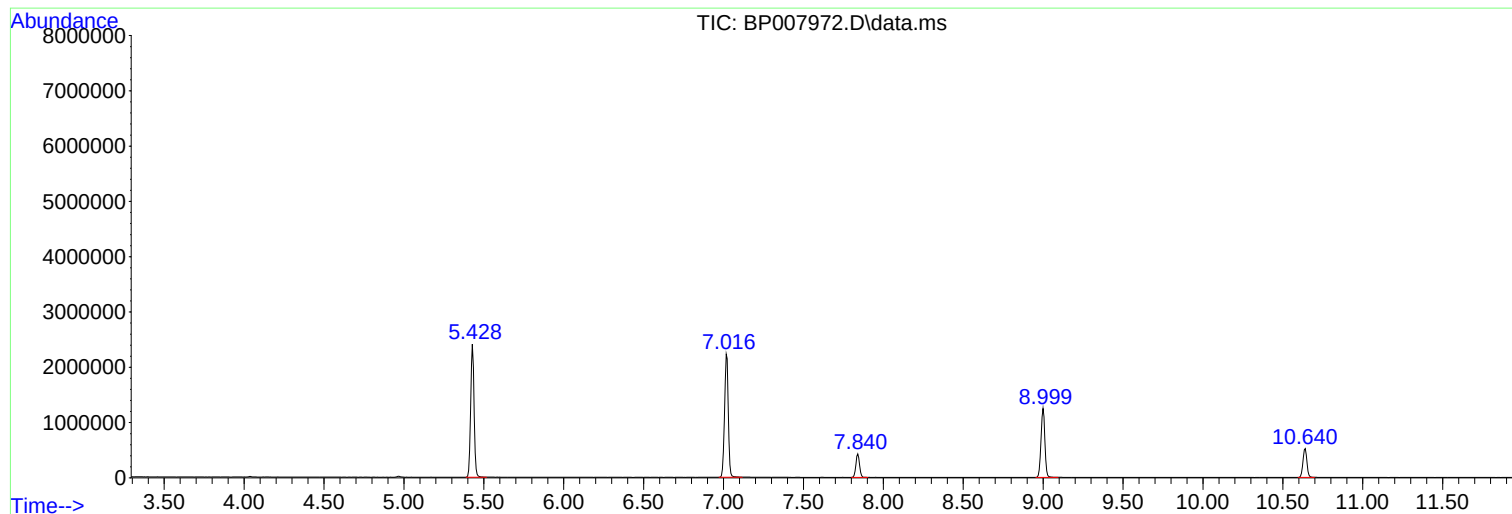

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111321\
Data File : BP007972.D
Acq On : 13 Nov 2021 17:55
Operator : CG/JU
Sample : PB140690BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB140690BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111321\
Data File : BP007972.D
Acq On : 13 Nov 2021 17:55
Operator : CG/JU
Sample : PB140690BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB140690BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------