


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111321\
 Data File : BP007962.D
 Acq On : 13 Nov 2021 11:43
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Nov 15 05:36:49 2021

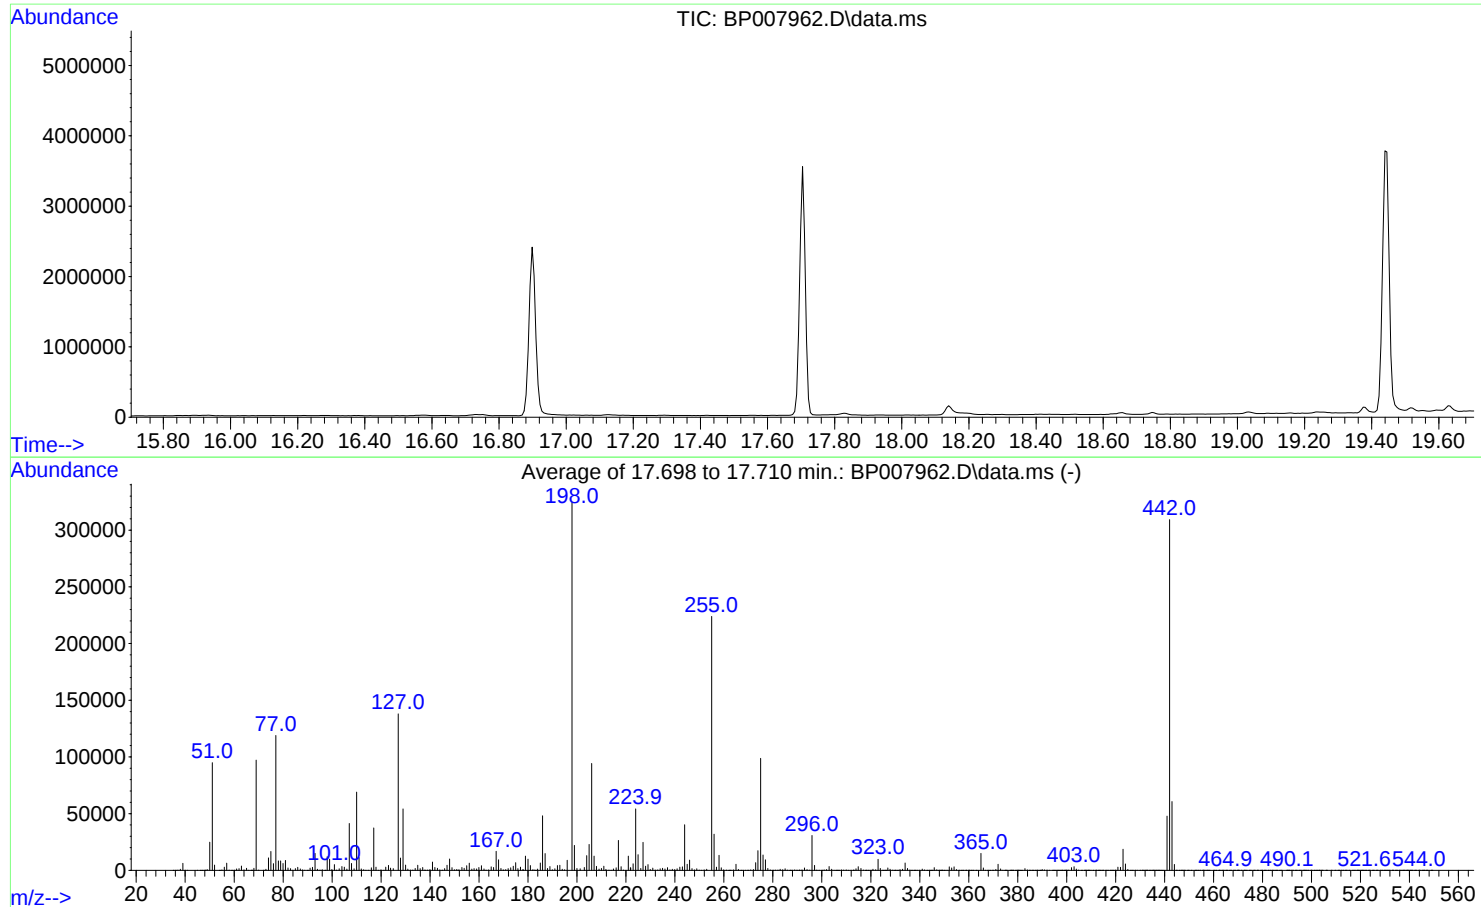




AutoFind: Scans 2450, 2451, 2452; Background Corrected with Scan 2441

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.3	94926	PASS
68	69	0.00	2	1.9	1876	PASS
69	198	0.00	100	30.0	97265	PASS
70	69	0.00	2	0.3	339	PASS
127	198	10	80	42.6	138015	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	324356	PASS
199	198	5	9	6.8	21984	PASS
275	198	10	60	30.5	98773	PASS
365	198	1	100	4.6	14927	PASS
441	198	0.01	100	14.7	47803	PASS
442	442	100	100	100.0	309184	PASS
443	442	15	24	19.6	60640	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111321\
 Data File : BP007962.D
 Acq On : 13 Nov 2021 11:43
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Nov 15 08:22:50 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 15 05:36:49 2021
 Response via : Initial Calibration

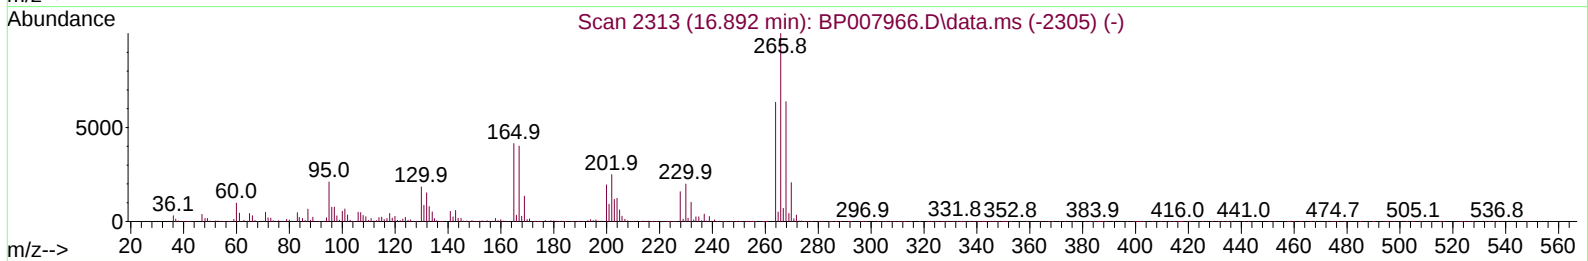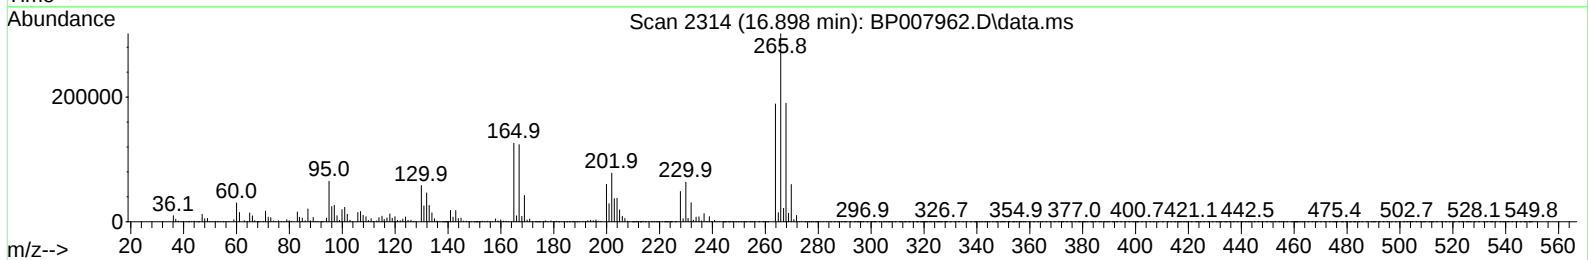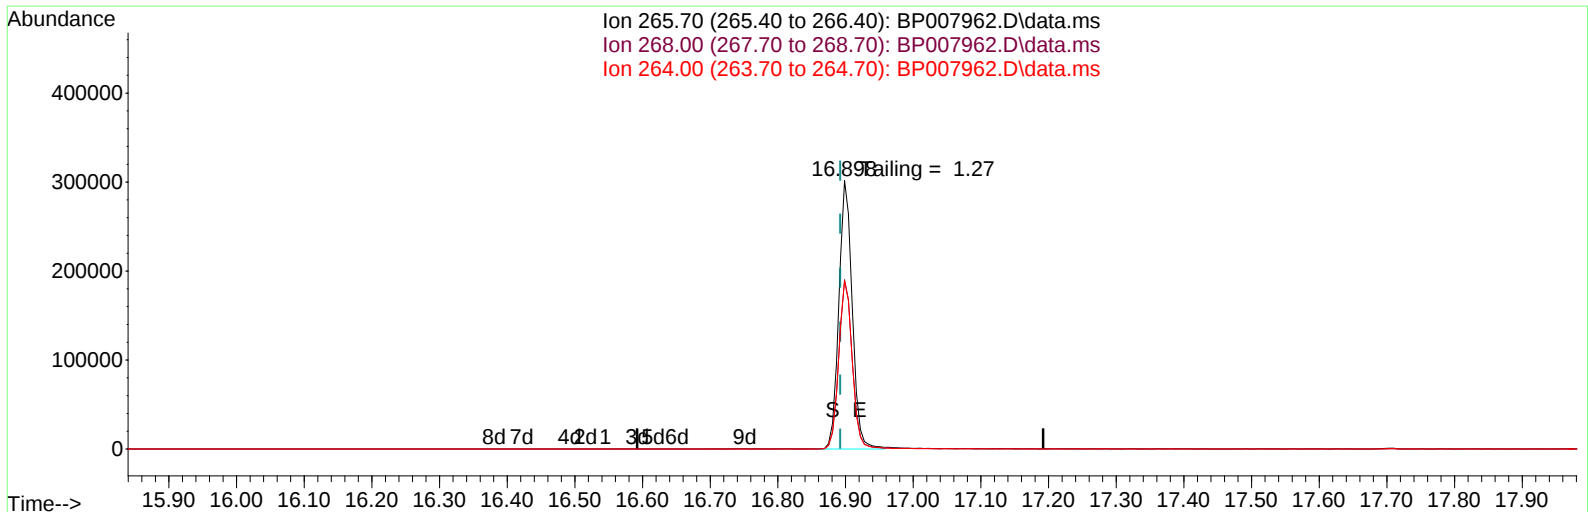

TIC: BP007962.D\data.ms

(70) Pentachlorophenol (C)

16.898min (+ 0.006) 137441.43 ng m




response 417306

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.60	63.08
264.00	60.90	62.68
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111321\
 Data File : BP007962.D
 Acq On : 13 Nov 2021 11:43
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Nov 15 08:22:50 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 15 05:36:49 2021
 Response via : Initial Calibration

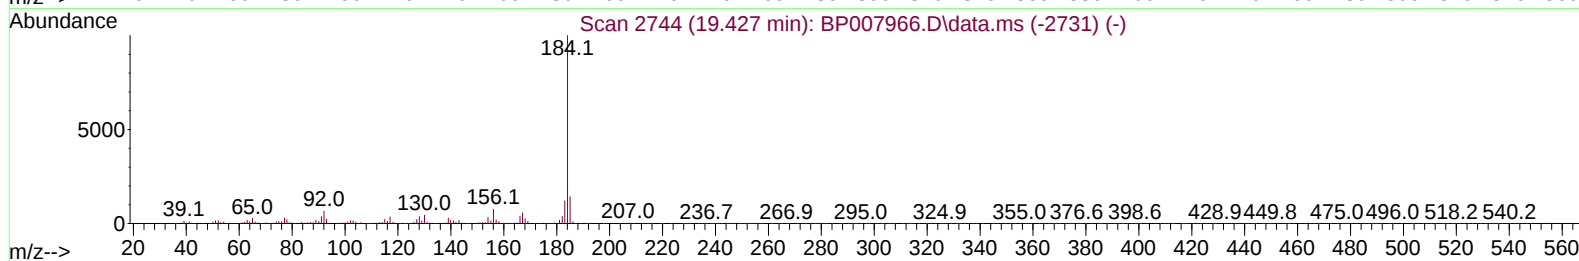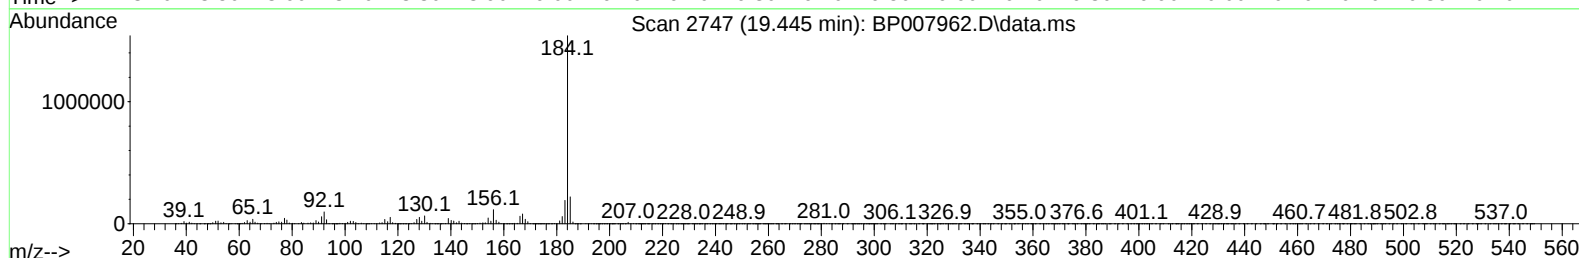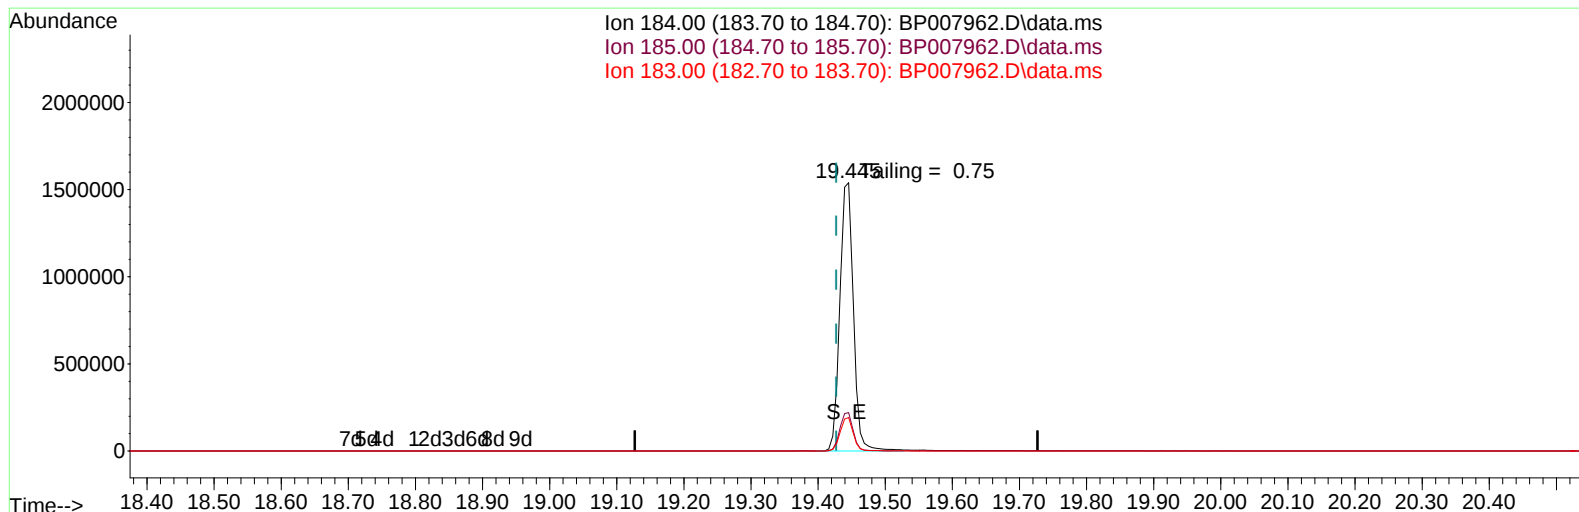

TIC: BP007962.D\data.ms

(77) Benzidine

19.445min (+ 0.018) 7973.63 ng m

response 2169002

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	14.34
183.00	11.40	12.47
0.00	0.00	0.00

Instrument :
BNA_P
ClientSampleId :
DFTPP

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/13/2021	BNA_P	BP007962.D
Compound Name	Response	Retention Time
DDT	1231994	20.651
DDD	19581	20.222
DDE	2827	19.728
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
22408	1254402	1.79

Instrument :
BNA_P
ClientSampleId :
DFTPP