

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111521\
Data File : BP007989.D
Acq On : 15 Nov 2021 19:19
Operator : CG/JU
Sample : PB140390BL
Misc : LOQ-WATER 10ppm
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB140390BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111321.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP007989.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.428	357	364	376	rBV	2762872	4004167	37.48%	9.292%
2	7.016	626	634	647	rBV	2543928	4102188	38.40%	9.520%
3	7.840	763	774	783	rBV	498120	799478	7.48%	1.855%
4	8.999	958	971	981	rBV	1421601	2370479	22.19%	5.501%
5	10.634	1239	1249	1265	rBV	574880	1023834	9.58%	2.376%
6	13.104	1661	1669	1684	rBV	3957272	6019678	56.35%	13.970%
7	14.475	1896	1902	1915	rBV	1002109	1482389	13.88%	3.440%
8	15.969	2144	2156	2180	rBV	3586663	5455874	51.07%	12.661%
9	17.234	2364	2371	2385	rBV	1320874	1948687	18.24%	4.522%
10	19.804	2801	2808	2819	rBV	8492801	10683464	100.00%	24.793%
11	21.327	3062	3067	3077	rBV	1925720	2500567	23.41%	5.803%
12	23.733	3469	3476	3490	rVB2	1318550	2700413	25.28%	6.267%




Sum of corrected areas: 43091218

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111521\
Data File : BP007989.D
Acq On : 15 Nov 2021 19:19
Operator : CG/JU
Sample : PB140390BL
Misc : LOQ-WATER 10ppm
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB140390BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

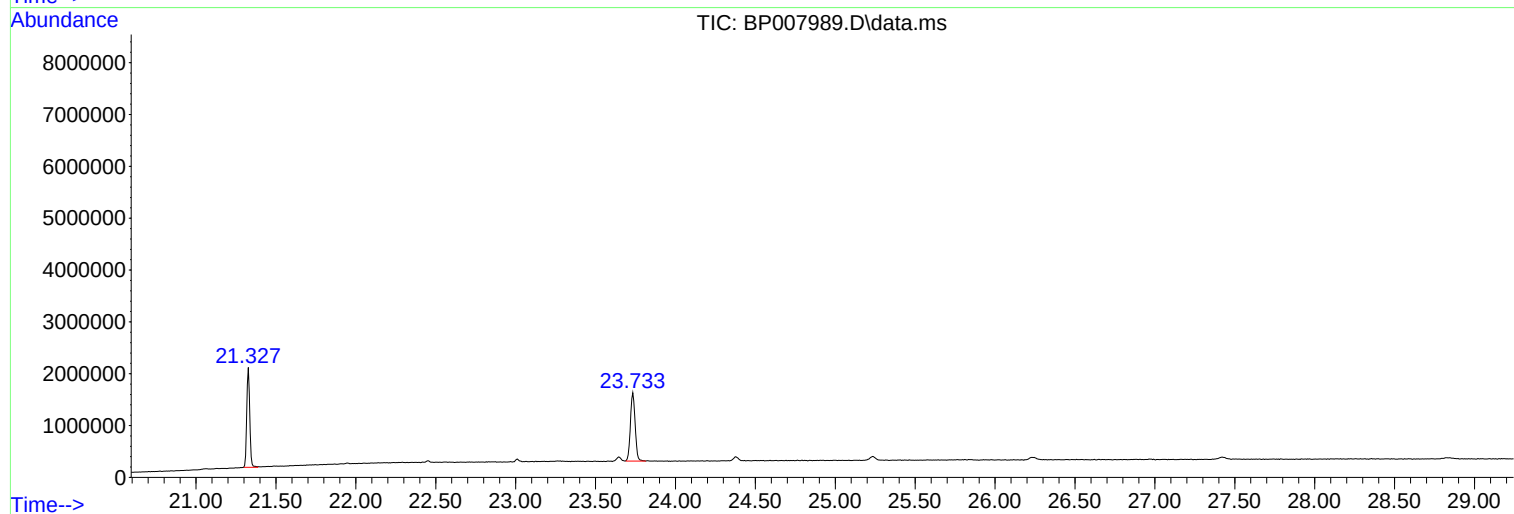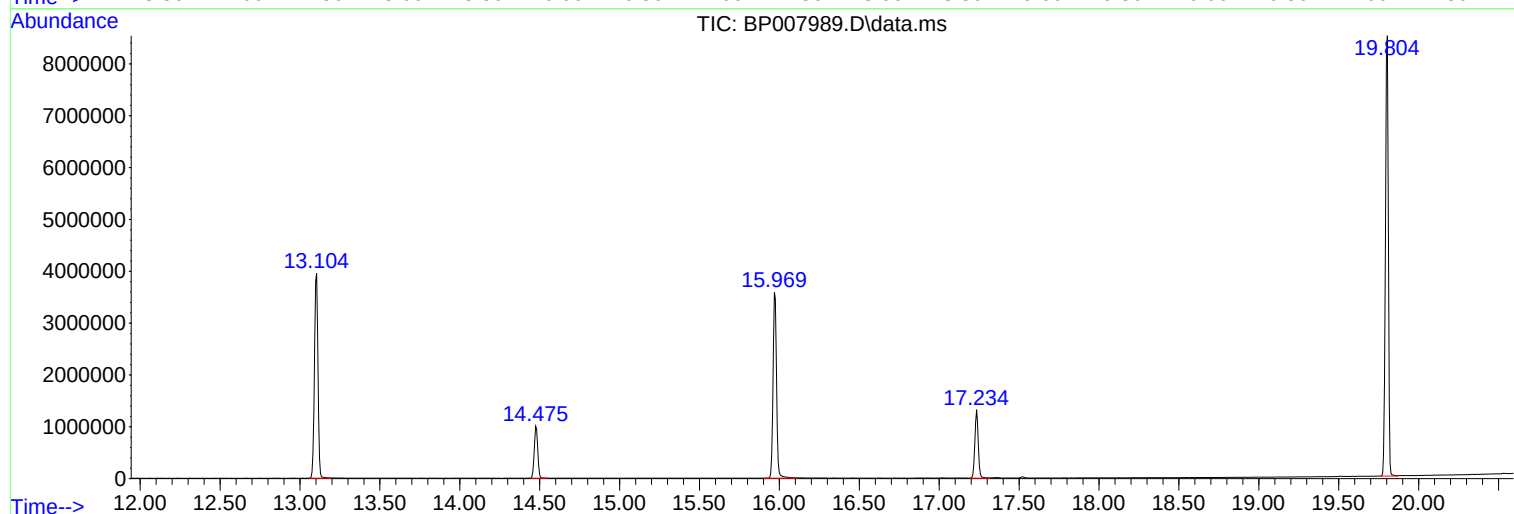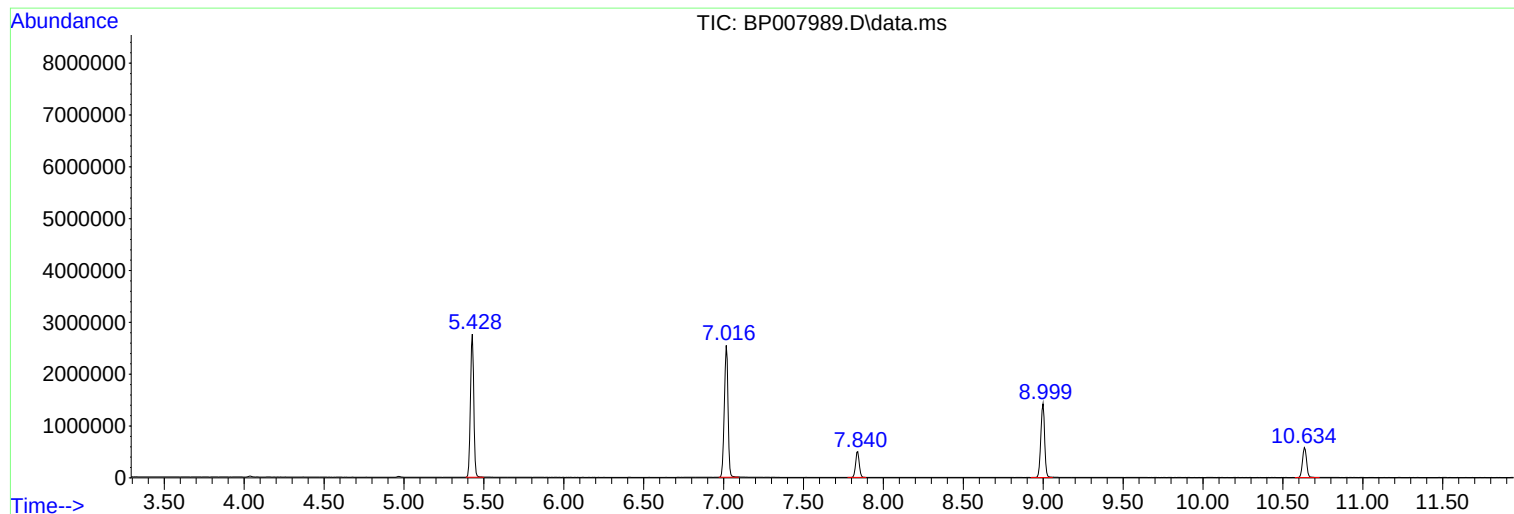

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111521\
Data File : BP007989.D
Acq On : 15 Nov 2021 19:19
Operator : CG/JU
Sample : PB140390BL
Misc : LOQ-WATER 10ppm
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB140390BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111521\
Data File : BP007989.D
Acq On : 15 Nov 2021 19:19
Operator : CG/JU
Sample : PB140390BL
Misc : LOQ-WATER 10ppm
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB140390BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------