
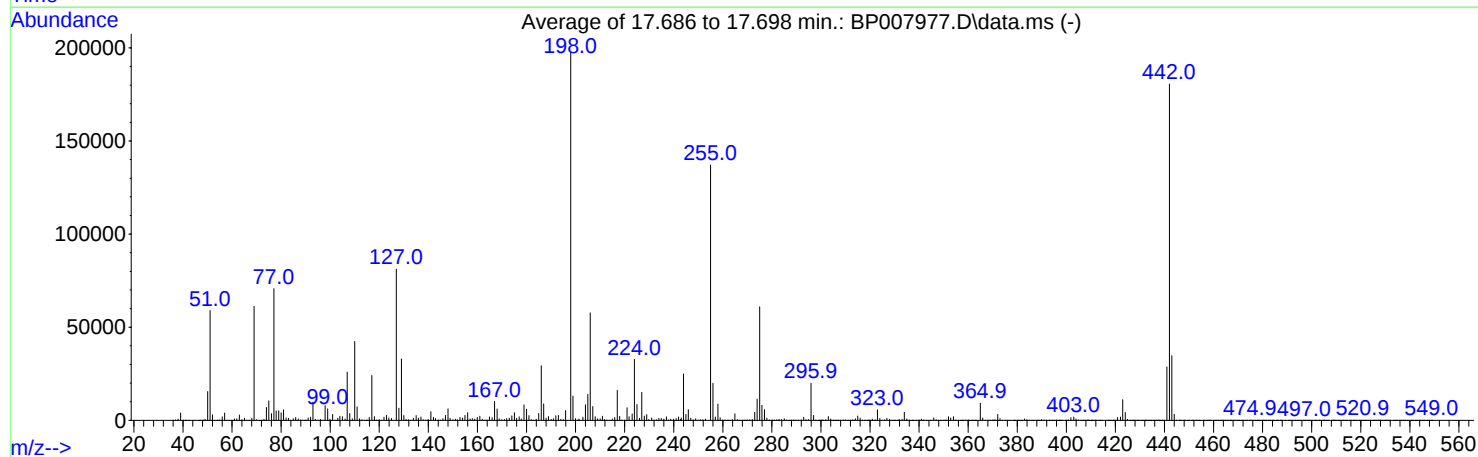


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111521\
 Data File : BP007977.D
 Acq On : 15 Nov 2021 09:41
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Nov 15 05:36:49 2021

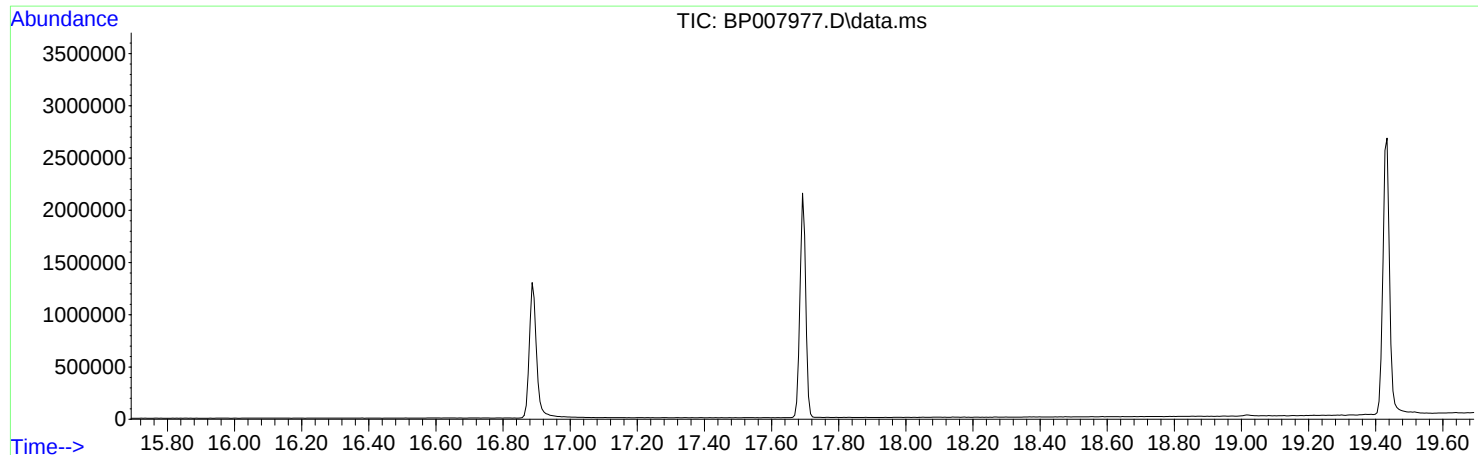


AutoFind: Scans 2448, 2449, 2450; Background Corrected with Scan 2439

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.9	58984	PASS
68	69	0.00	2	1.9	1164	PASS
69	198	0.00	100	31.0	61237	PASS
70	69	0.00	2	0.5	323	PASS
127	198	10	80	41.1	81162	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	197504	PASS
199	198	5	9	6.6	13093	PASS
275	198	10	60	30.9	60971	PASS
365	198	1	100	4.6	9183	PASS
441	198	0.01	100	14.5	28694	PASS
442	442	100	100	100.0	180536	PASS
443	442	15	24	19.2	34683	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111521\
Data File : BP007977.D
Acq On : 15 Nov 2021 09:41
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Nov 15 12:21:52 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 15 12:21:36 2021
Response via : Initial Calibration

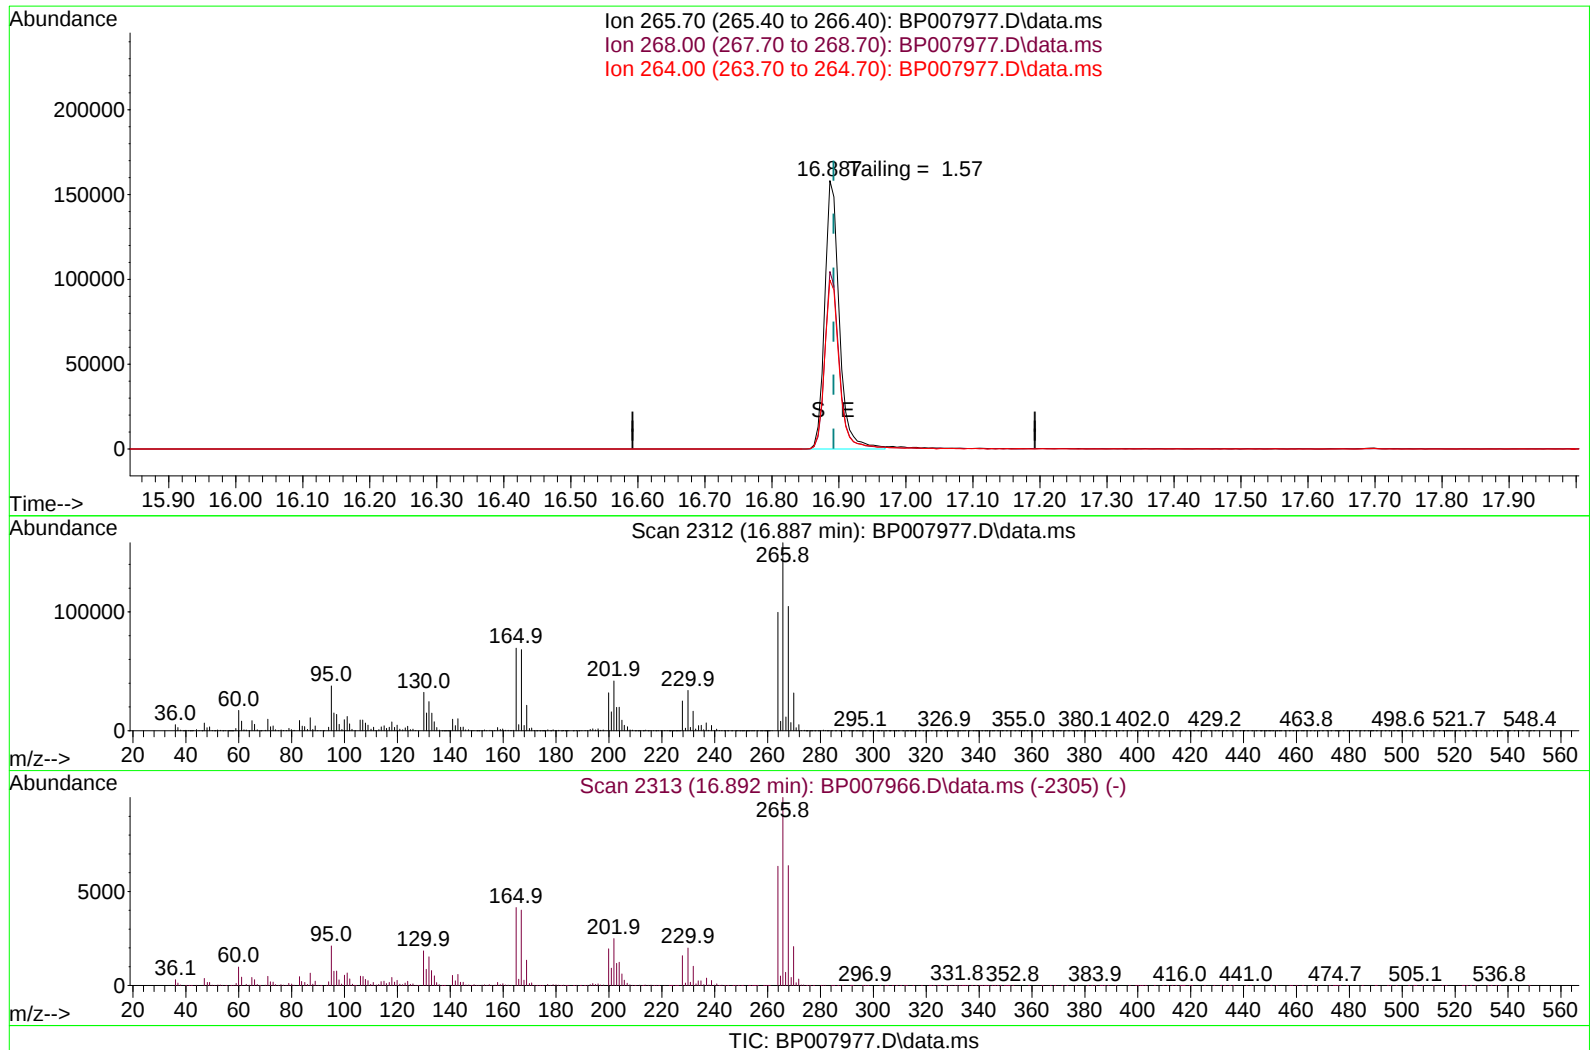

TIC: BP007977.D\data.ms

(70) Pentachlorophenol (C)

16.887min (-0.006) 2149349.59 ng




response 241702

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.60	66.11
264.00	60.90	62.98
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111521\
Data File : BP007977.D
Acq On : 15 Nov 2021 09:41
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Nov 15 12:21:52 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 15 12:21:36 2021
Response via : Initial Calibration

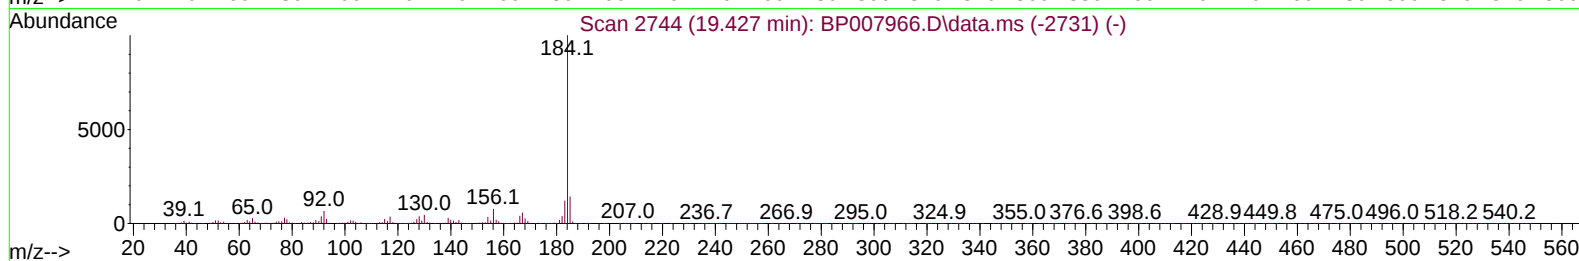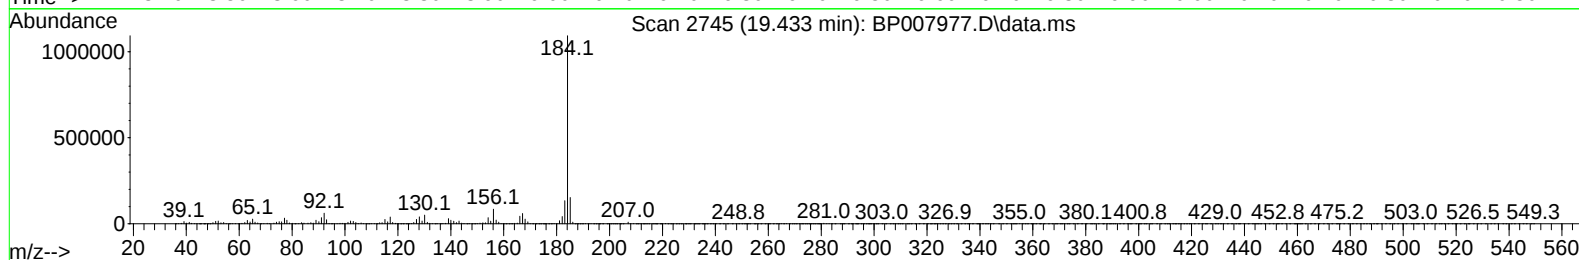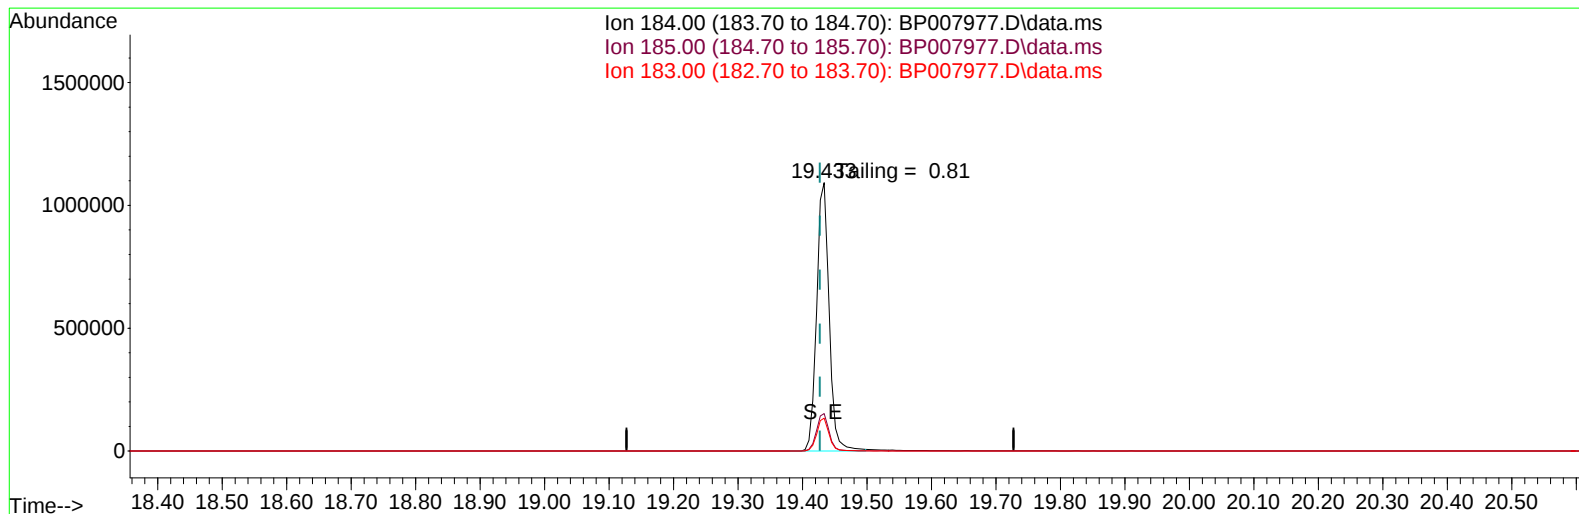

TIC: BP007977.D\data.ms

(77) Benzidine

19.433min (+ 0.006) 672733.55 ng

response 1496686

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	13.98
183.00	11.40	12.25
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/15/2021	BNA_P	BP007977.D
Compound Name	Response	Retention Time
DDT	806639	20.63
DDD	12115	20.21
DDE	2779	19.71
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
14894	821533	1.81

Instrument :
BNA_P
ClientSampleId :
DFTPP