

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111624\
 Data File : BP023167.D
 Acq On : 16 Nov 2024 10:57
 Operator : RC/JU
 Sample : PB164997BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK997

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP023167.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.122	19	23	32	rVB	18130	22479	0.88%	0.106%
2	3.534	89	93	116	rBV	191011	342365	13.44%	1.608%
3	3.834	141	144	151	rVB6	4214	7748	0.30%	0.036%
4	6.687	623	629	632	rBV9	1342	2965	0.12%	0.014%
5	6.758	635	641	661	rVV	203530	434235	17.05%	2.040%
6	6.905	661	666	678	rVV	185752	314299	12.34%	1.476%
7	7.099	692	699	712	rBV	259158	439514	17.25%	2.064%
8	7.552	769	776	793	rBV	175653	331580	13.02%	1.557%
9	8.269	891	898	925	rBV	236424	581225	22.82%	2.730%
10	8.710	965	973	986	rBV	266305	463612	18.20%	2.178%
11	8.840	990	995	1002	rBV	18785	35078	1.38%	0.165%
12	9.422	1087	1094	1108	rBV	218971	412172	16.18%	1.936%
13	9.957	1178	1185	1202	rBV	251715	605900	23.79%	2.846%
14	10.310	1238	1245	1257	rVB	283219	461380	18.11%	2.167%
15	10.469	1265	1272	1292	rBV	208829	569767	22.37%	2.676%
16	11.946	1517	1523	1526	rBV3	3172	6950	0.27%	0.033%
17	13.610	1796	1806	1819	rBV	735198	1144962	44.95%	5.378%
18	13.875	1842	1851	1868	rBV2	691501	1209847	47.50%	5.682%
19	14.187	1894	1904	1916	rBV	411872	751607	29.51%	3.530%
20	14.469	1945	1952	1956	rBV	121225	236795	9.30%	1.112%
21	14.610	1973	1976	1981	rVB6	7349	12110	0.48%	0.057%
22	15.198	2070	2076	2090	rBV	1168714	1651849	64.85%	7.758%
23	15.369	2098	2105	2118	rBV	242915	500665	19.65%	2.352%
24	15.457	2118	2120	2127	rVB4	9233	14095	0.55%	0.066%
25	15.581	2139	2141	2150	rVB10	2647	5082	0.20%	0.024%
26	15.739	2162	2168	2170	rBV7	1366	2660	0.10%	0.012%
27	16.010	2211	2214	2221	rVB9	2494	3836	0.15%	0.018%
28	16.663	2323	2325	2333	rVB8	2124	3228	0.13%	0.015%
29	16.998	2376	2382	2392	rVB	752919	1063452	41.75%	4.995%
30	17.104	2392	2400	2418	rBV	1167975	2002642	78.62%	9.406%
31	17.951	2538	2544	2547	rBV7	6535	12083	0.47%	0.057%
32	18.910	2705	2707	2711	rVB5	3512	3361	0.13%	0.016%
33	19.033	2724	2728	2733	rBV2	18988	27932	1.10%	0.131%
34	19.116	2738	2742	2746	rVV	15758	22762	0.89%	0.107%
35	19.486	2799	2805	2817	rBV	1773298	2473464	97.10%	11.617%
36	21.433	3130	3136	3148	rBV2	796364	1340564	52.63%	6.296%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111624\
Data File : BP023167.D
Acq On : 16 Nov 2024 10:57
Operator : RC/JU
Sample : PB164997BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK997

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Title : SVOA CALIBRATION

37	24.433	3638	3646	3660	rVB	983786	2547279	100.00%	11.964%
38	24.663	3677	3685	3696	rBV	448391	1229345	48.26%	5.774%




Sum of corrected areas: 21290889

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111624\
Data File : BP023167.D
Acq On : 16 Nov 2024 10:57
Operator : RC/JU
Sample : PB164997BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK997

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

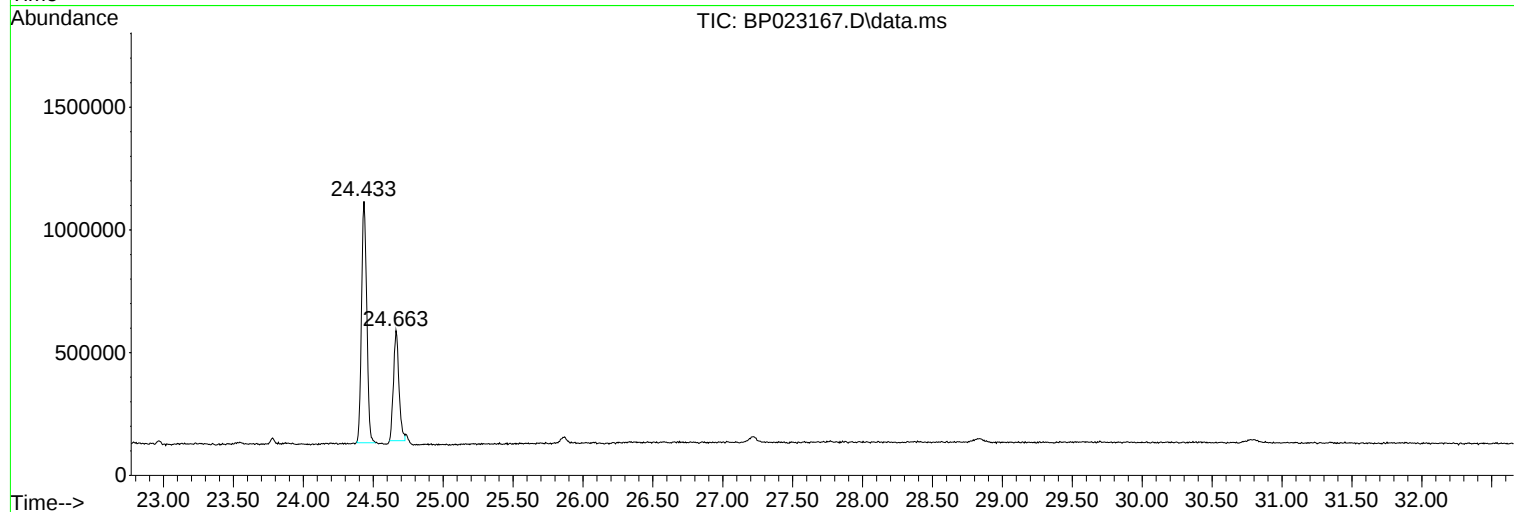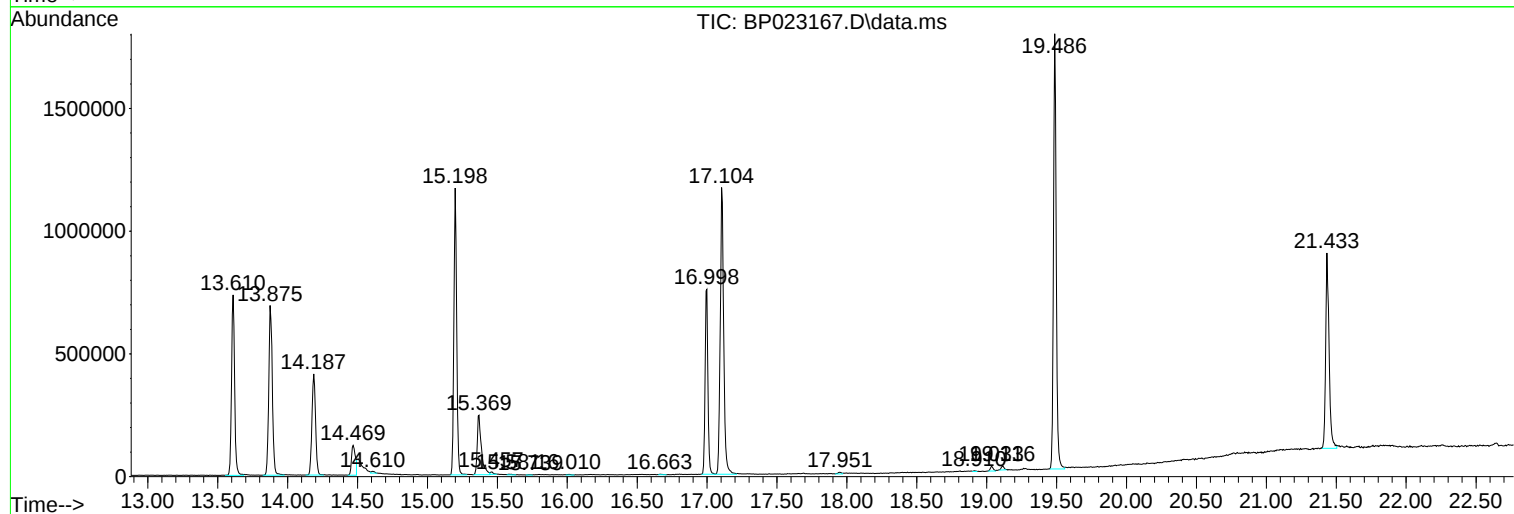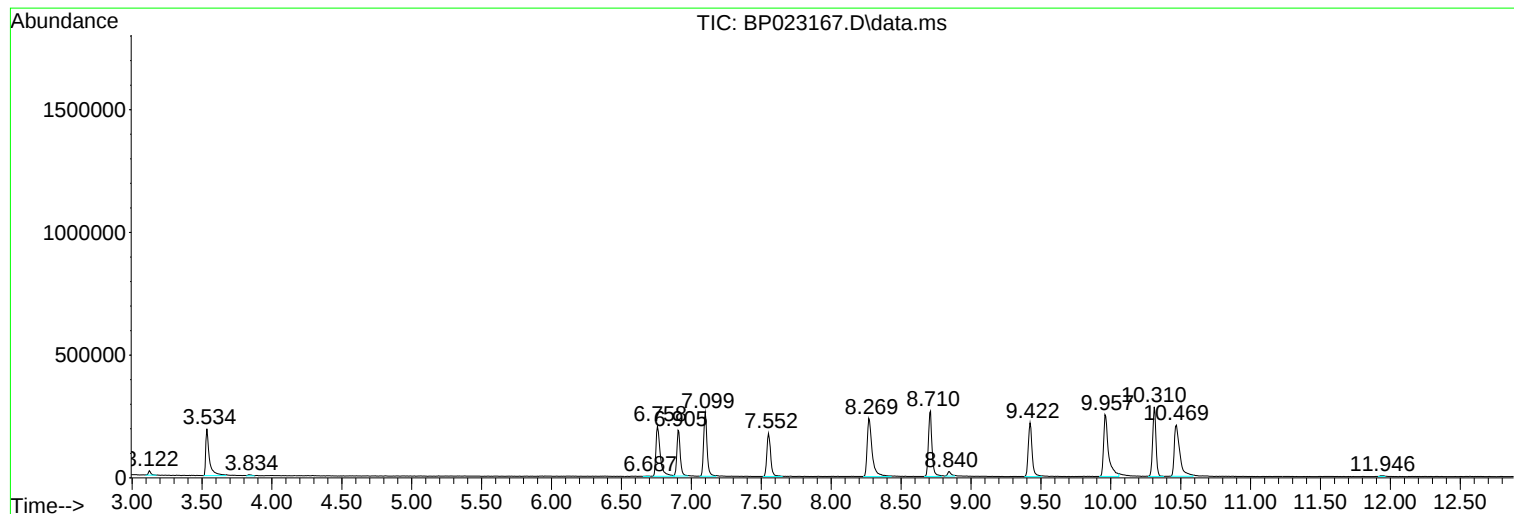

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111624\
Data File : BP023167.D
Acq On : 16 Nov 2024 10:57
Operator : RC/JU
Sample : PB164997BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK997

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111624\
Data File : BP023167.D
Acq On : 16 Nov 2024 10:57
Operator : RC/JU
Sample : PB164997BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK997

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc