

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111624\
 Data File : BP023183.D
 Acq On : 16 Nov 2024 22:28
 Operator : RC/JU
 Sample : PB164821BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK821

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP023183.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.134	20	25	33	rBV	15798	22704	1.10%	0.122%
2	3.546	91	95	112	rBV	168723	306123	14.84%	1.652%
3	3.852	143	147	151	rVB3	3294	3839	0.19%	0.021%
4	4.028	175	177	182	rVB6	1496	2344	0.11%	0.013%
5	6.781	638	645	663	rBV	196598	399212	19.35%	2.154%
6	6.922	663	669	680	rVB	168579	272506	13.21%	1.470%
7	7.122	696	703	718	rBV	225429	392729	19.03%	2.119%
8	7.575	772	780	791	rBV	197483	344874	16.71%	1.861%
9	8.287	895	901	920	rBV	252764	508139	24.63%	2.742%
10	8.716	967	974	991	rBV	231677	410994	19.92%	2.217%
11	9.434	1088	1096	1111	rBV	179789	361165	17.50%	1.949%
12	9.975	1181	1188	1215	rBV	226320	560647	27.17%	3.025%
13	10.322	1240	1247	1258	rVB	269508	462929	22.44%	2.498%
14	10.475	1264	1273	1294	rBV	223449	526270	25.51%	2.839%
15	11.957	1519	1525	1531	rBV8	3521	8277	0.40%	0.045%
16	13.593	1796	1803	1820	rBV	528922	919251	44.55%	4.960%
17	13.875	1843	1851	1862	rBV	704681	998323	48.38%	5.386%
18	14.187	1897	1904	1917	rBV	540961	736559	35.70%	3.974%
19	14.481	1946	1954	1978	rBV2	94098	380451	18.44%	2.053%
20	15.210	2070	2078	2089	rBV	893575	1342033	65.04%	7.241%
21	15.357	2097	2103	2116	rBV	203263	368434	17.86%	1.988%
22	15.451	2117	2119	2133	rVB9	8004	16292	0.79%	0.088%
23	16.675	2322	2327	2331	rBV7	1488	2768	0.13%	0.015%
24	16.781	2343	2345	2350	rVB5	2044	2525	0.12%	0.014%
25	16.998	2375	2382	2393	rBV	658887	1027472	49.80%	5.544%
26	17.098	2393	2399	2417	rVB	1121136	1582592	76.70%	8.539%
27	19.022	2722	2726	2732	rBV3	12847	20433	0.99%	0.110%
28	19.116	2738	2742	2746	rVB3	10711	16033	0.78%	0.087%
29	19.486	2798	2805	2818	rBV	1210012	1938017	93.93%	10.456%
30	21.433	3131	3136	3150	rVB	748653	1221024	59.18%	6.588%
31	24.433	3636	3646	3667	rVB	788913	2063293	100.00%	11.132%
32	24.651	3675	3683	3701	rVB	451736	1316373	63.80%	7.102%




Sum of corrected areas: 18534625

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111624\
Data File : BP023183.D
Acq On : 16 Nov 2024 22:28
Operator : RC/JU
Sample : PB164821BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK821

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

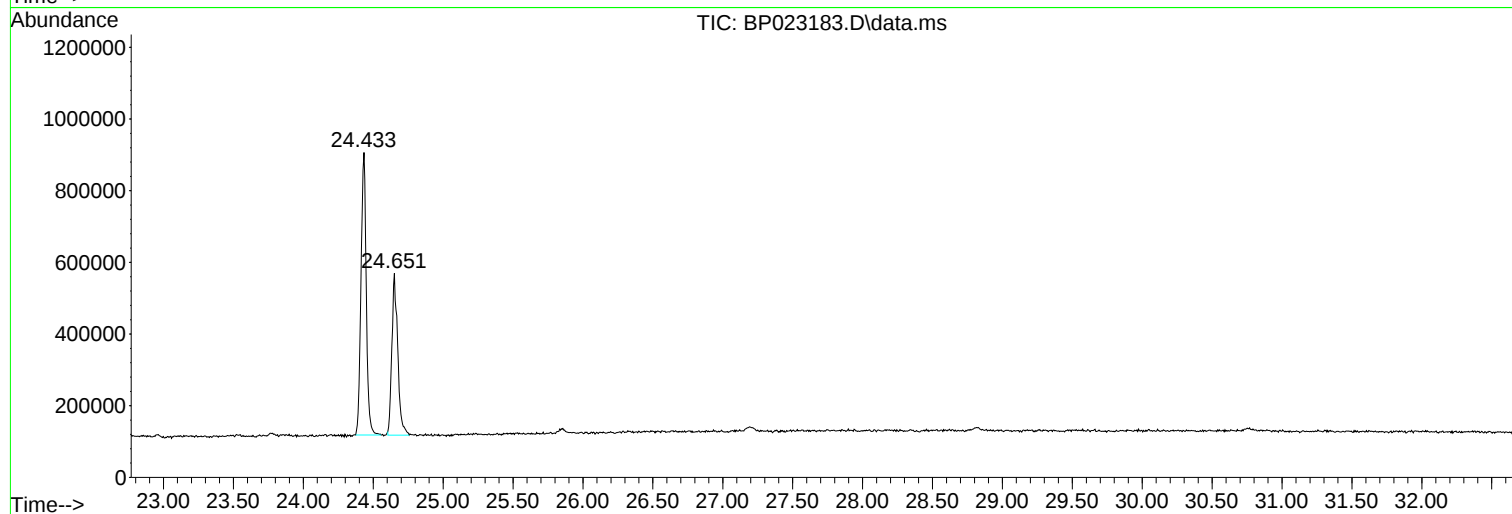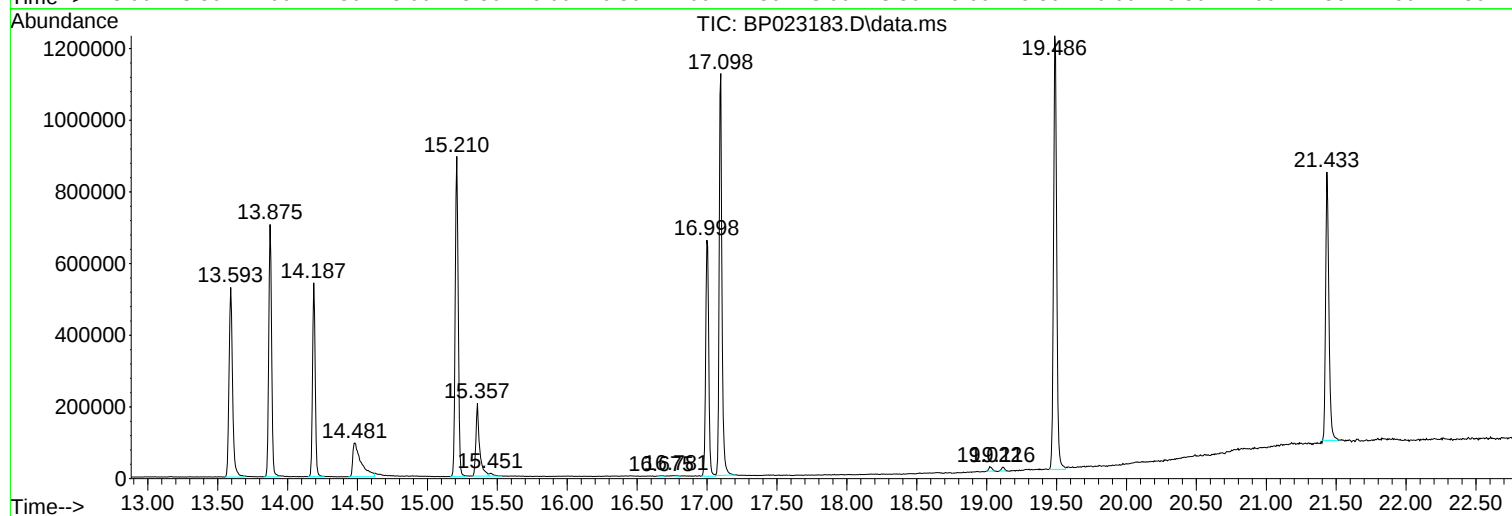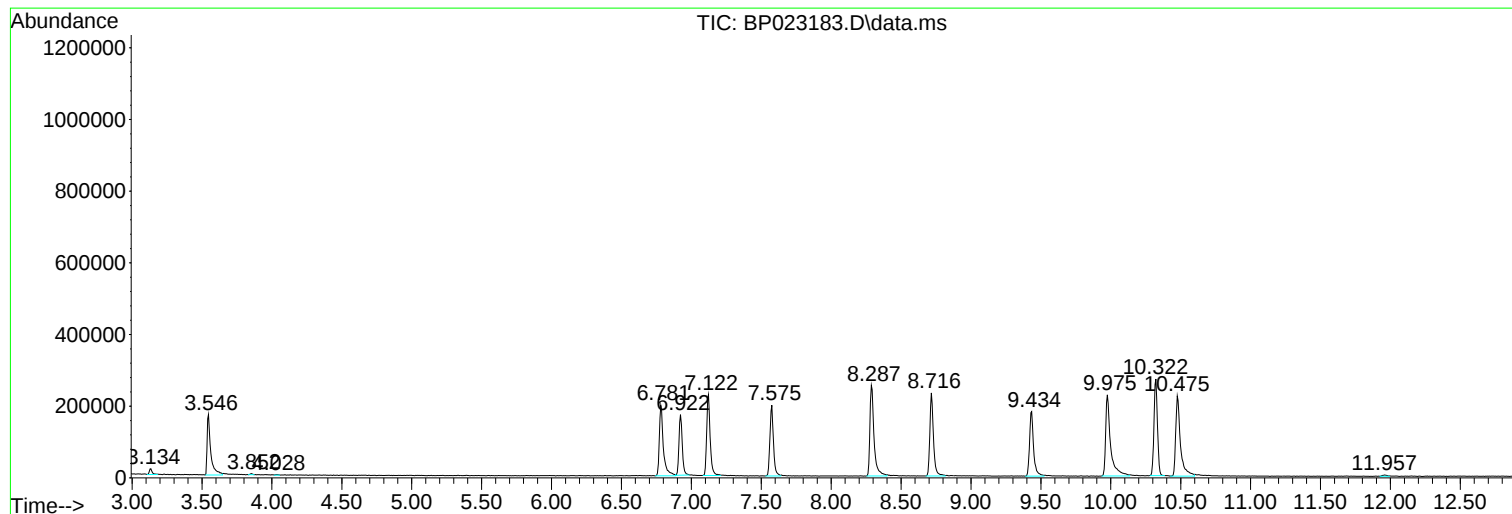

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111624\
Data File : BP023183.D
Acq On : 16 Nov 2024 22:28
Operator : RC/JU
Sample : PB164821BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK821

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111624\
Data File : BP023183.D
Acq On : 16 Nov 2024 22:28
Operator : RC/JU
Sample : PB164821BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK821

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc