
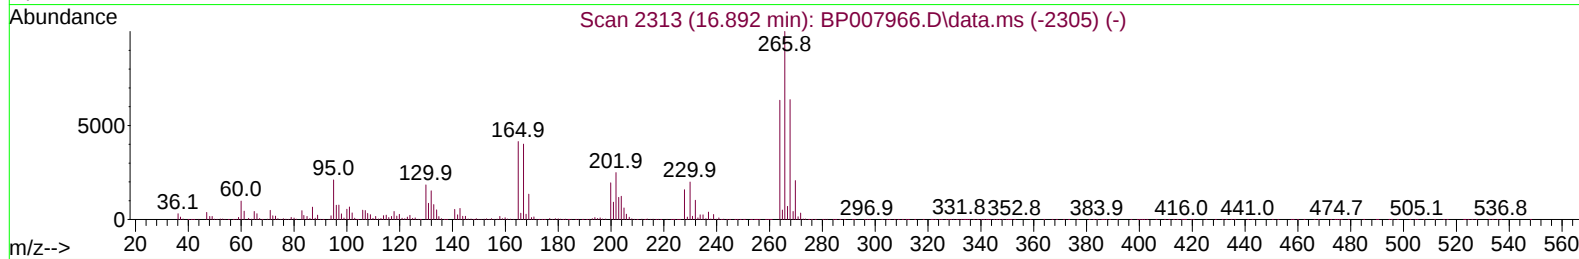
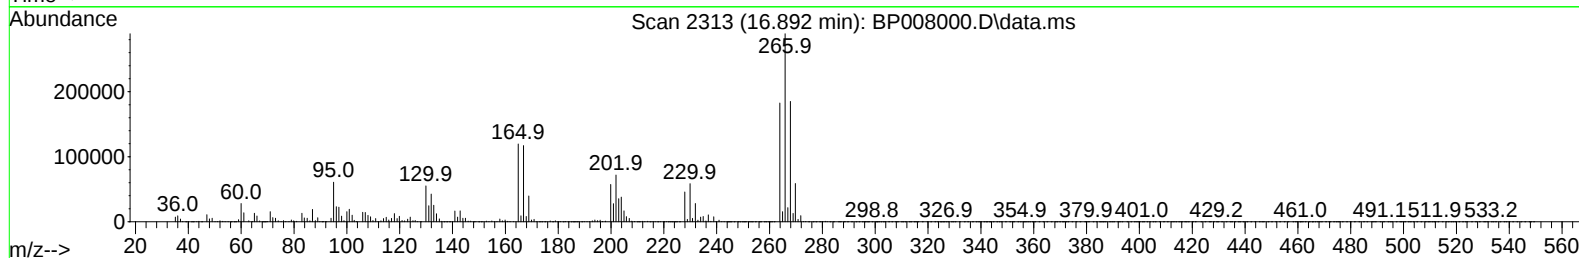


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111721\
Data File : BP008000.D
Acq On : 17 Nov 2021 09:02
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 17 10:36:46 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 15 05:36:49 2021
Response via : Initial Calibration

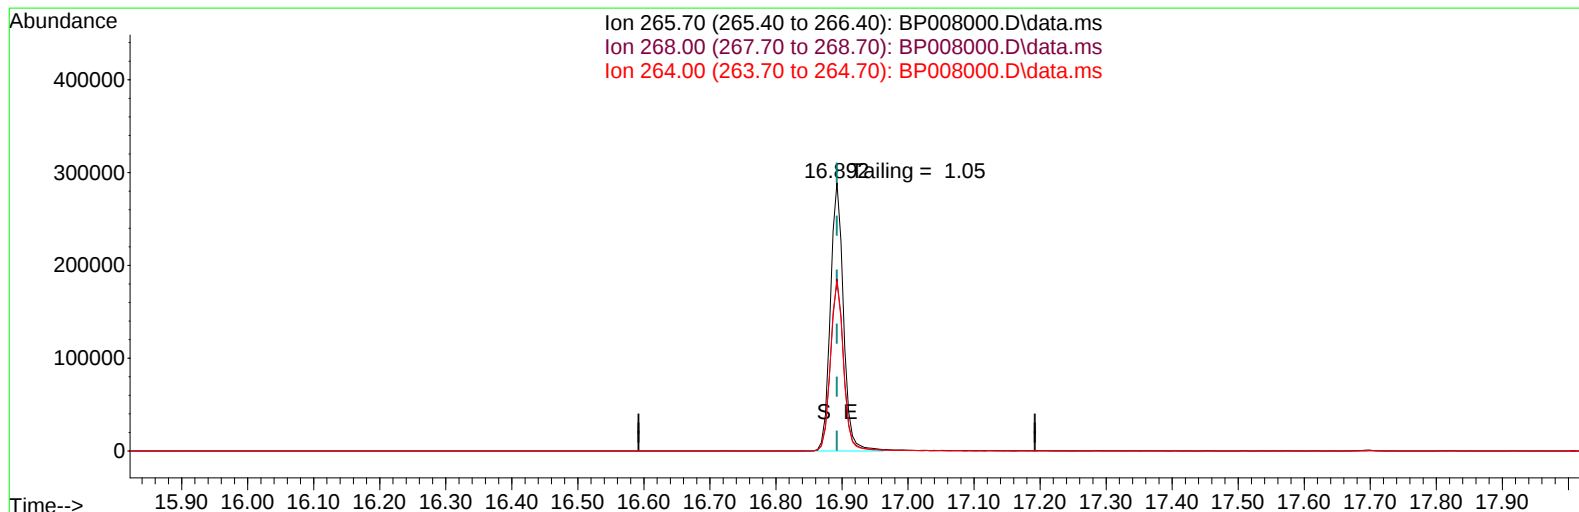

TIC: BP008000.D\data.ms

(70) Pentachlorophenol (C)




16.892min (+ 0.000) 177235.28 ng

response 401462

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.60	64.01
264.00	60.90	63.19
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111721\
Data File : BP008000.D
Acq On : 17 Nov 2021 09:02
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 17 10:36:46 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 15 05:36:49 2021
Response via : Initial Calibration

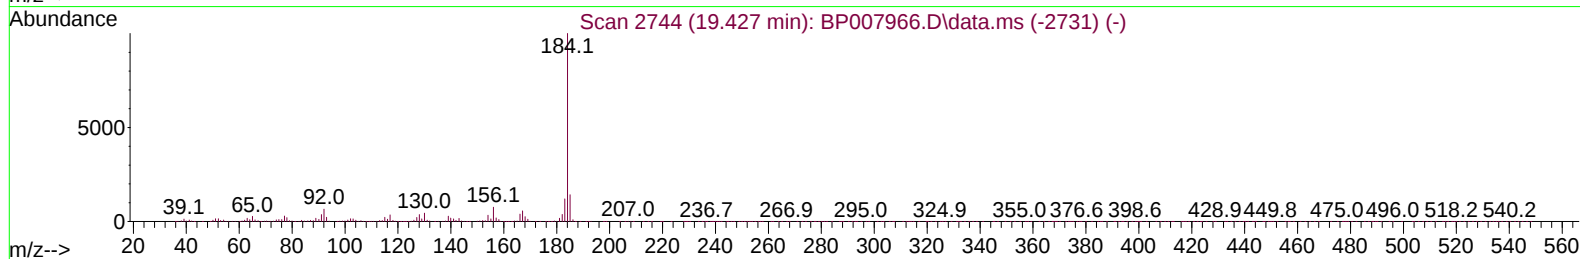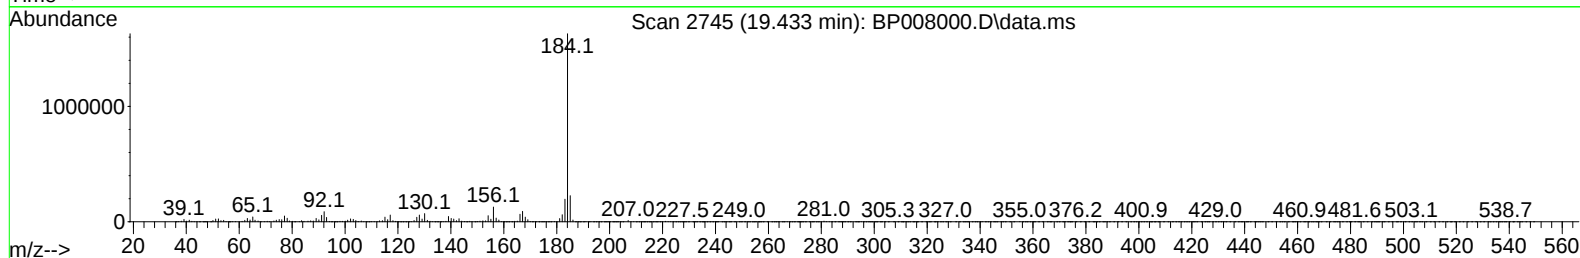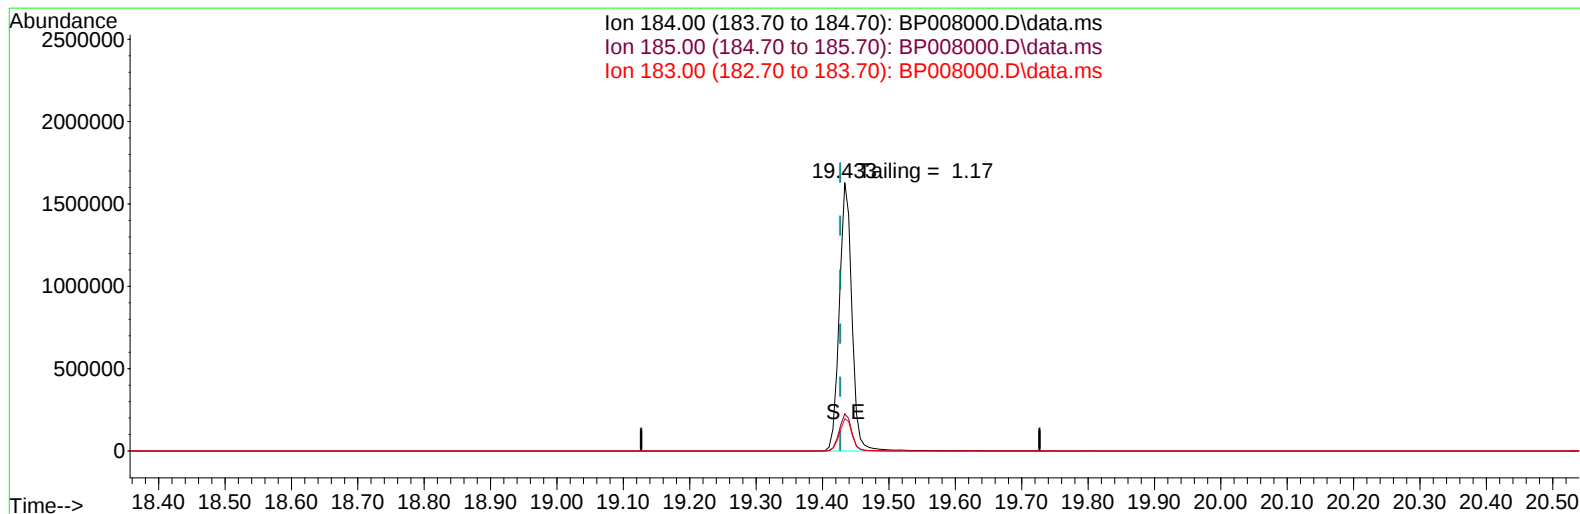

TIC: BP008000.D\data.ms

(77) Benzidine**19.433min (+ 0.006) 14165.69 ng****response 2136974**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	13.91
183.00	11.40	12.03
0.00	0.00	0.00