

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111721\
 Data File : BP008002.D
 Acq On : 17 Nov 2021 10:20
 Operator : CG/JU
 Sample : PB140347BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB140347BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP008002.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.428	357	364	381	rBV	2825693	4191707	39.61%	9.769%
2	7.016	626	634	647	rBV	2448782	3946592	37.29%	9.198%
3	7.840	767	774	784	rBV	485222	766474	7.24%	1.786%
4	8.999	961	971	986	rBV	1493776	2471766	23.36%	5.760%
5	10.640	1241	1250	1267	rBV	609683	1058460	10.00%	2.467%
6	13.104	1660	1669	1685	rBV	4117506	6075758	57.41%	14.160%
7	14.481	1896	1903	1921	rBV	1001384	1489298	14.07%	3.471%
8	15.975	2149	2157	2182	rBV	3622896	5288105	49.97%	12.324%
9	17.234	2365	2371	2384	rBV	1291614	1885375	17.81%	4.394%
10	19.804	2802	2808	2821	rBV	8632103	10583433	100.00%	24.665%
11	21.327	3062	3067	3079	rBV	1875789	2473982	23.38%	5.766%
12	23.733	3469	3476	3487	rVB	1308940	2677956	25.30%	6.241%




Sum of corrected areas: 42908906

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111721\
Data File : BP008002.D
Acq On : 17 Nov 2021 10:20
Operator : CG/JU
Sample : PB140347BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB140347BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

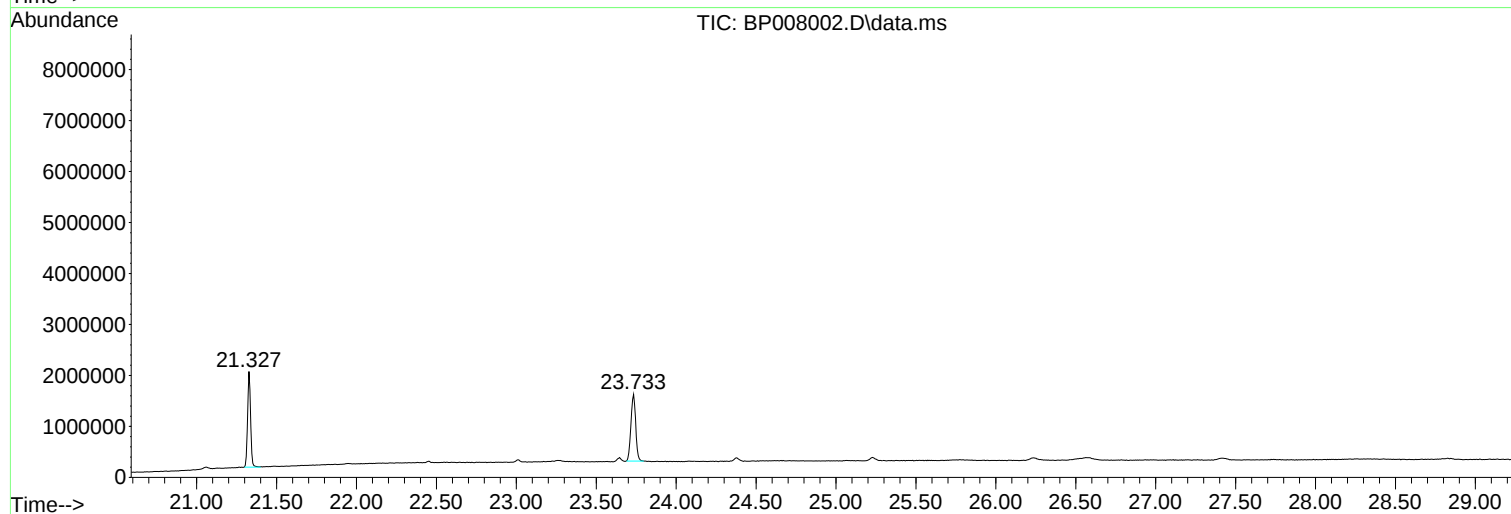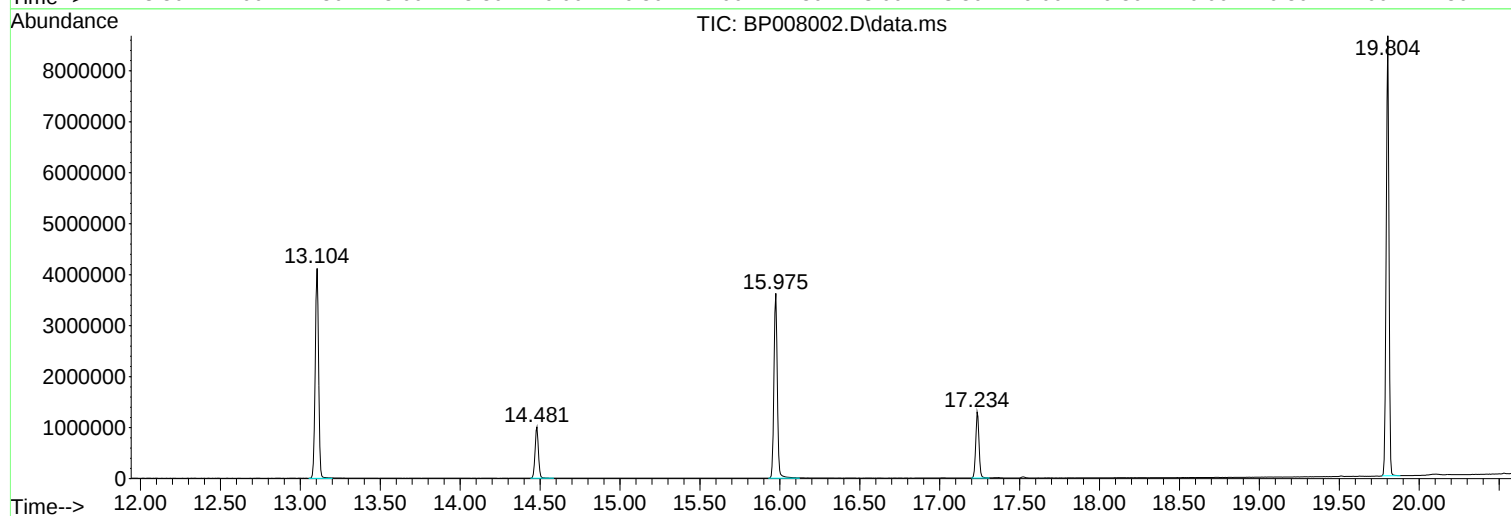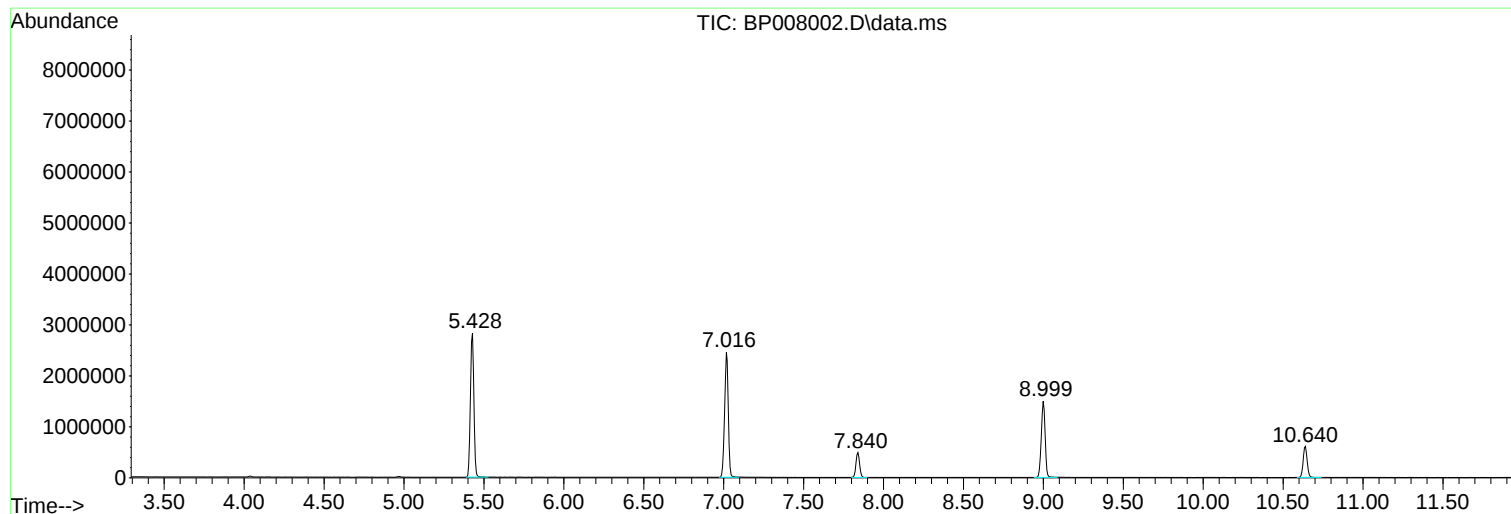

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111721\
Data File : BP008002.D
Acq On : 17 Nov 2021 10:20
Operator : CG/JU
Sample : PB140347BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB140347BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111721\
Data File : BP008002.D
Acq On : 17 Nov 2021 10:20
Operator : CG/JU
Sample : PB140347BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB140347BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------