


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111721\
 Data File : BP008000.D
 Acq On : 17 Nov 2021 09:02
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Nov 15 05:36:49 2021

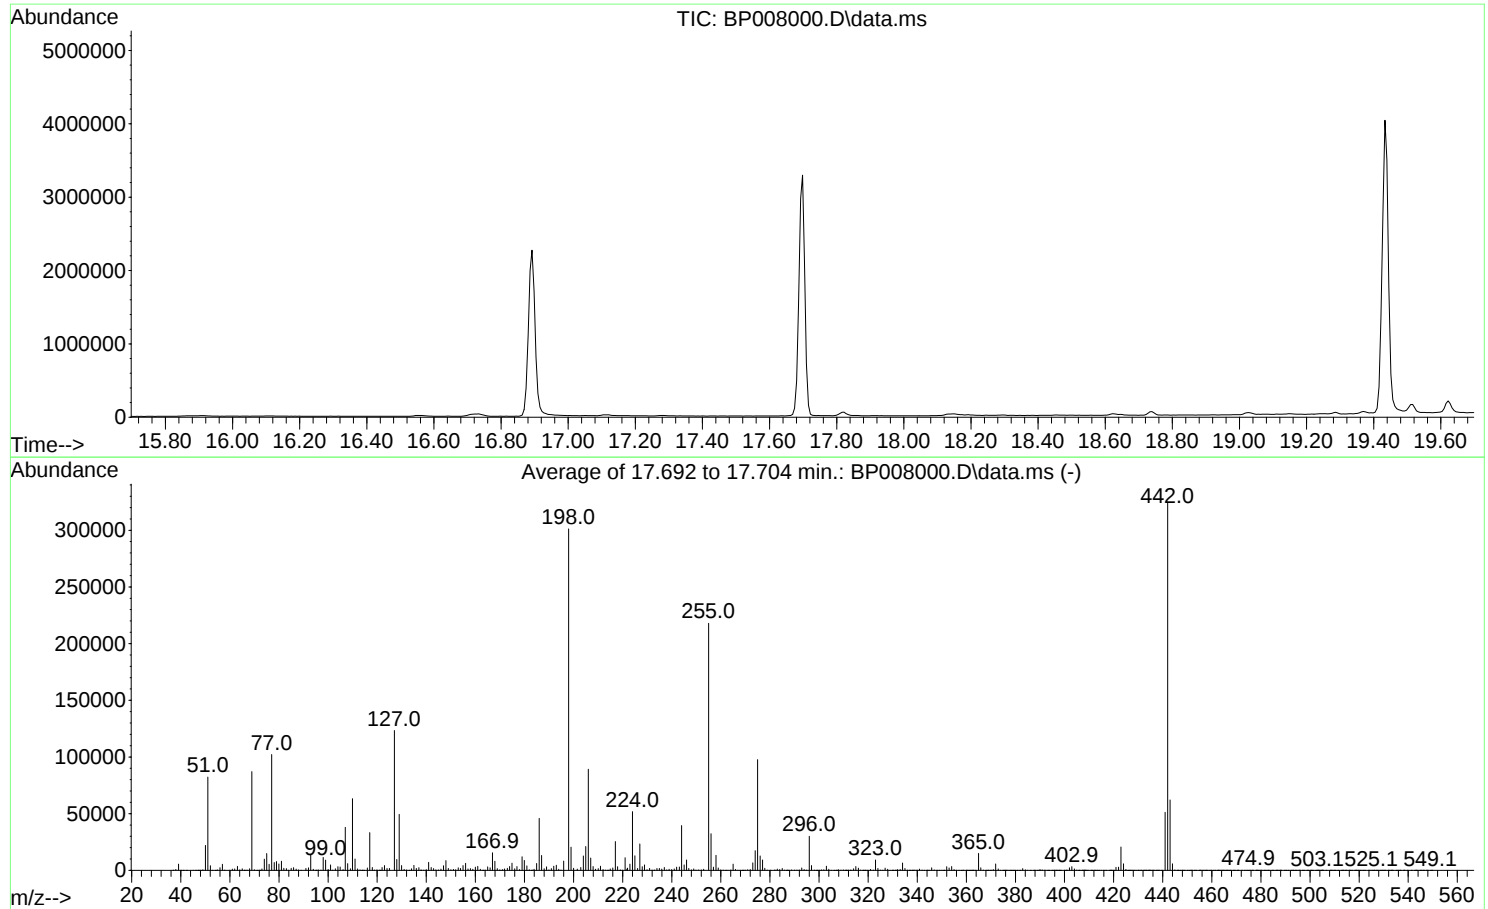

AutoFind: Scans 2449, 2450, 2451; Background Corrected with Scan 2439

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.3	82324	PASS
68	69	0.00	2	1.6	1395	PASS
69	198	0.00	100	28.9	87024	PASS
70	69	0.00	2	0.7	618	PASS
127	198	10	80	41.0	123357	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	301205	PASS
199	198	5	9	6.8	20441	PASS
275	198	10	60	32.4	97690	PASS
365	198	1	100	5.0	14939	PASS
441	198	0.01	100	17.0	51211	PASS
442	442	100	100	100.0	324501	PASS
443	442	15	24	19.1	62094	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
11/17/2021	BNA_P	<u>BP008000.D</u>
Compound Name	Response	Retention Time
DDT	1231348	20.63
DDD	15468	20.21
DDE	2894	19.71
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
18362	1249710	1.47

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111721\
 Data File : BP008000.D
 Acq On : 17 Nov 2021 09:02
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Nov 17 10:36:46 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 15 05:36:49 2021
 Response via : Initial Calibration

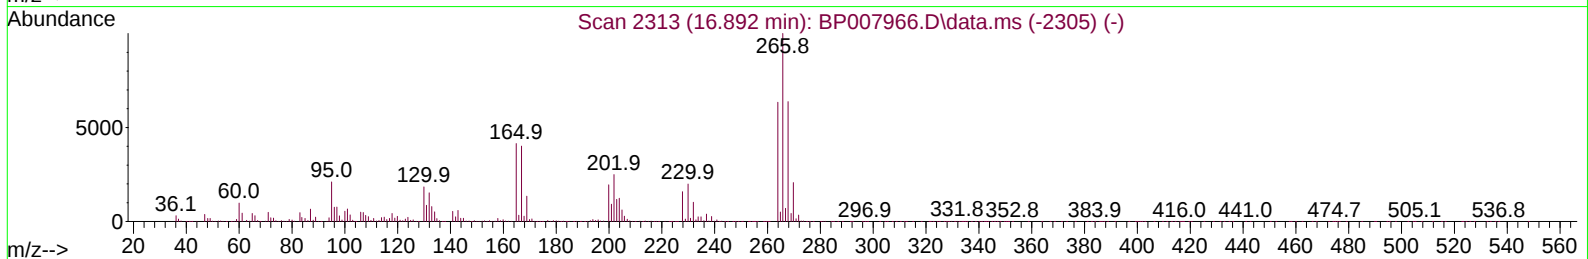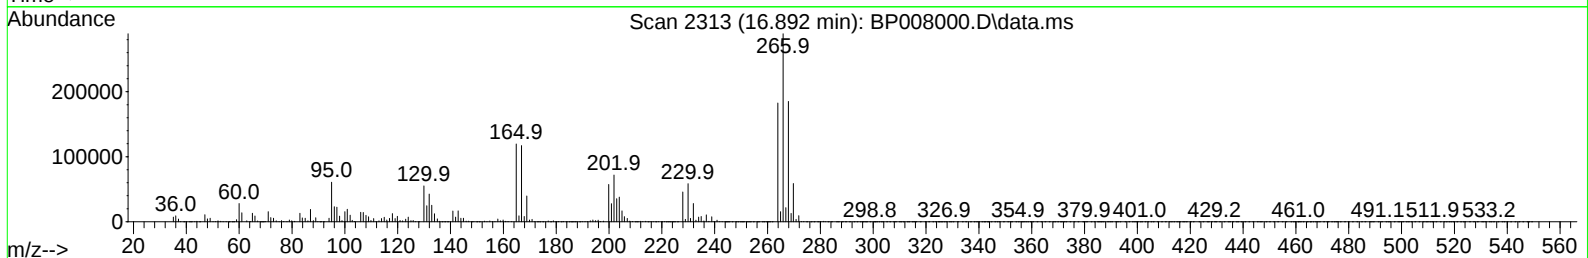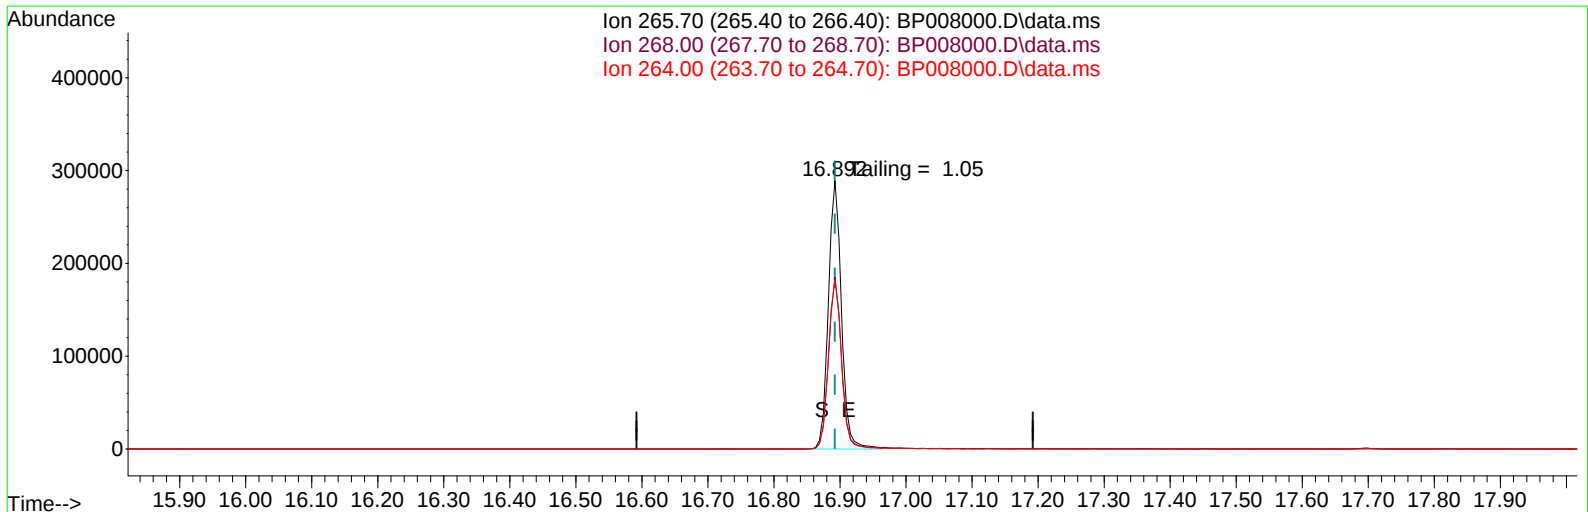

TIC: BP008000.D\data.ms

(70) Pentachlorophenol (C)

16.892min (+ 0.000) 177235.28 ng




response 401462

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.60	64.01
264.00	60.90	63.19
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111721\
Data File : BP008000.D
Acq On : 17 Nov 2021 09:02
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Nov 17 10:36:46 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 15 05:36:49 2021
Response via : Initial Calibration

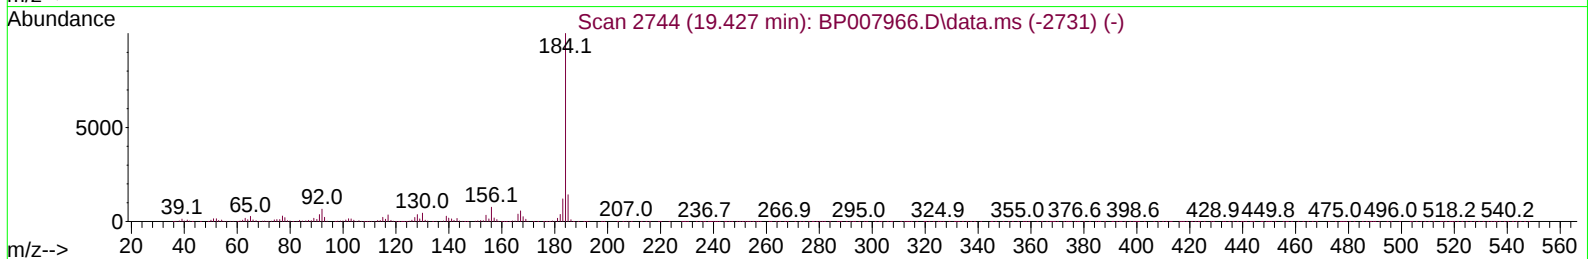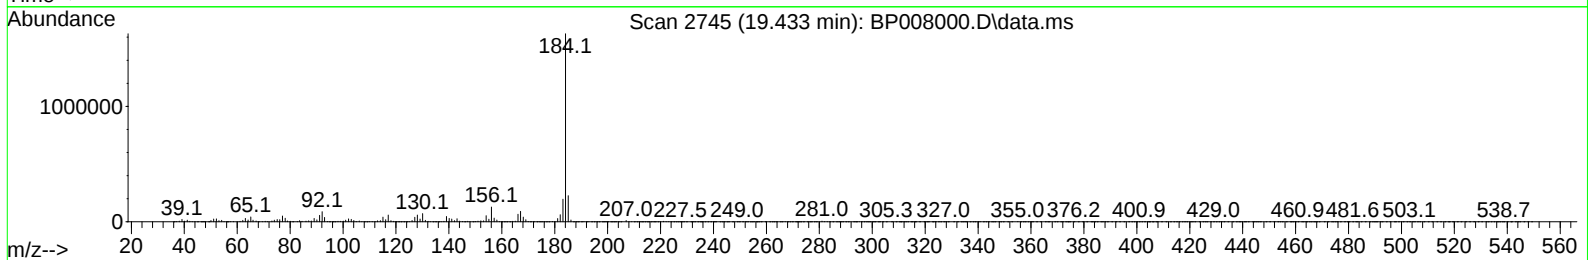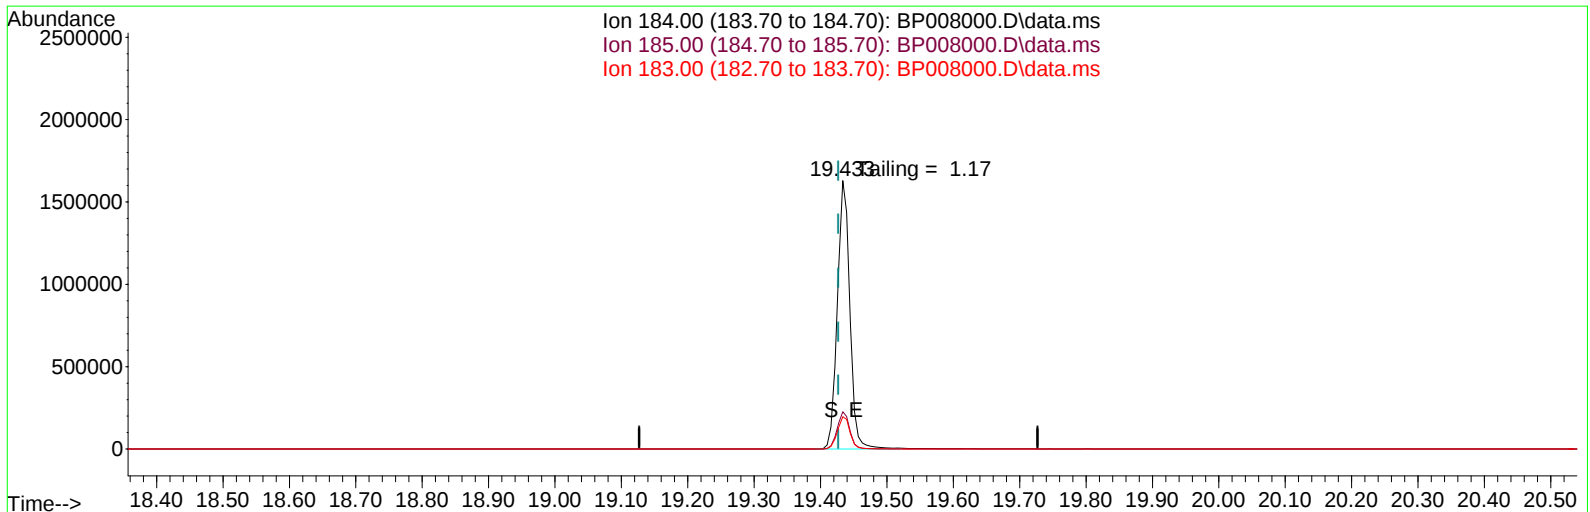

TIC: BP008000.D\data.ms

(77) Benzidine

19.433min (+ 0.006) 14165.69 ng

response 2136974

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	13.91
183.00	11.40	12.03
0.00	0.00	0.00