
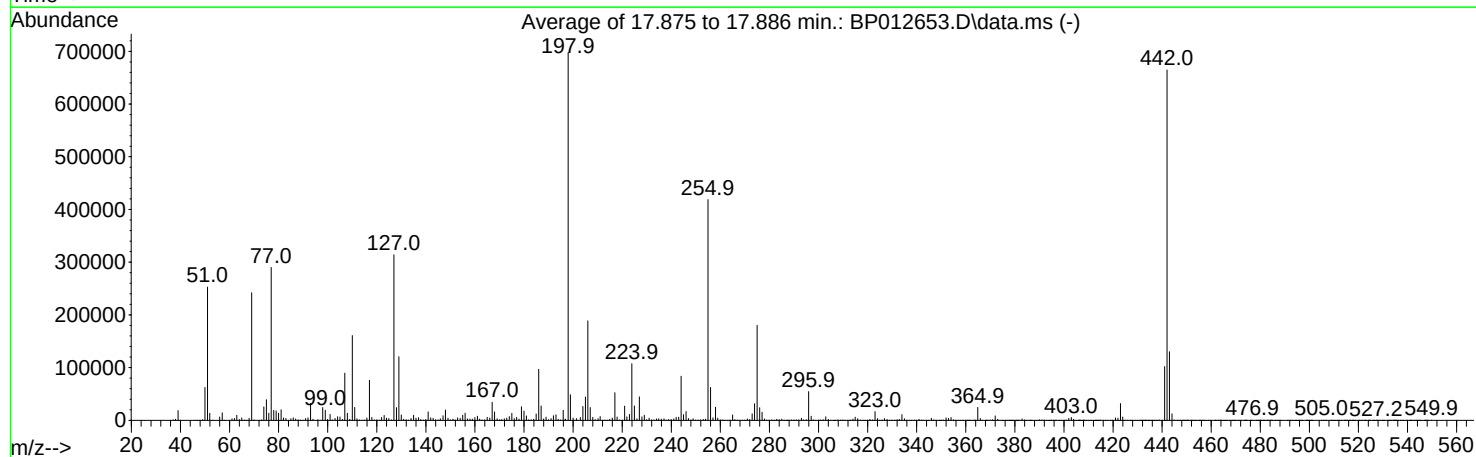


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111722\
 Data File : BP012653.D
 Acq On : 17 Nov 2022 09:22
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Nov 18 00:16:03 2022

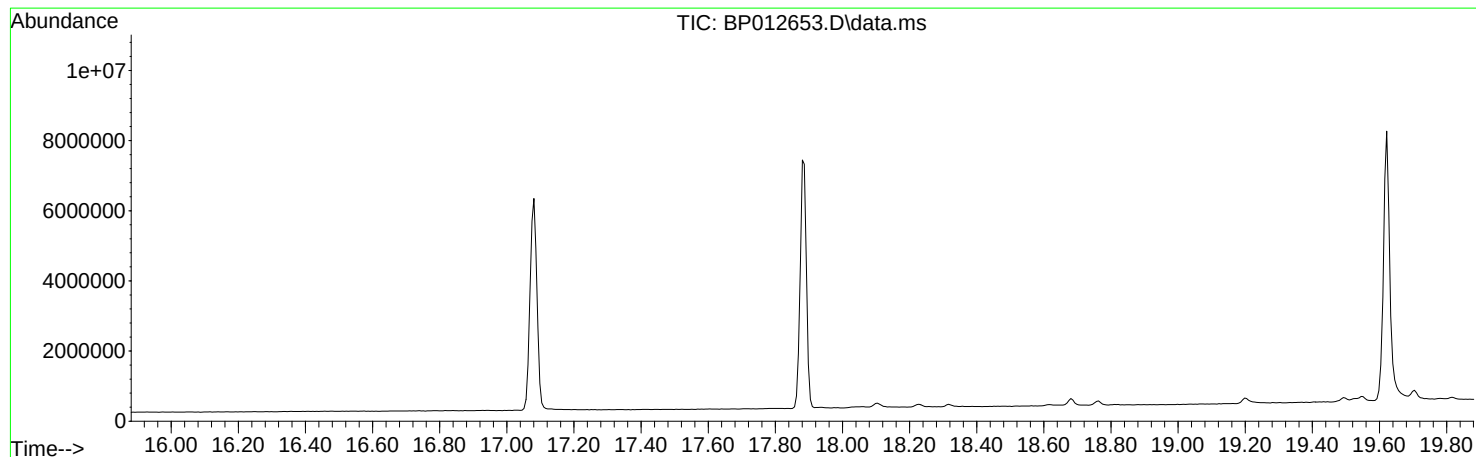




AutoFind: Scans 2531, 2532, 2533; Background Corrected with Scan 2523

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.2	252746	PASS
68	69	0.00	2	1.5	3722	PASS
69	198	0.00	100	34.7	242047	PASS
70	69	0.00	2	0.3	821	PASS
127	198	10	80	45.0	313963	PASS
197	198	0.00	2	0.3	2254	PASS
198	198	100	100	100.0	697944	PASS
199	198	5	9	6.9	48493	PASS
275	198	10	60	25.8	180037	PASS
365	198	1	100	3.5	24561	PASS
441	198	0.01	100	14.6	101949	PASS
442	442	100	100	100.0	664832	PASS
443	442	15	24	19.6	130053	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111722\
 Data File : BP012653.D
 Acq On : 17 Nov 2022 09:22
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Nov 18 05:31:33 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 18 00:16:03 2022
 Response via : Initial Calibration

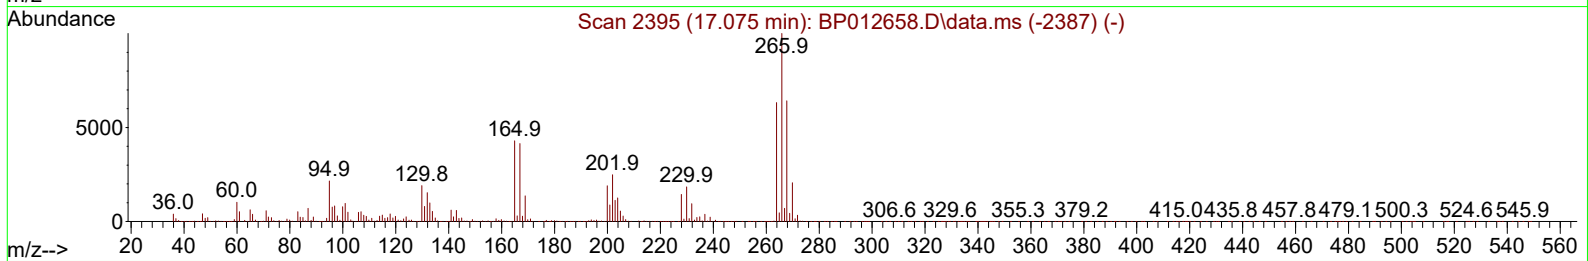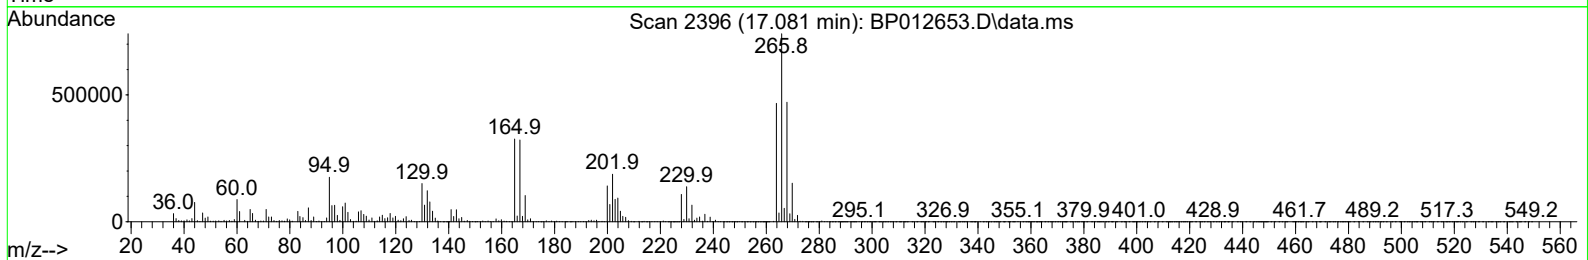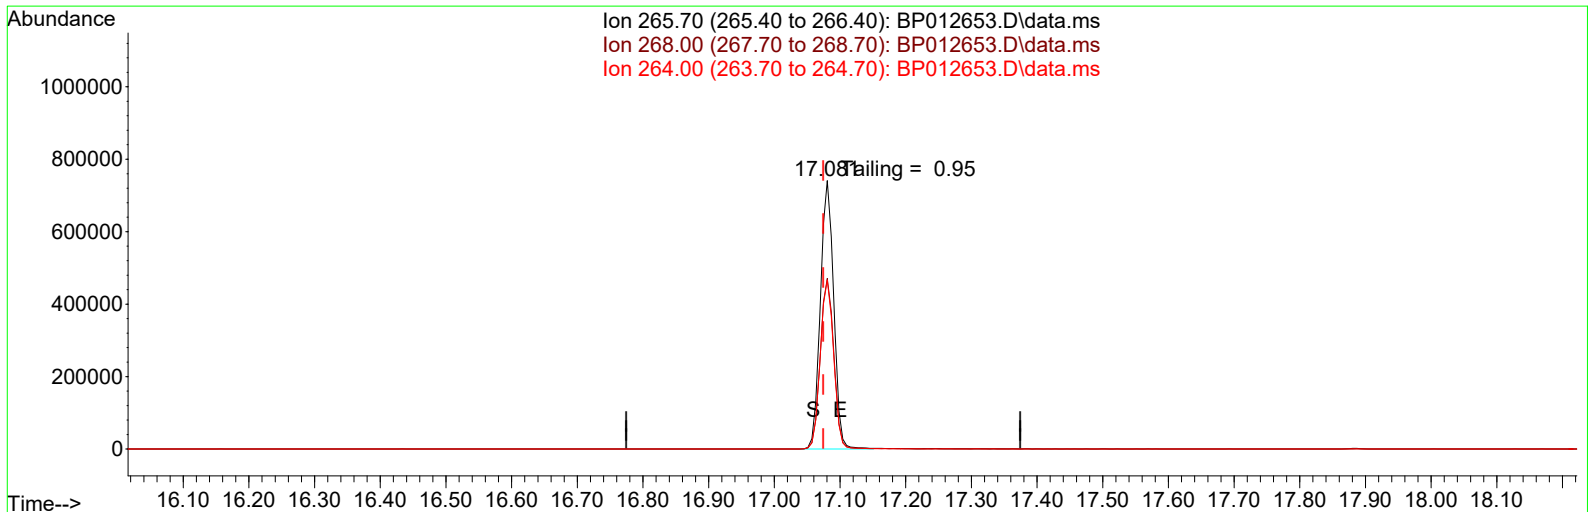

TIC: BP012653.D\data.ms

(70) Pentachlorophenol (C)

17.081min (+ 0.006) 288265.27 ng




response 1045930

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.20	63.59
264.00	63.20	63.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111722\
Data File : BP012653.D
Acq On : 17 Nov 2022 09:22
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Nov 18 05:31:33 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 18 00:16:03 2022
Response via : Initial Calibration

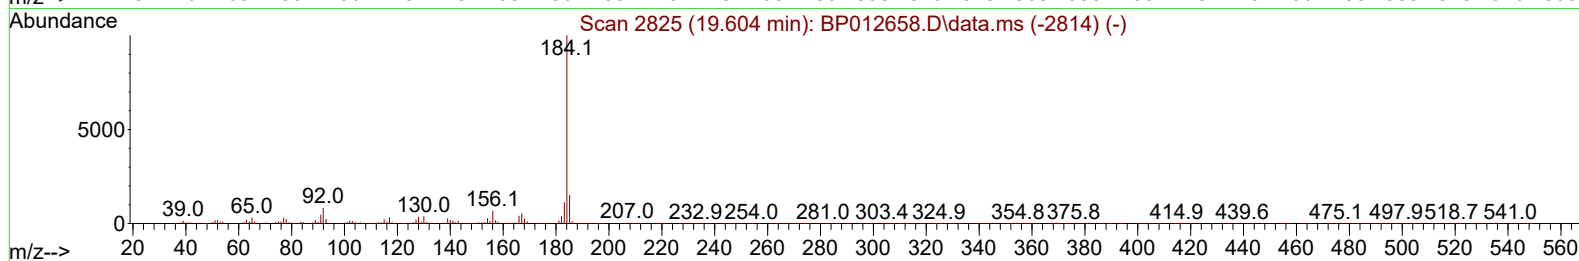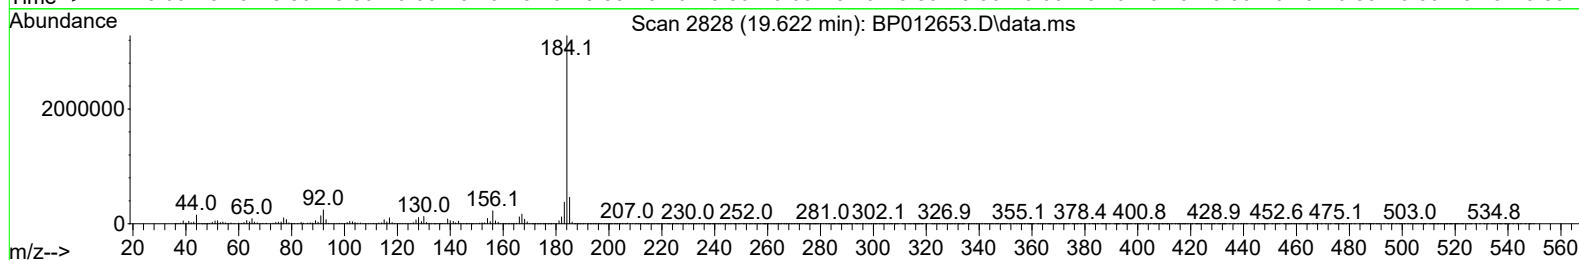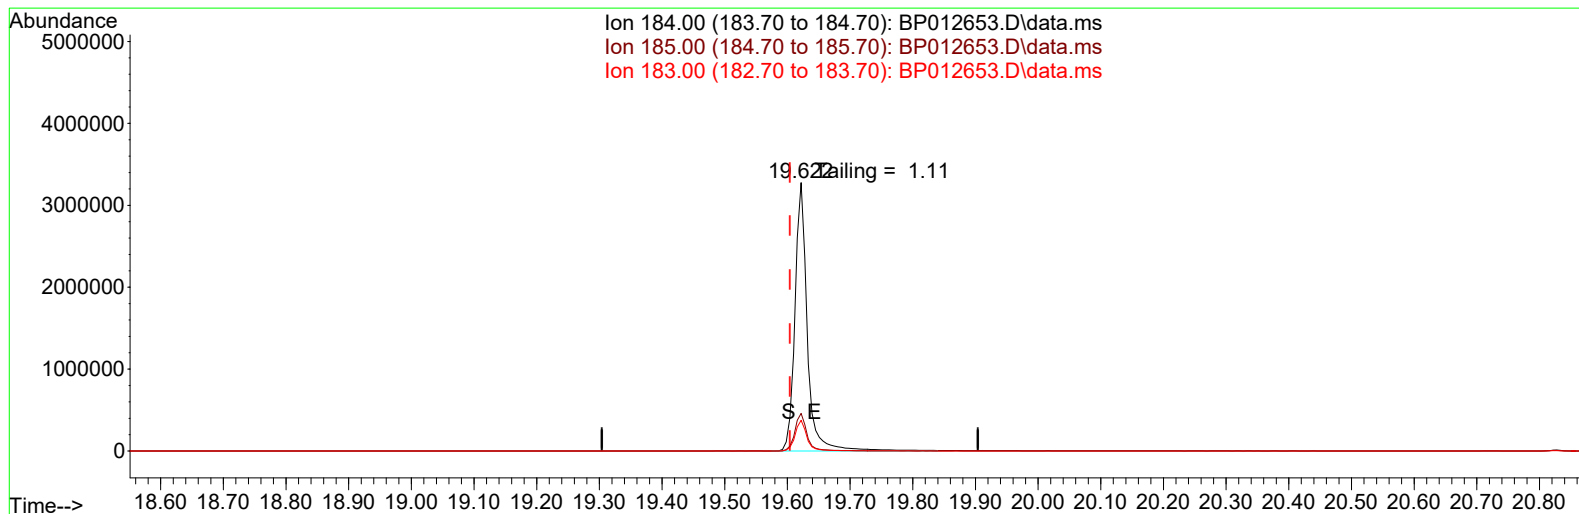

TIC: BP012653.D\data.ms

(77) Benzidine

19.622min (+ 0.018) 1109456.37 ng

response 4517436

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.00
183.00	11.20	11.48
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/17/2022	BNA_P	<u>BP012653.D</u>
Compound Name	Response	Retention Time
DDT	2194551	20.828
DDD	32018	20.392
DDE	853	19.898
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
32871	2227422	1.48

Instrument :
BNA_P
ClientSampleId :
DFTPP