
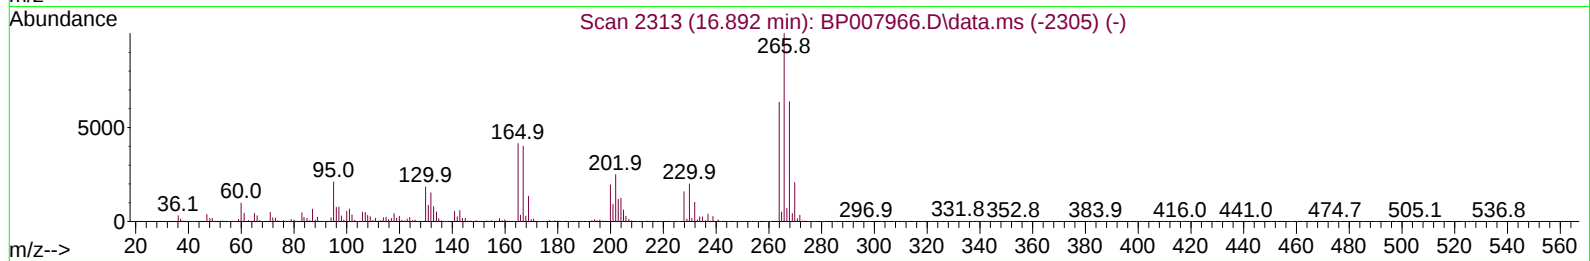
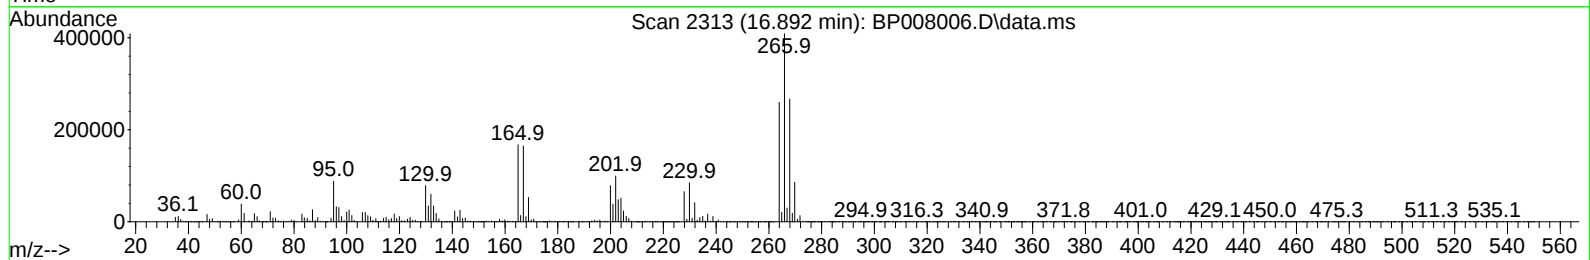


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111821\
Data File : BP008006.D
Acq On : 18 Nov 2021 08:53
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 18 10:02:27 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 15 05:36:49 2021
Response via : Initial Calibration

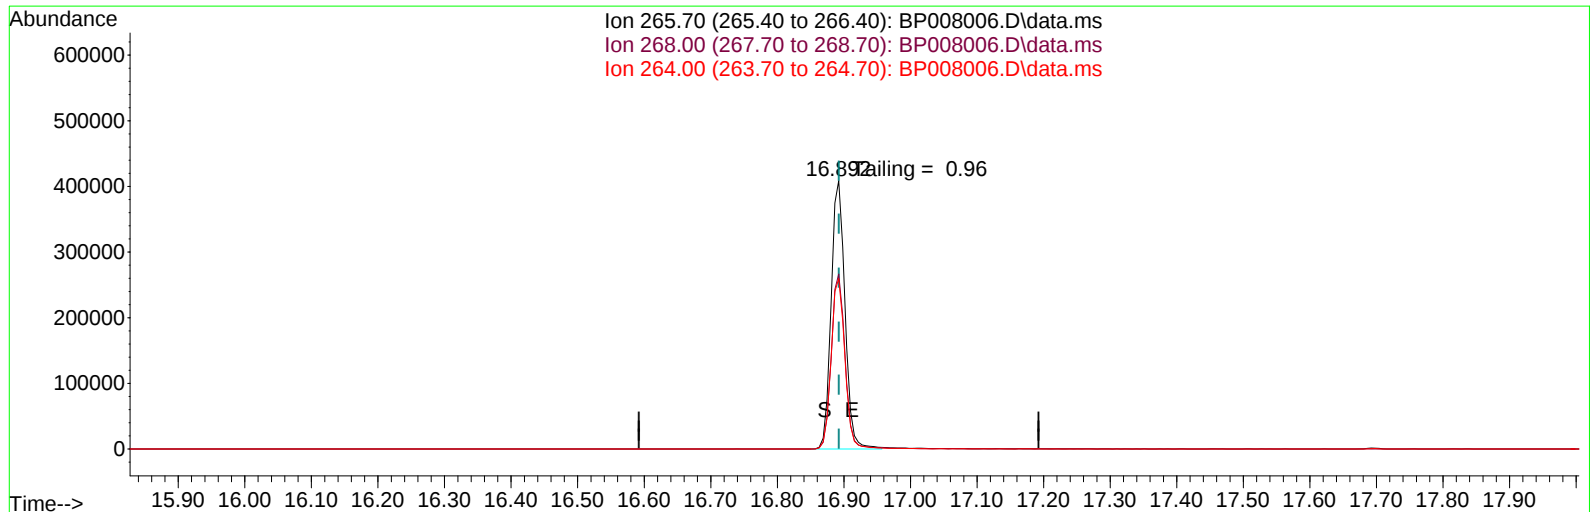

TIC: BP008006.D\data.ms

(70) Pentachlorophenol (C)




16.892min (+ 0.000) 121697.76 ng

response 594335

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.60	65.25
264.00	60.90	63.48
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111821\  
Data File : BP008006.D  
Acq On    : 18 Nov 2021  08:53  
Operator  : CG/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: Nov 18 10:02:27 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 15 05:36:49 2021
Response via : Initial Calibration

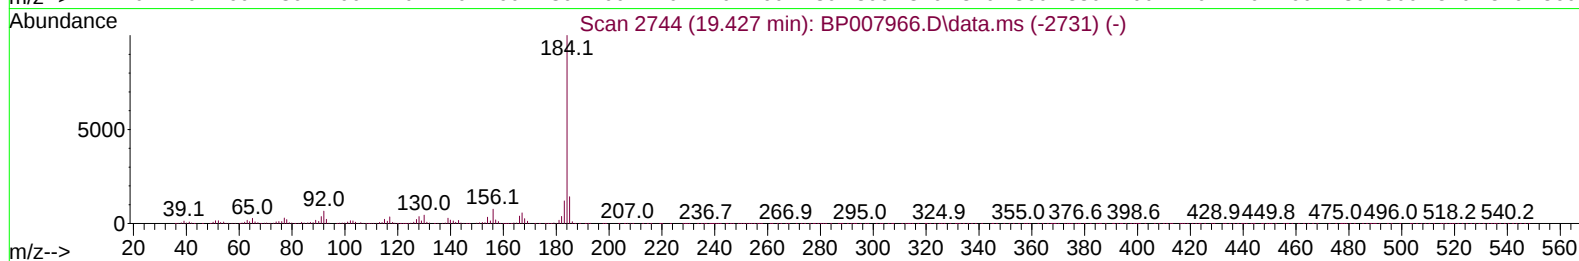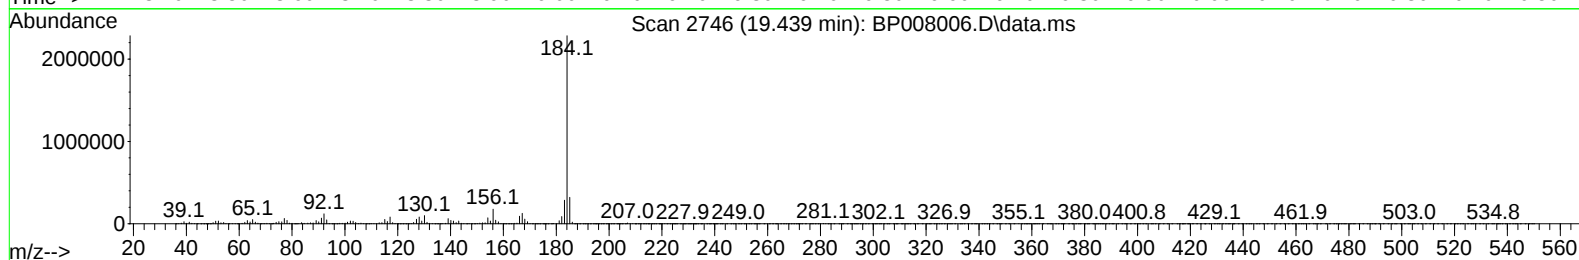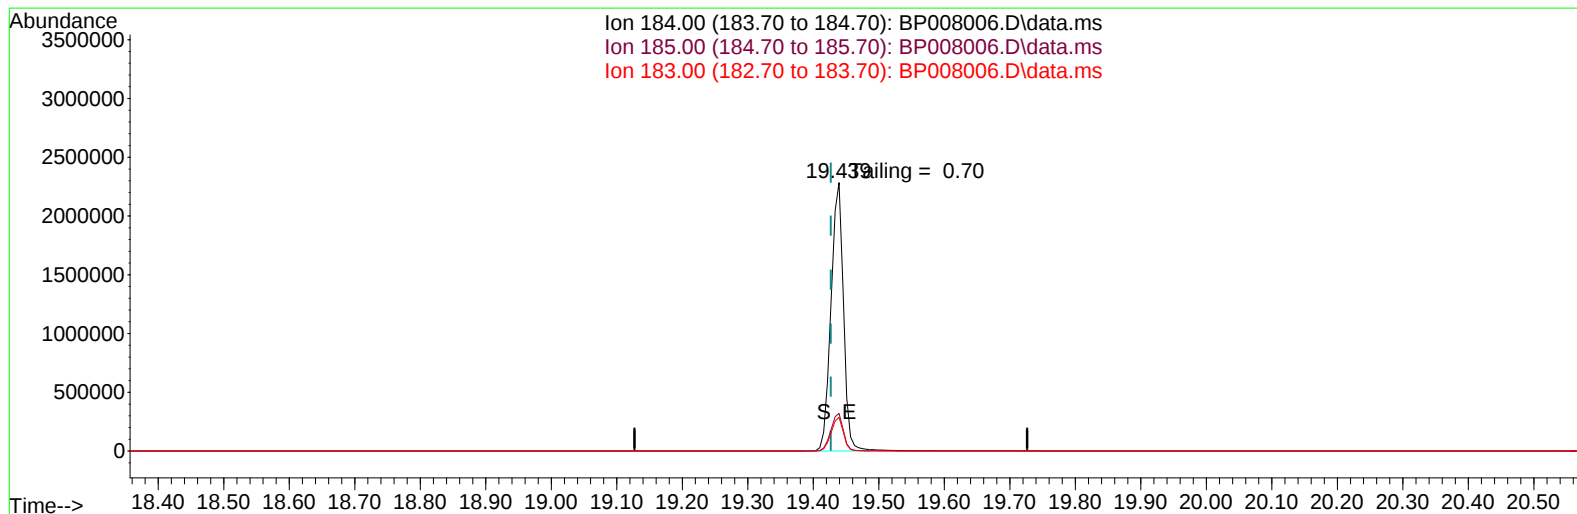

TIC: BP008006.D\data.ms

(77) Benzidine

19.439min (+ 0.012) 22312.33 ng

response 3047217

Ion	Exp%	Act%
-----	------	------

184.00	100.00	100.00
--------	--------	--------

185.00	14.00	14.01
--------	-------	-------

183.00	11.40	12.51
--------	-------	-------

0.00 0.00 0.00