
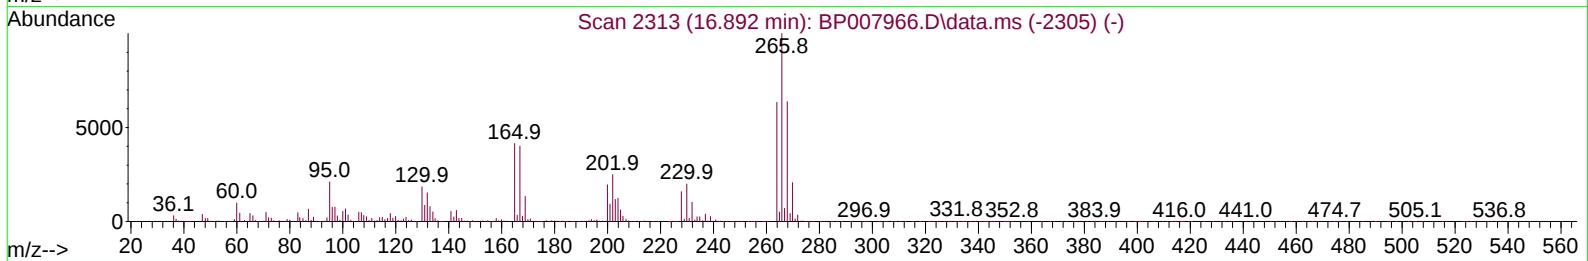
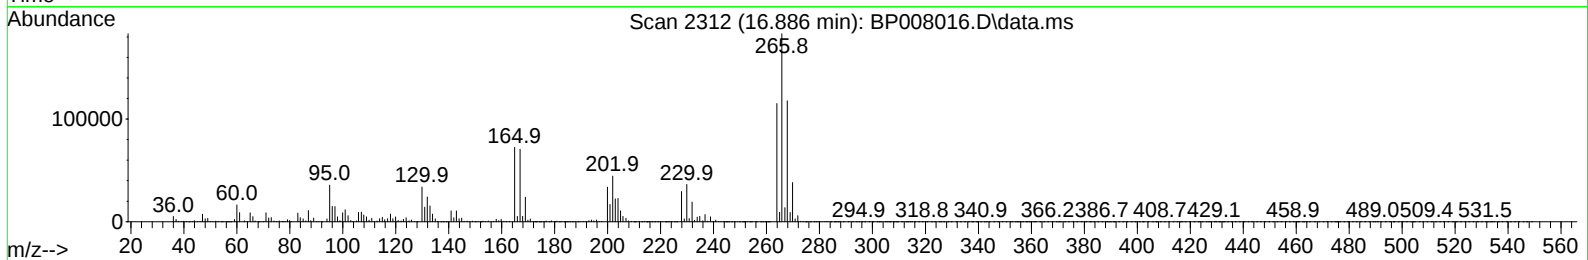


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111821\
Data File : BP008016.D
Acq On : 18 Nov 2021 14:56
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 18 17:11:28 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 15 05:36:49 2021
Response via : Initial Calibration

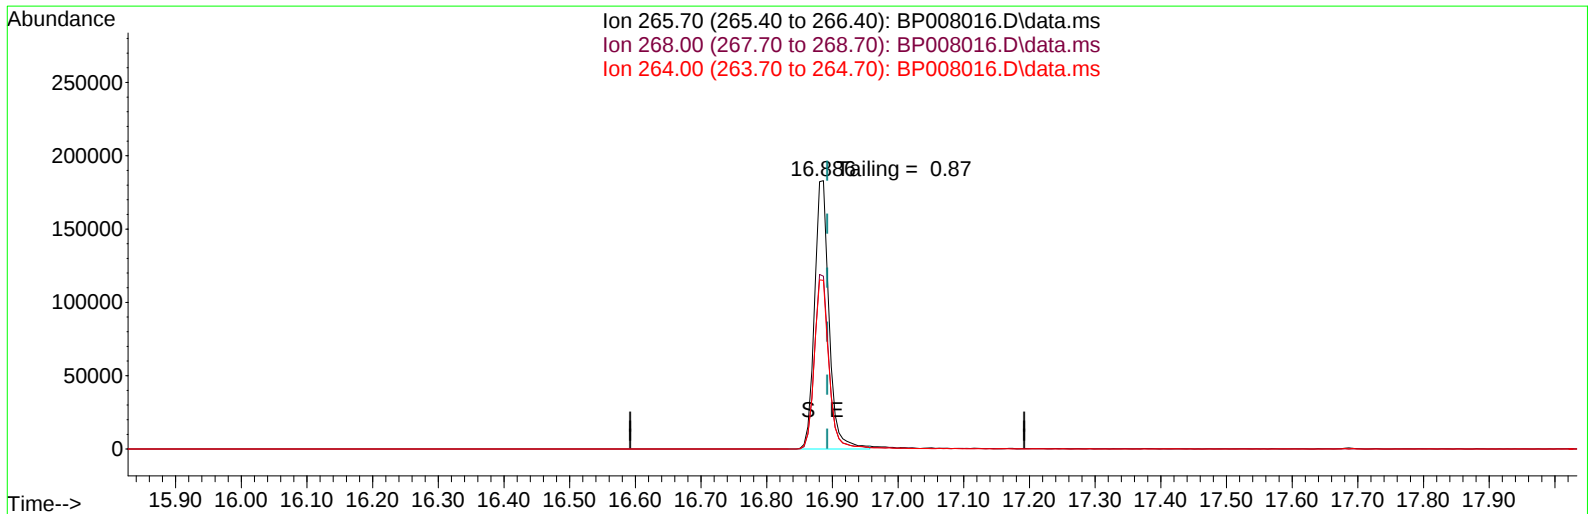

TIC: BP008016.D\data.ms

(70) Pentachlorophenol (C)




16.886min (-0.006) 2965937.09 ng

response 285883

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.60	64.38
264.00	60.90	62.85
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111821\
 Data File : BP008016.D
 Acq On : 18 Nov 2021 14:56
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 18 17:11:28 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 15 05:36:49 2021
 Response via : Initial Calibration

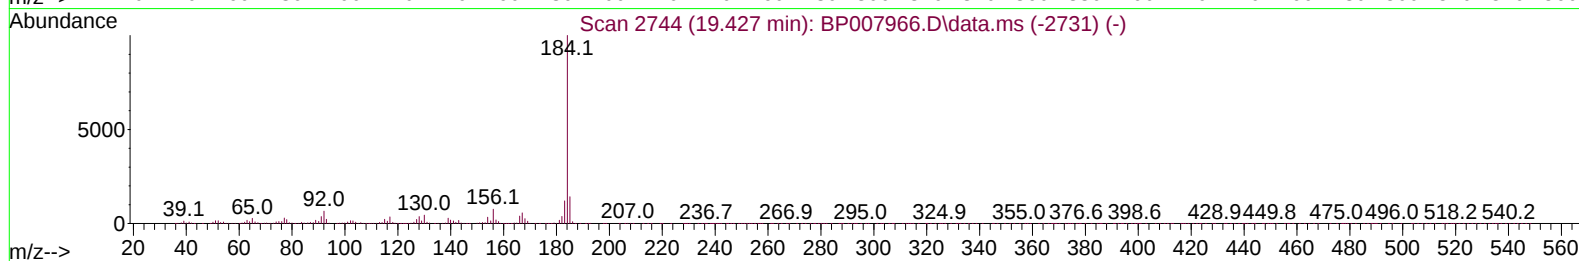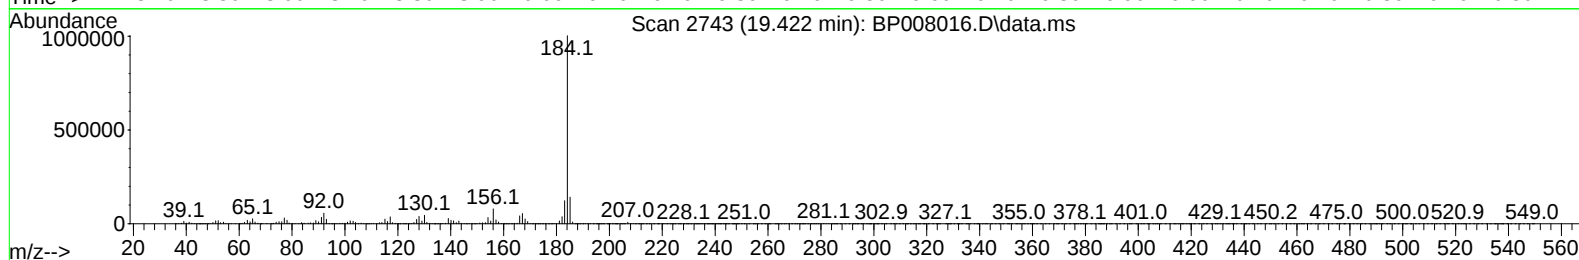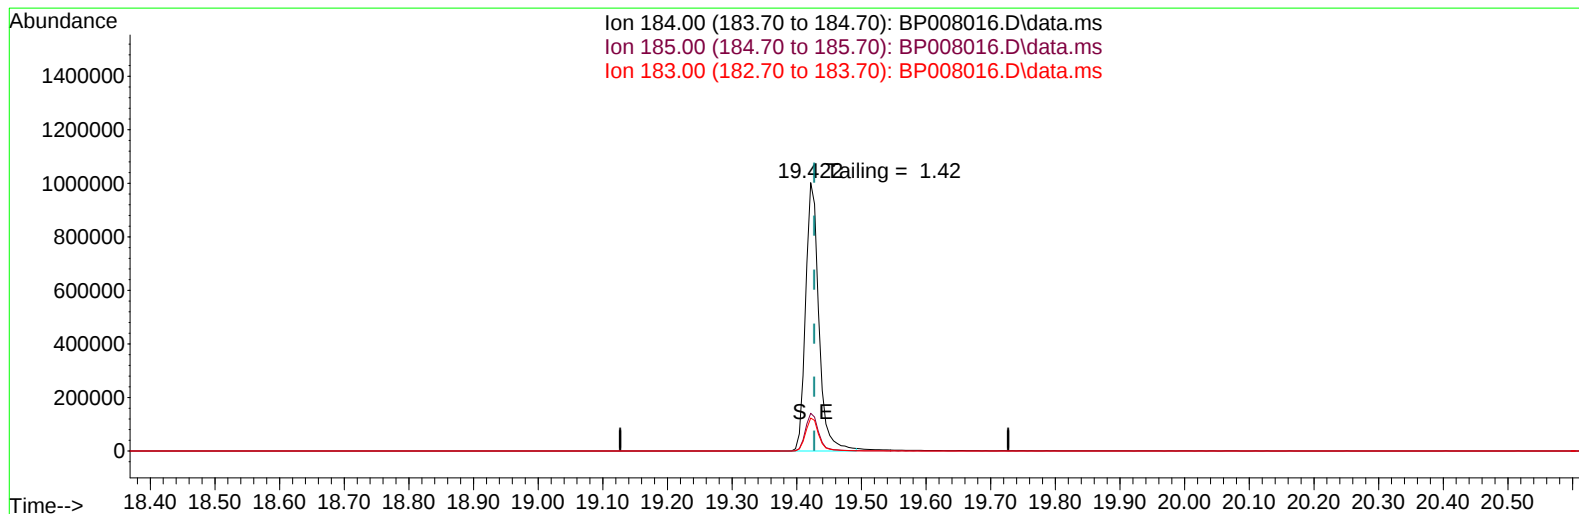

TIC: BP008016.D\data.ms

(77) Benzidine**19.422min (-0.005) 1719539.09 ng****response 1451090**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	14.09
183.00	11.40	12.29
0.00	0.00	0.00