

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111821\
 Data File : BP008008.D
 Acq On : 18 Nov 2021 10:03
 Operator : CG/JU
 Sample : PB140849BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB140849BL

Quant Time: Nov 18 10:51:59 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 15 05:36:49 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.834	152	115944	20.000	ng	0.00
21) Naphthalene-d8	10.634	136	463545	20.000	ng	0.00
39) Acenaphthene-d10	14.475	164	320650	20.000	ng	0.00
64) Phenanthrene-d10	17.233	188	740697	20.000	ng	# 0.00
76) Chrysene-d12	21.322	240	925665	20.000	ng	#-0.01
86) Perylene-d12	23.721	264	1071260	20.000	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.422	112	1039197	145.399	ng	0.00
7) Phenol-d6	7.016	99	1277899	134.399	ng	0.00
23) Nitrobenzene-d5	8.999	82	727827	84.023	ng	0.00
42) 2,4,6-Tribromophenol	15.969	330	689611	136.691	ng	0.00
45) 2-Fluorobiphenyl	13.098	172	1863952	81.541	ng	0.00
79) Terphenyl-d14	19.798	244	3721798	81.528	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111821\
Data File : BP008008.D
Acq On : 18 Nov 2021 10:03
Operator : CG/JU
Sample : PB140849BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB140849BL

Quant Time: Nov 18 10:51:59 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 15 05:36:49 2021
Response via : Initial Calibration




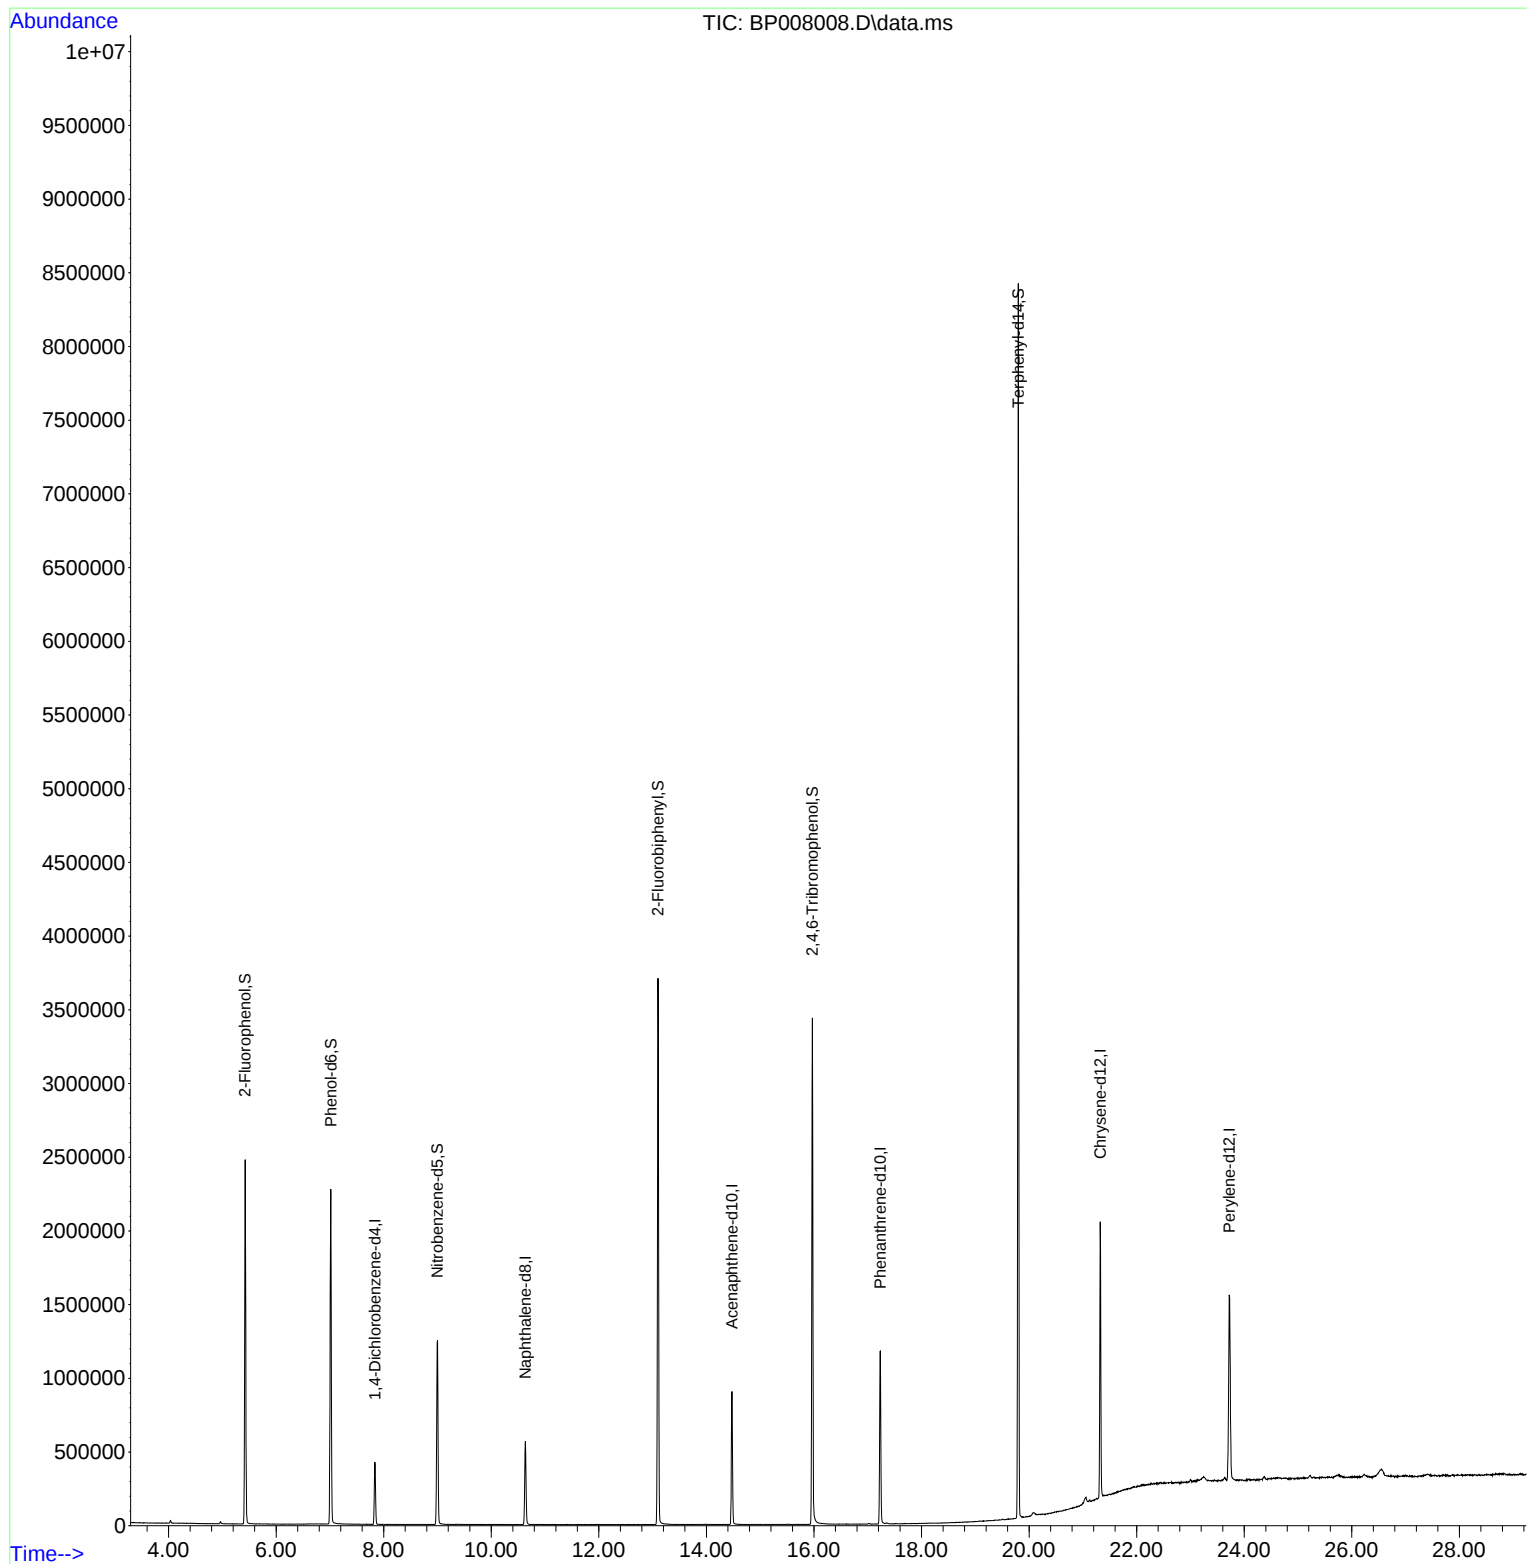


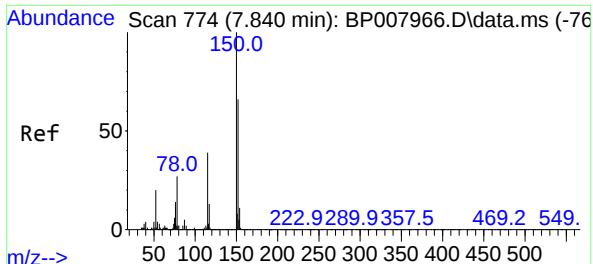

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.834 min Scan# 71
Delta R.T. -0.006 min
Lab File: BP008008.D
Acq: 18 Nov 2021 10:03




Instrument :
BNA_P
ClientSampleId :
PB140849BL


Tgt Ion:152 Resp: 115944
Ion Ratio Lower Upper
152 100
150 157.3 124.1 186.1
115 65.1 48.1 72.1

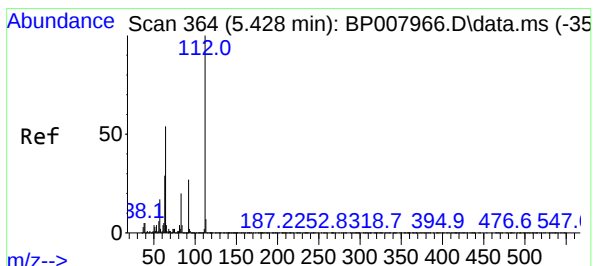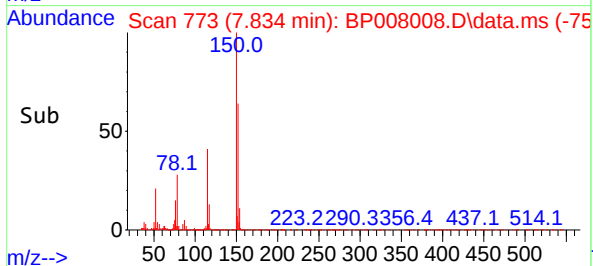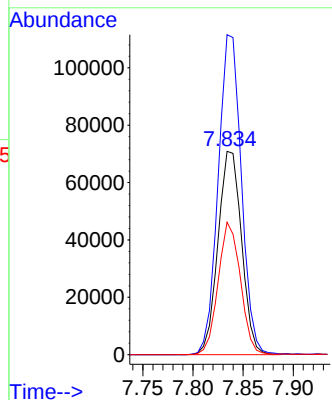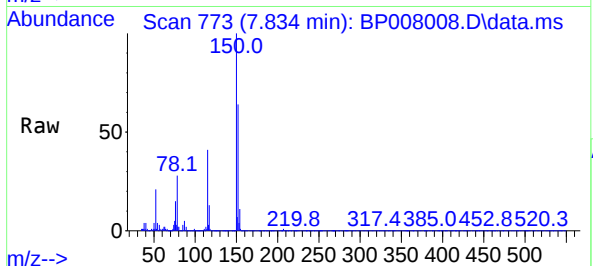

#5
2-Fluorophenol
Concen: 145.399 ng
RT: 5.422 min Scan# 363
Delta R.T. -0.006 min
Lab File: BP008008.D
Acq: 18 Nov 2021 10:03

Tgt Ion:112 Resp: 1039197
Ion Ratio Lower Upper
112 100
64 55.9 46.6 70.0
63 29.8 25.0 37.6


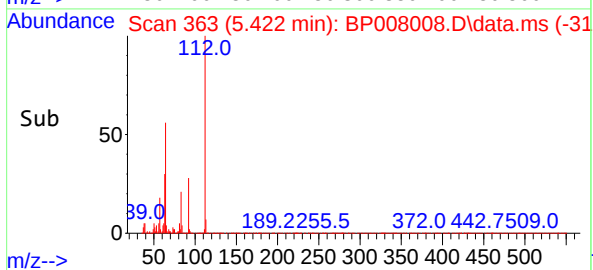
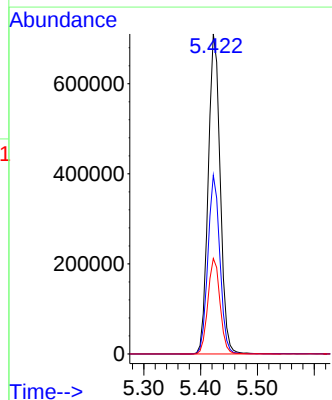
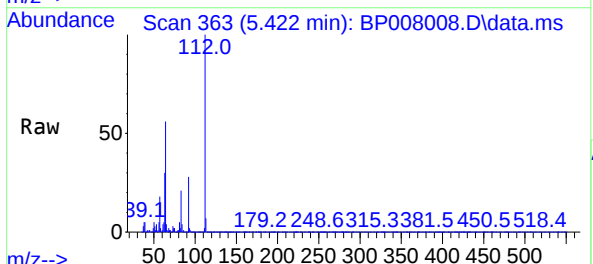


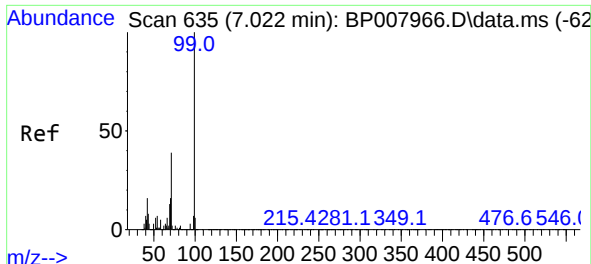

#7
Phenol-d6
Concen: 134.399 ng
RT: 7.016 min Scan# 61
Delta R.T. -0.006 min
Lab File: BP008008.D
Acq: 18 Nov 2021 10:03




Instrument :
BNA_P
ClientSampleId :
PB140849BL


Tgt Ion: 99 Resp: 1277899
Ion Ratio Lower Upper
99 100
42 17.0 14.9 22.3
71 40.1 29.2 43.8

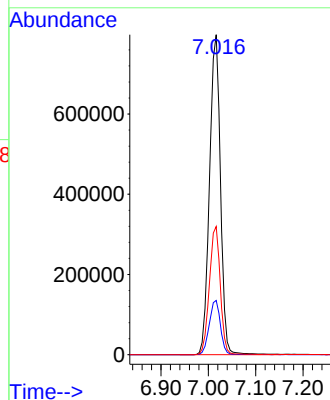

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.634 min Scan# 1249
Delta R.T. -0.006 min
Lab File: BP008008.D
Acq: 18 Nov 2021 10:03

Tgt Ion: 136 Resp: 463545
Ion Ratio Lower Upper
136 100
137 10.5 8.6 13.0
54 7.0 6.2 9.4
68 4.7 4.7 7.1


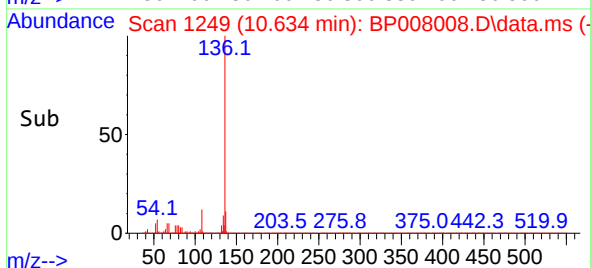
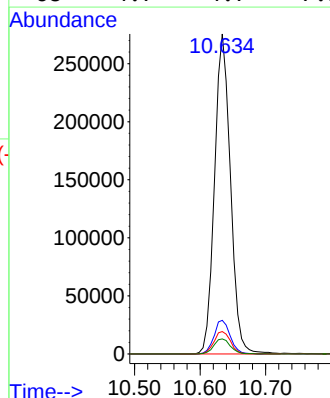
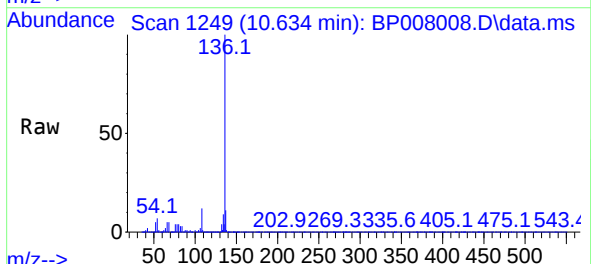


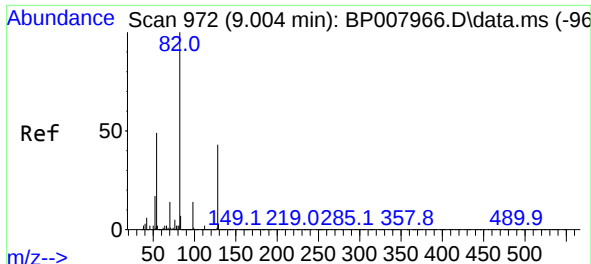

#23
Nitrobenzene-d5
Concen: 84.023 ng
RT: 8.999 min Scan# 91
Delta R.T. -0.005 min
Lab File: BP008008.D
Acq: 18 Nov 2021 10:03




Instrument :
BNA_P
ClientSampleId :
PB140849BL


Tgt Ion: 82 Resp: 727827
Ion Ratio Lower Upper
82 100
128 42.6 32.6 48.8
54 49.4 40.4 60.6

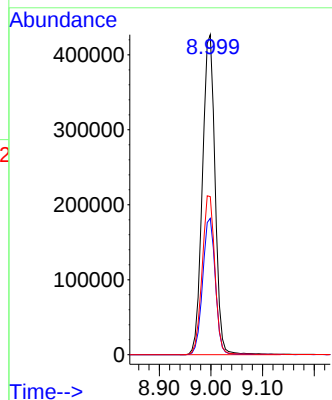

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.475 min Scan# 1902
Delta R.T. -0.006 min
Lab File: BP008008.D
Acq: 18 Nov 2021 10:03

Tgt Ion: 164 Resp: 320650
Ion Ratio Lower Upper
164 100
162 102.0 81.1 121.7
160 45.3 36.0 54.0


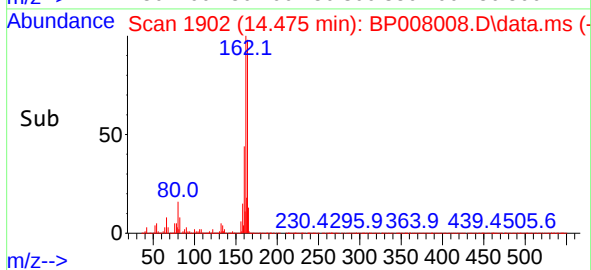
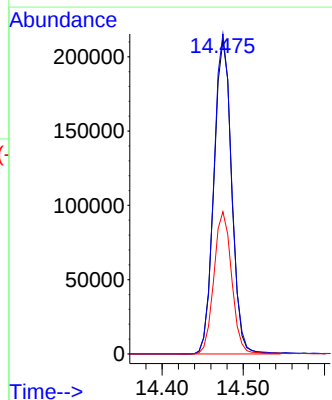
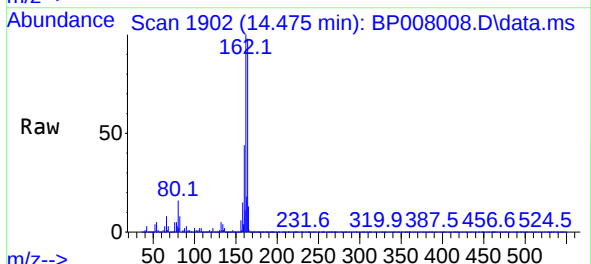




#42
2,4,6-Tribromophenol
Concen: 136.691 ng
RT: 15.969 min Scan# 2157
Delta R.T. -0.006 min
Lab File: BP008008.D
Acq: 18 Nov 2021 10:03




Instrument :
BNA_P
ClientSampleId :
PB140849BL


Tgt Ion:330 Resp: 689611
Ion Ratio Lower Upper
330 100
332 97.0 78.9 118.3
141 30.5 30.7 46.1#

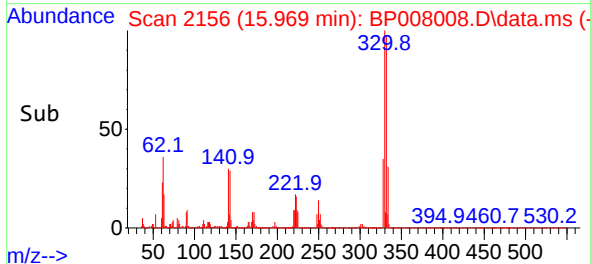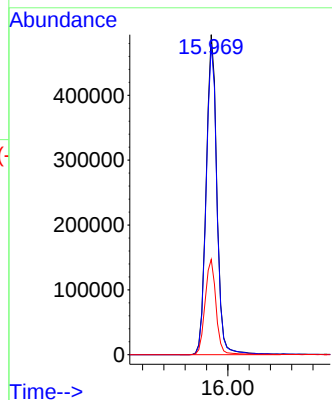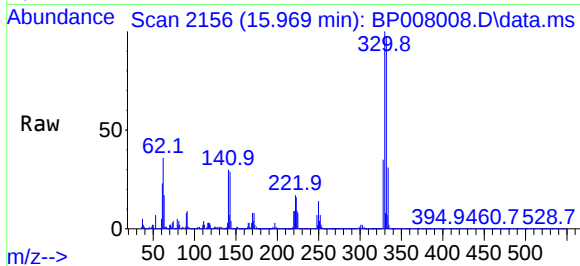

#45
2-Fluorobiphenyl
Concen: 81.541 ng
RT: 13.098 min Scan# 1668
Delta R.T. -0.006 min
Lab File: BP008008.D
Acq: 18 Nov 2021 10:03

Tgt Ion:172 Resp: 1863952
Ion Ratio Lower Upper
172 100
171 36.2 28.2 42.2
170 23.6 19.0 28.4


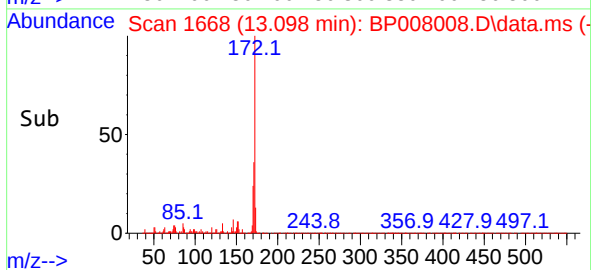
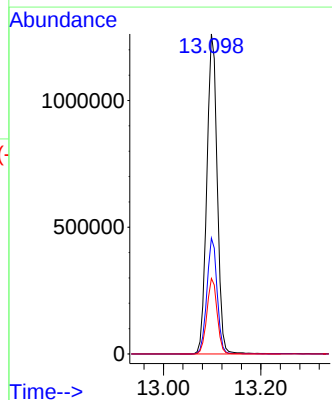
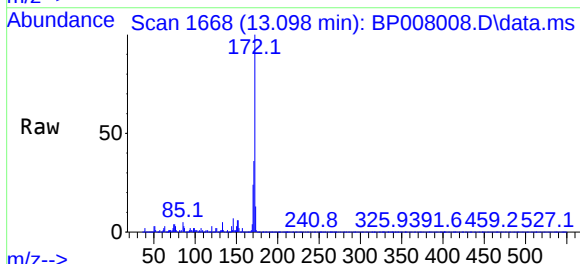


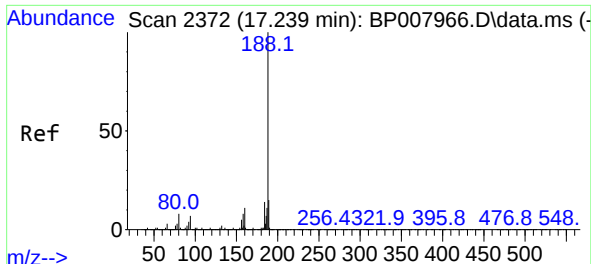

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.233 min Scan# 21
Delta R.T. -0.006 min
Lab File: BP008008.D
Acq: 18 Nov 2021 10:03




Instrument :
BNA_P
ClientSampleId :
PB140849BL


Tgt Ion:188 Resp: 740697
Ion Ratio Lower Upper
188 100
94 6.6 7.1 10.7#
80 7.4 7.8 11.6#

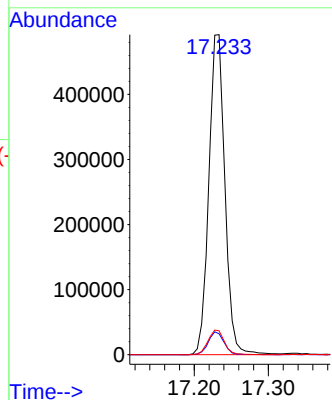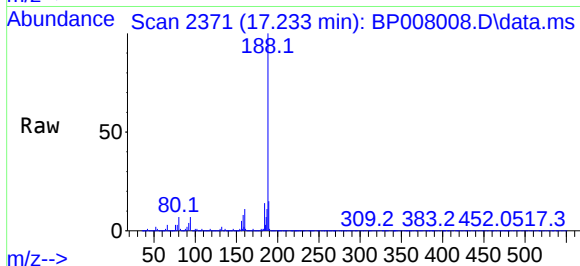

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.322 min Scan# 3066
Delta R.T. -0.012 min
Lab File: BP008008.D
Acq: 18 Nov 2021 10:03

Tgt Ion:240 Resp: 925665
Ion Ratio Lower Upper
240 100
120 7.8 7.8 11.8#
236 26.4 20.6 30.8


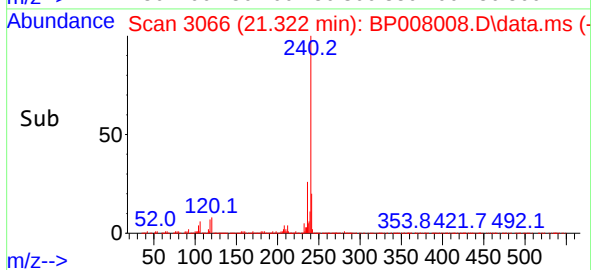
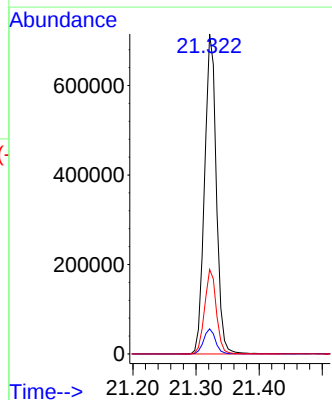
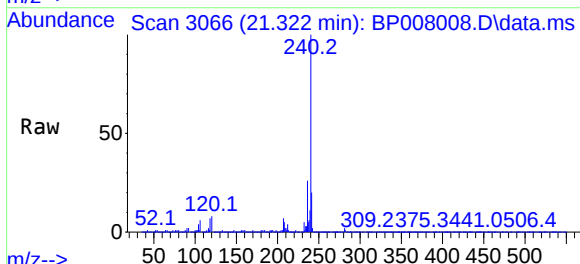


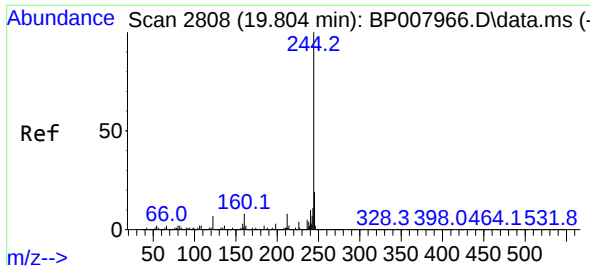

#79
 Terphenyl-d14
 Concen: 81.528 ng
 RT: 19.798 min Scan# 21
 Delta R.T. -0.006 min
 Lab File: BP008008.D
 Acq: 18 Nov 2021 10:03

Instrument :
 BNA_P
 ClientSampleId :
 PB140849BL

Tgt Ion:244 Resp: 3721798
 Ion Ratio Lower Upper
 244 100
 212 7.6 6.2 9.2
 122 7.1 7.8 11.8#

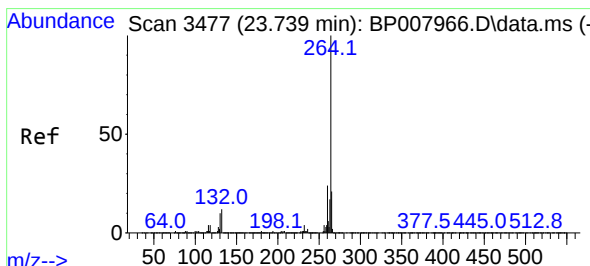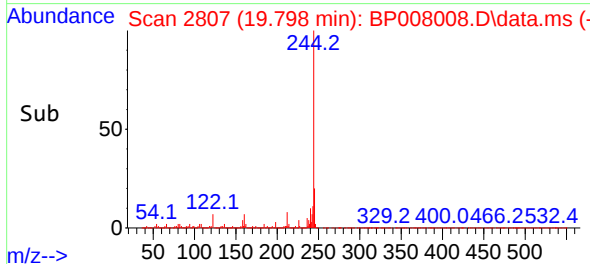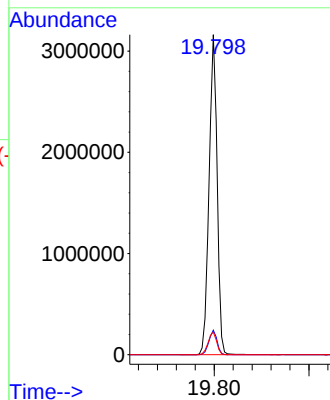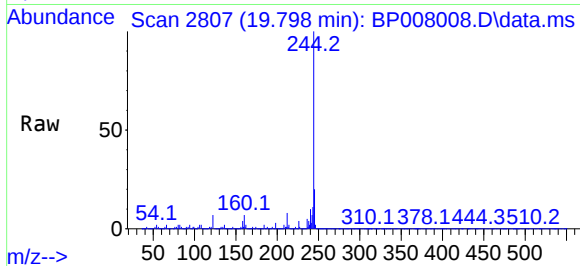

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 23.721 min Scan# 3474
 Delta R.T. -0.018 min
 Lab File: BP008008.D
 Acq: 18 Nov 2021 10:03

Tgt Ion:264 Resp: 1071260
 Ion Ratio Lower Upper
 264 100
 260 24.1 19.1 28.7
 265 22.1 16.7 25.1

