

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111821\
 Data File : BP008022.D
 Acq On : 18 Nov 2021 18:27
 Operator : CG/JU
 Sample : M4666-01RE
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CONCRETERE

Quant Time: Nov 19 02:24:12 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 15 05:36:49 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.834	152	100390	20.000	ng	0.00
21) Naphthalene-d8	10.628	136	331533	20.000	ng	#-0.01
39) Acenaphthene-d10	14.469	164	210017	20.000	ng	-0.01
64) Phenanthrene-d10	17.228	188	463313	20.000	ng	#-0.01
76) Chrysene-d12	21.322	240	571384	20.000	ng	#-0.01
86) Perylene-d12	23.721	264	646239	20.000	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.422	112	44486	7.189	ng	0.00
7) Phenol-d6	7.011	99	268001	32.553	ng	-0.01
23) Nitrobenzene-d5	8.987	82	340836	55.015	ng	-0.02
42) 2,4,6-Tribromophenol	15.969	330	4752	1.438	ng	0.00
45) 2-Fluorobiphenyl	13.093	172	752623	50.268	ng	-0.01
79) Terphenyl-d14	19.792	244	1367104	48.515	ng	-0.01
Target Compounds						
						Qvalue
80) Butylbenzylphthalate	20.475	149	41089	2.912	ng	92
81) Benzo(a)anthracene	21.304	228	96209	2.558	ng	99
83) Chrysene	21.357	228	114082	3.164	ng	98
84) Bis(2-ethylhexyl)phtha...	21.239	149	52501	2.606	ng	# 95
85) Di-n-octyl phthalate	22.163	149	130197	3.507	ng	# 99
88) Benzo(b)fluoranthene	22.992	252	126653	3.292	ng	100
89) Benzo(k)fluoranthene	23.039	252	125868	3.275	ng	96
90) Benzo(a)pyrene	23.616	252	74907	2.277	ng	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111821\
Data File : BP008022.D
Acq On : 18 Nov 2021 18:27
Operator : CG/JU
Sample : M4666-01RE
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CONCRETERE

Quant Time: Nov 19 02:24:12 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 15 05:36:49 2021
Response via : Initial Calibration




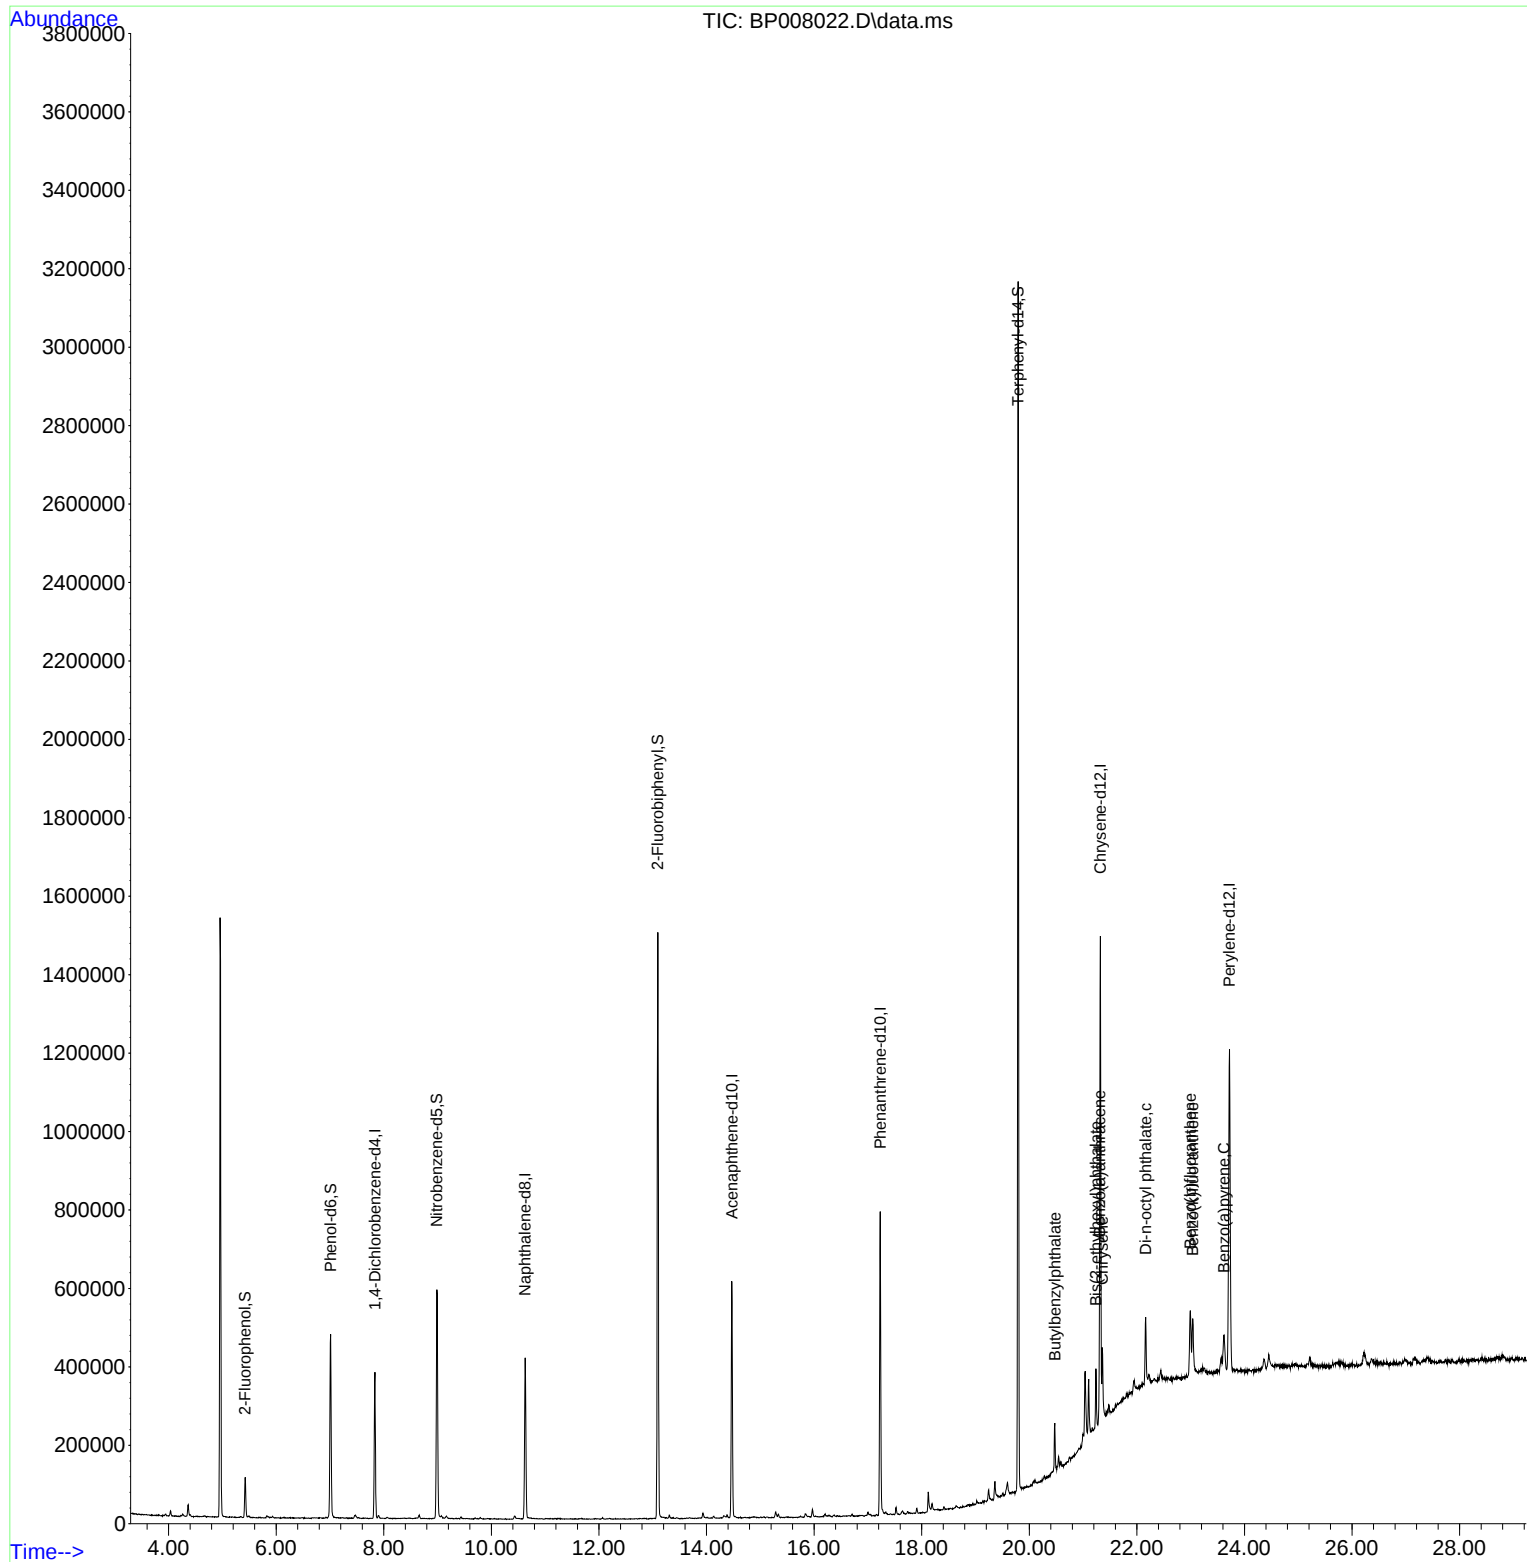




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.834 min Scan# 71
Delta R.T. -0.006 min
Lab File: BP008022.D
Acq: 18 Nov 2021 18:27




Instrument :
BNA_P
ClientSampleId :
CONCRETERE


Tgt Ion:152 Resp: 100390
Ion Ratio Lower Upper
152 100
150 156.5 124.1 186.1
115 63.9 48.1 72.1

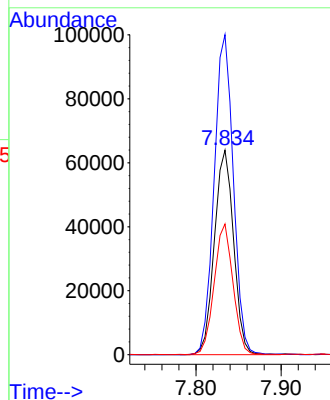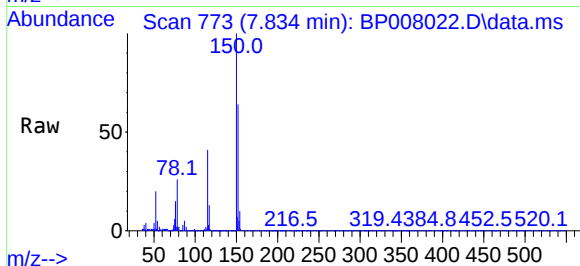

#5
2-Fluorophenol
Concen: 7.189 ng
RT: 5.422 min Scan# 363
Delta R.T. -0.006 min
Lab File: BP008022.D
Acq: 18 Nov 2021 18:27

Tgt Ion:112 Resp: 44486
Ion Ratio Lower Upper
112 100
64 58.6 46.6 70.0
63 29.8 25.0 37.6


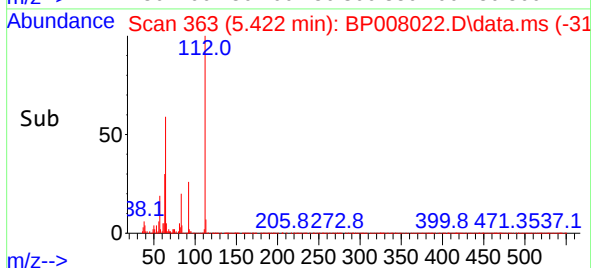
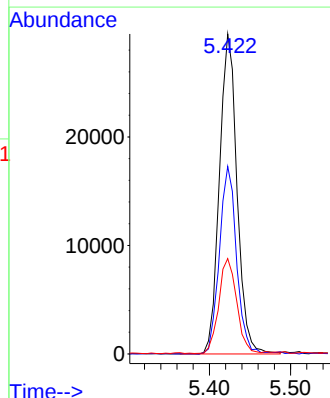
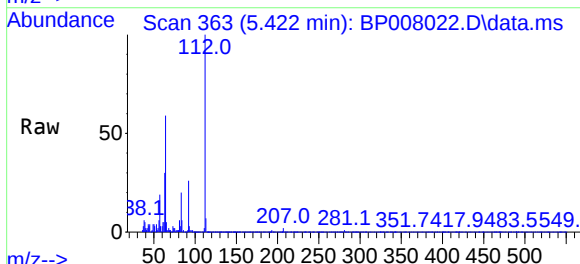




#7
Phenol-d6
Concen: 32.553 ng
RT: 7.011 min Scan# 61
Delta R.T. -0.011 min
Lab File: BP008022.D
Acq: 18 Nov 2021 18:27




Instrument :
BNA_P
ClientSampleId :
CONCRETERE


Tgt Ion: 99 Resp: 268001
Ion Ratio Lower Upper
99 100
42 16.9 14.9 22.3
71 40.0 29.2 43.8

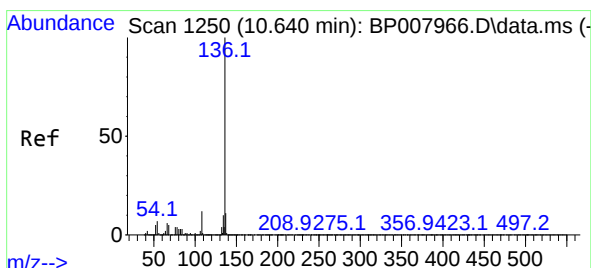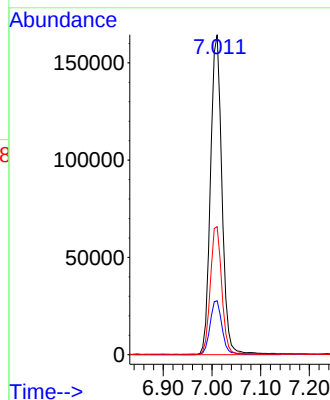

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.628 min Scan# 1248
Delta R.T. -0.012 min
Lab File: BP008022.D
Acq: 18 Nov 2021 18:27

Tgt Ion: 136 Resp: 331533
Ion Ratio Lower Upper
136 100
137 10.5 8.6 13.0
54 7.2 6.2 9.4
68 4.7 4.7 7.1#


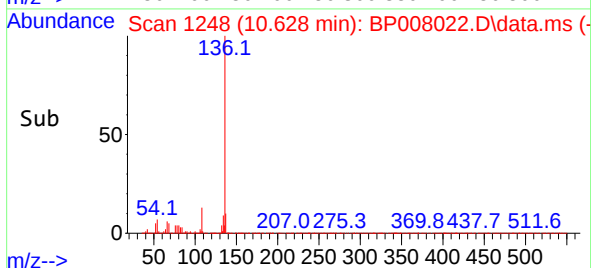
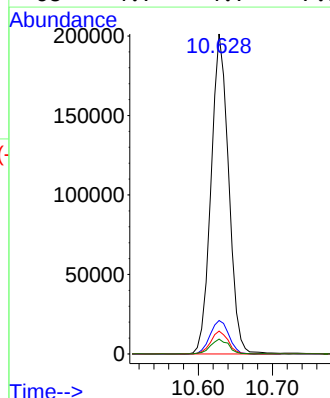





#23
Nitrobenzene-d5
Concen: 55.015 ng
RT: 8.987 min Scan# 90
Delta R.T. -0.017 min
Lab File: BP008022.D
Acq: 18 Nov 2021 18:27




Instrument :
BNA_P
ClientSampleId :
CONCRETERE


Tgt Ion: 82 Resp: 340836
Ion Ratio Lower Upper
82 100
128 42.6 32.6 48.8
54 49.4 40.4 60.6

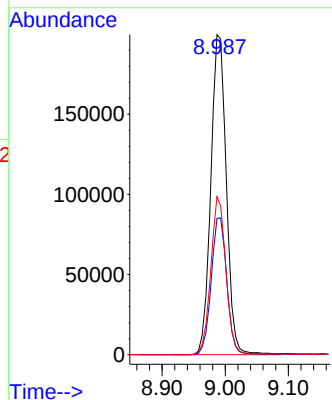

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.469 min Scan# 1901
Delta R.T. -0.012 min
Lab File: BP008022.D
Acq: 18 Nov 2021 18:27

Tgt Ion: 164 Resp: 210017
Ion Ratio Lower Upper
164 100
162 101.1 81.1 121.7
160 45.9 36.0 54.0


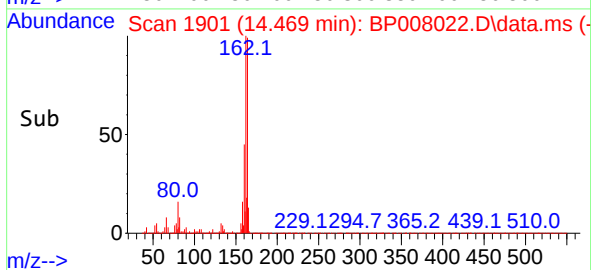
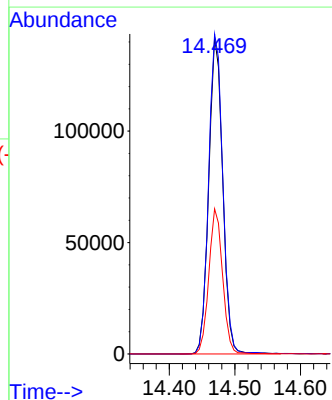





#42
2,4,6-Tribromophenol
Concen: 1.438 ng
RT: 15.969 min Scan# 2157
Delta R.T. -0.006 min
Lab File: BP008022.D
Acq: 18 Nov 2021 18:27




Instrument :
BNA_P
ClientSampleId :
CONCRETERE


Tgt Ion:330 Resp: 4752
Ion Ratio Lower Upper
330 100
332 89.5 78.9 118.3
141 31.4 30.7 46.1

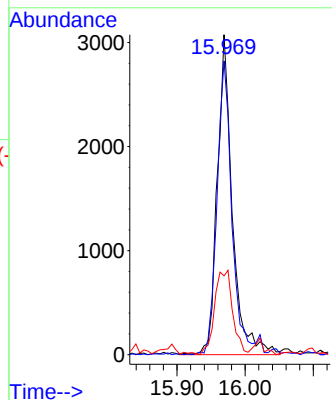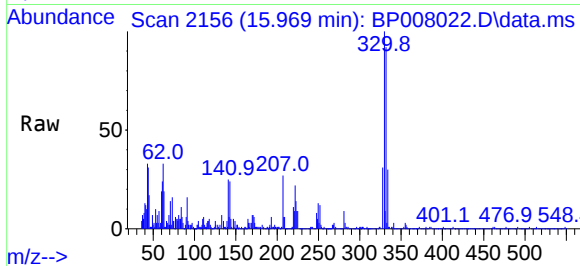

#45
2-Fluorobiphenyl
Concen: 50.268 ng
RT: 13.093 min Scan# 1667
Delta R.T. -0.011 min
Lab File: BP008022.D
Acq: 18 Nov 2021 18:27

Tgt Ion:172 Resp: 752623
Ion Ratio Lower Upper
172 100
171 35.8 28.2 42.2
170 23.0 19.0 28.4


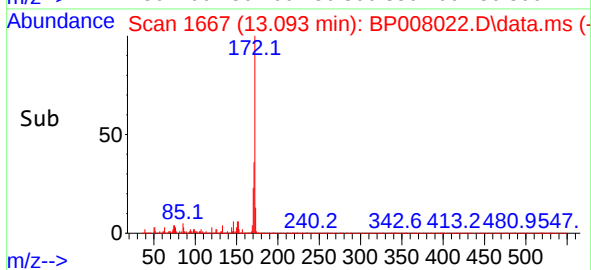
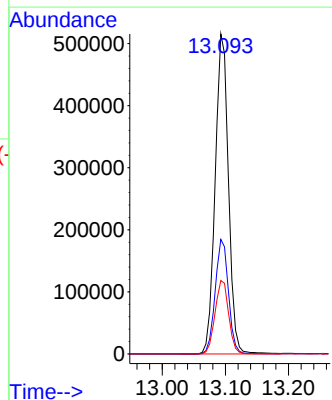
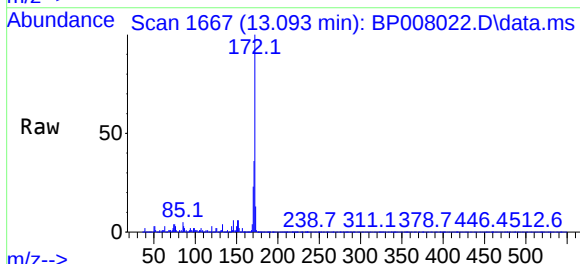




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.228 min Scan# 21
Delta R.T. -0.012 min
Lab File: BP008022.D
Acq: 18 Nov 2021 18:27




Instrument :
BNA_P
ClientSampleId :
CONCRETERE


Tgt Ion:188 Resp: 463313
Ion Ratio Lower Upper
188 100
94 6.7 7.1 10.7#
80 7.3 7.8 11.6#

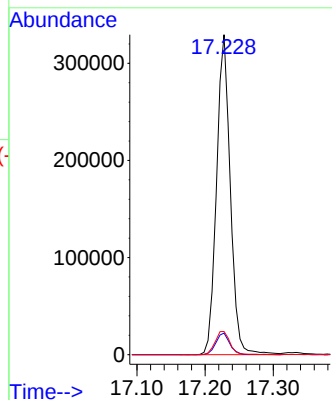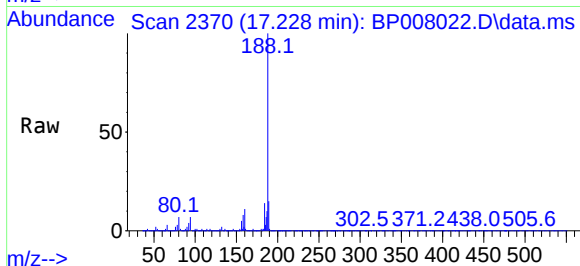

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.322 min Scan# 3066
Delta R.T. -0.012 min
Lab File: BP008022.D
Acq: 18 Nov 2021 18:27

Tgt Ion:240 Resp: 571384
Ion Ratio Lower Upper
240 100
120 7.7 7.8 11.8#
236 25.7 20.6 30.8


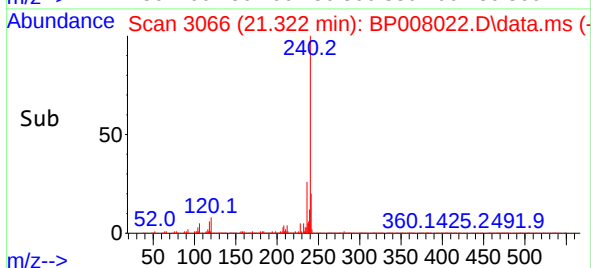
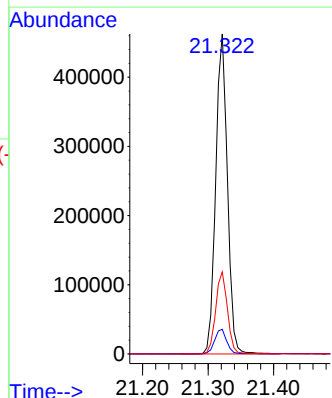
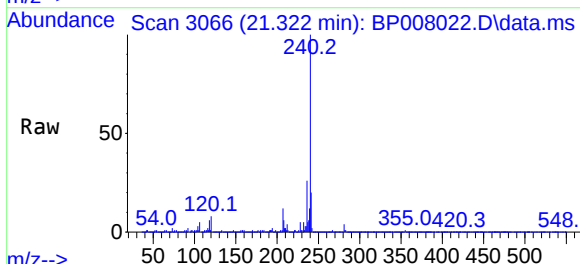




#79
Terphenyl-d14
Concen: 48.515 ng
RT: 19.792 min Scan# 21
Delta R.T. -0.012 min
Lab File: BP008022.D
Acq: 18 Nov 2021 18:27




Instrument :
BNA_P
ClientSampleId :
CONCRETERE


Tgt Ion:244 Resp: 1367104
Ion Ratio Lower Upper
244 100
212 7.5 6.2 9.2
122 7.6 7.8 11.8#

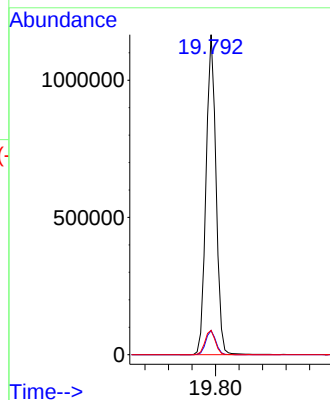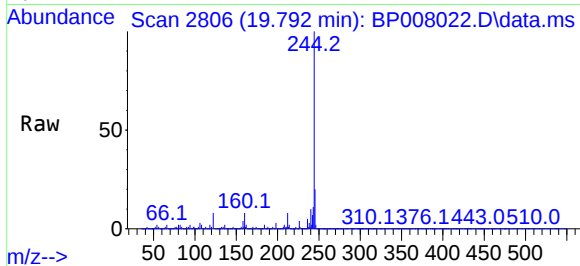

#80
Butylbenzylphthalate
Concen: 2.912 ng
RT: 20.475 min Scan# 2922
Delta R.T. -0.006 min
Lab File: BP008022.D
Acq: 18 Nov 2021 18:27

Tgt Ion:149 Resp: 41089
Ion Ratio Lower Upper
149 100
91 63.9 56.6 85.0
206 24.6 17.4 26.2


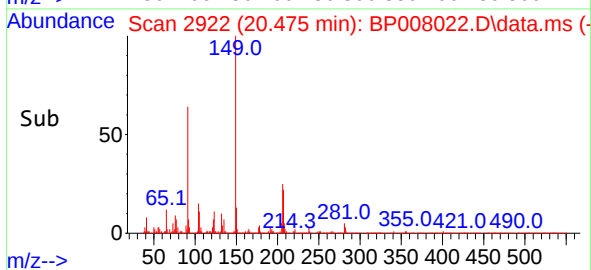
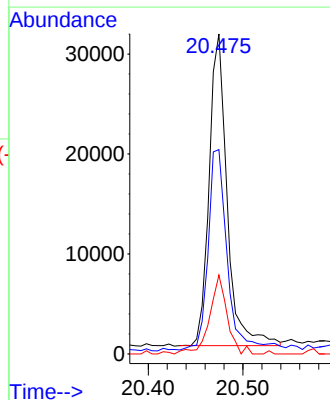
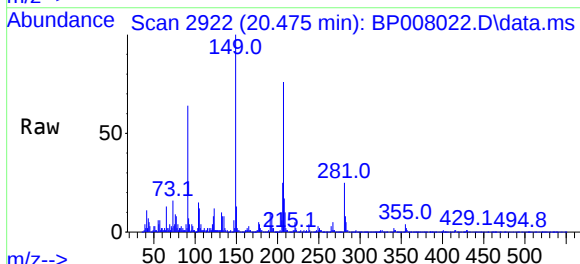




#81
Benzo(a)anthracene
Concen: 2.558 ng
RT: 21.304 min Scan# 3065
Delta R.T. -0.012 min
Lab File: BP008022.D
Acq: 18 Nov 2021 18:27




Instrument :
BNA_P
ClientSampleId :
CONCRETERE


Tgt Ion:228 Resp: 96209
Ion Ratio Lower Upper
228 100
226 26.4 21.8 32.6
229 20.3 15.7 23.5

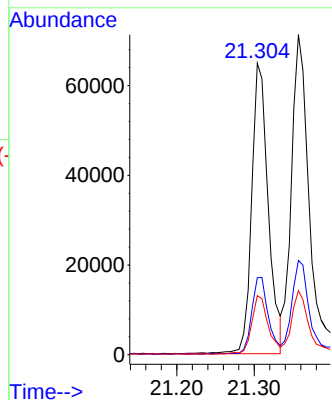

#83
Chrysene
Concen: 3.164 ng
RT: 21.357 min Scan# 3072
Delta R.T. -0.012 min
Lab File: BP008022.D
Acq: 18 Nov 2021 18:27

Tgt Ion:228 Resp: 114082
Ion Ratio Lower Upper
228 100
226 29.4 24.6 37.0
229 20.0 15.7 23.5


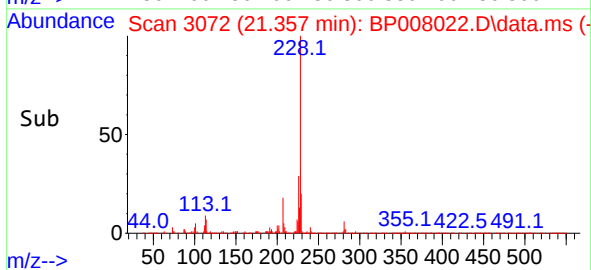
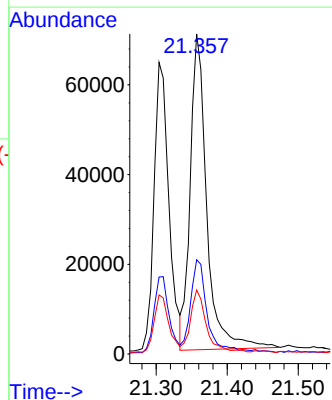





#84
Bis(2-ethylhexyl)phthalate
Concen: 2.606 ng
RT: 21.239 min Scan# 30
Delta R.T. -0.006 min
Lab File: BP008022.D
Acq: 18 Nov 2021 18:27




Instrument :
BNA_P
ClientSampleId :
CONCRETERE


Tgt Ion:149 Resp: 52501
Ion Ratio Lower Upper
149 100
167 29.7 21.6 32.4
279 5.1 3.3 4.9#

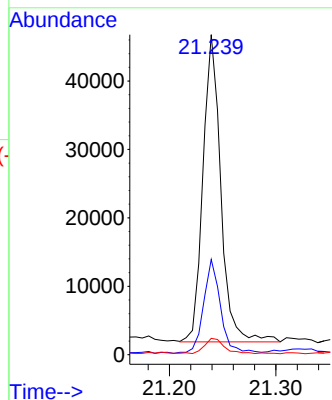

#85
Di-n-octyl phthalate
Concen: 3.507 ng
RT: 22.163 min Scan# 3209
Delta R.T. -0.012 min
Lab File: BP008022.D
Acq: 18 Nov 2021 18:27

Tgt Ion:149 Resp: 130197
Ion Ratio Lower Upper
149 100
167 2.1 1.3 1.9#
43 8.7 7.3 10.9


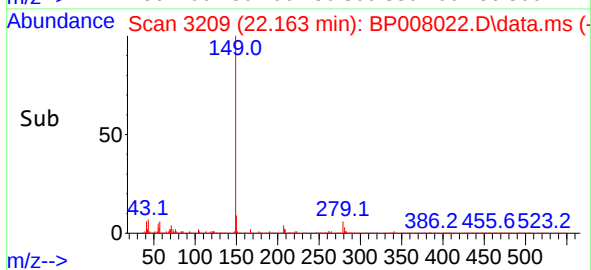
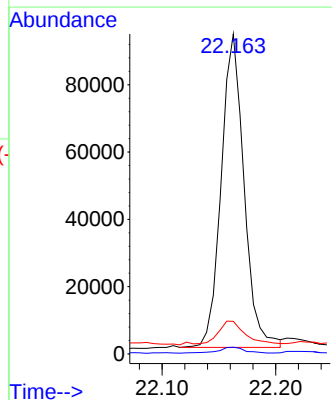





#86
Perylene-d12
Concen: 20.000 ng
RT: 23.721 min Scan# 34
Delta R.T. -0.017 min
Lab File: BP008022.D
Acq: 18 Nov 2021 18:27




Instrument :
BNA_P
ClientSampleId :
CONCRETERE


Tgt Ion:264 Resp: 646239
Ion Ratio Lower Upper
264 100
260 23.8 19.1 28.7
265 22.2 16.7 25.1

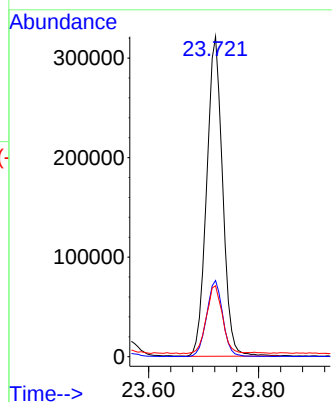

#88
Benzo(b)fluoranthene
Concen: 3.292 ng
RT: 22.992 min Scan# 3350
Delta R.T. -0.017 min
Lab File: BP008022.D
Acq: 18 Nov 2021 18:27

Tgt Ion:252 Resp: 126653
Ion Ratio Lower Upper
252 100
253 22.0 17.4 26.2
125 9.2 7.4 11.0


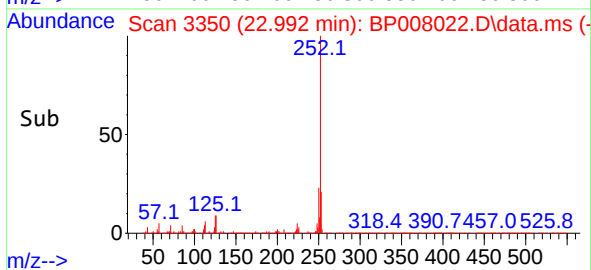
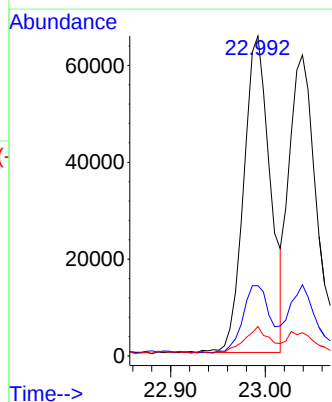





#89
Benzo(k)fluoranthene
Concen: 3.275 ng
RT: 23.039 min Scan# 31
Delta R.T. -0.018 min
Lab File: BP008022.D
Acq: 18 Nov 2021 18:27

Instrument :
BNA_P
ClientSampleId :
CONCRETERE

Tgt Ion:252 Resp: 125868
Ion Ratio Lower Upper
252 100
253 23.7 17.6 26.4
125 7.7 7.4 11.0

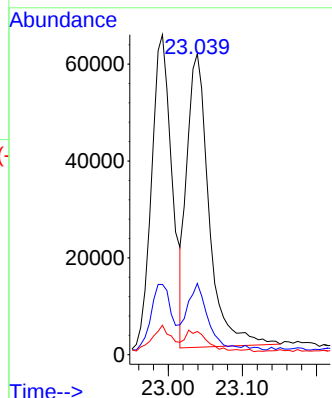

#90
Benzo(a)pyrene
Concen: 2.277 ng
RT: 23.616 min Scan# 3456
Delta R.T. -0.017 min
Lab File: BP008022.D
Acq: 18 Nov 2021 18:27

Tgt Ion:252 Resp: 74907
Ion Ratio Lower Upper
252 100
253 22.2 17.6 26.4
125 9.1 8.4 12.6

