

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111821\
Data File : BP008008.D
Acq On : 18 Nov 2021 10:03
Operator : CG/JU
Sample : PB140849BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB140849BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111321.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP008008.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.422	356	363	379	rBV	2471565	3596416	36.20%	9.062%
2	7.016	626	634	652	rBV	2270592	3674106	36.99%	9.258%
3	7.834	766	773	783	rBV	422991	678906	6.83%	1.711%
4	8.999	963	971	981	rBV	1249279	2144592	21.59%	5.404%
5	10.634	1240	1249	1264	rBV	564544	967302	9.74%	2.437%
6	13.098	1660	1668	1686	rBV	3706803	5419800	54.56%	13.656%
7	14.475	1895	1902	1912	rBV	902336	1375951	13.85%	3.467%
8	15.969	2148	2156	2185	rBV	3435095	4942304	49.75%	12.453%
9	17.233	2363	2371	2386	rBV	1173825	1791482	18.03%	4.514%
10	19.798	2801	2807	2818	rBV	8374831	9934010	100.00%	25.031%
11	21.322	3061	3066	3074	rBV	1872525	2437325	24.54%	6.141%
12	23.721	3468	3474	3491	rVB2	1255466	2725286	27.43%	6.867%




Sum of corrected areas: 39687480

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111821\
Data File : BP008008.D
Acq On : 18 Nov 2021 10:03
Operator : CG/JU
Sample : PB140849BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB140849BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

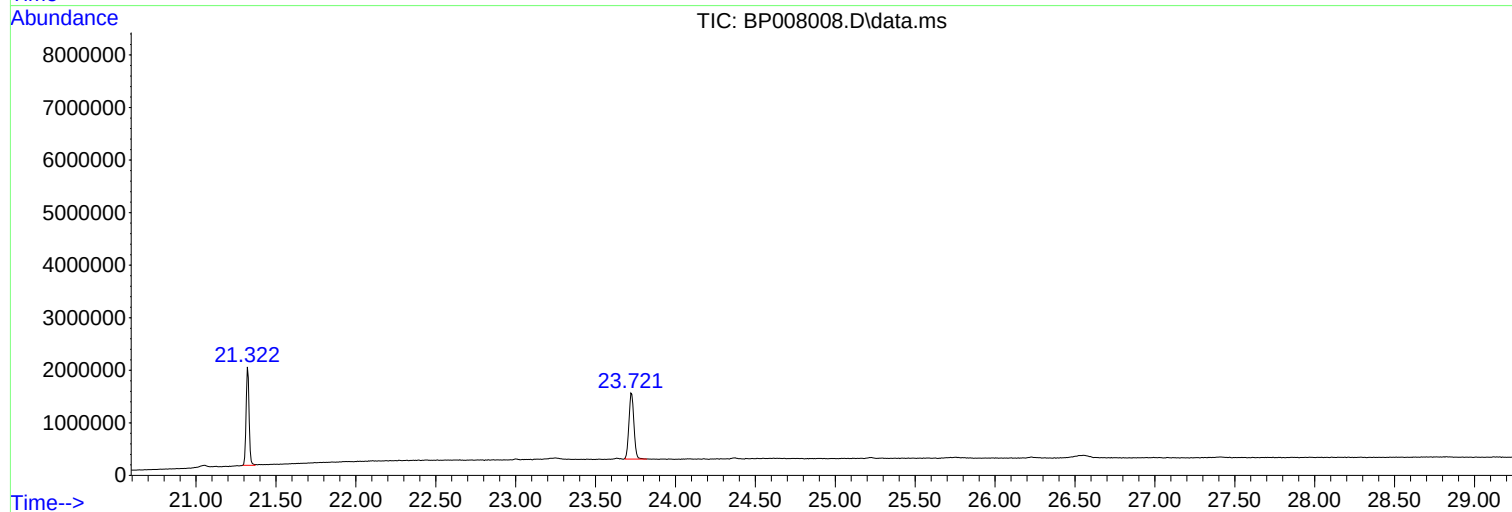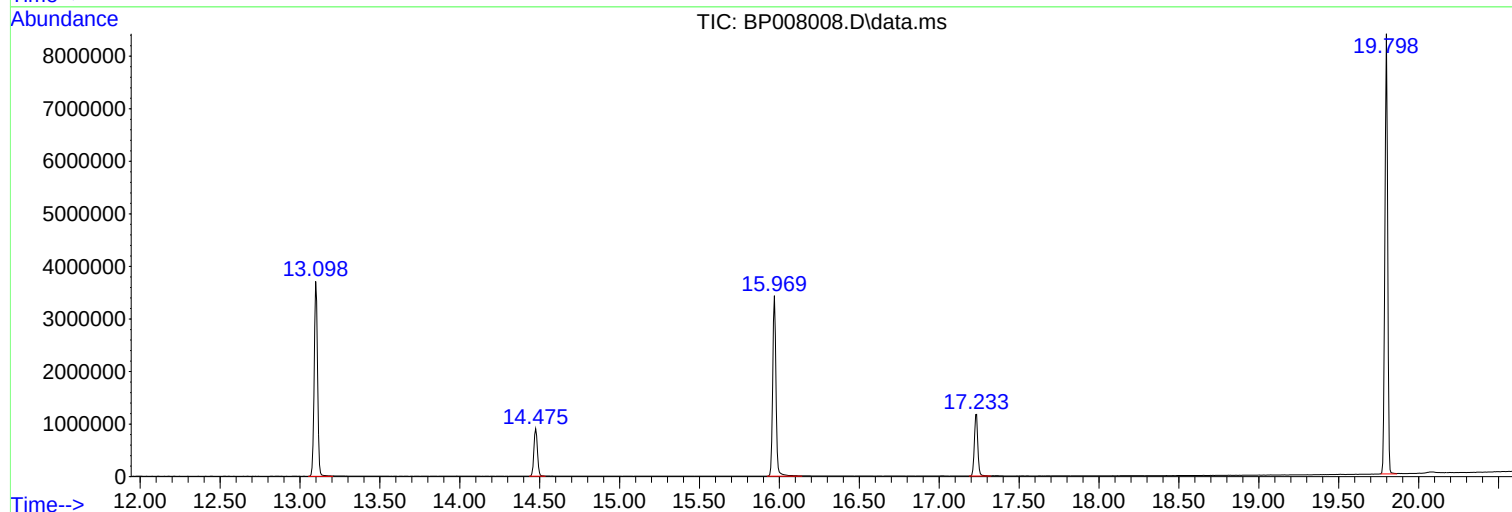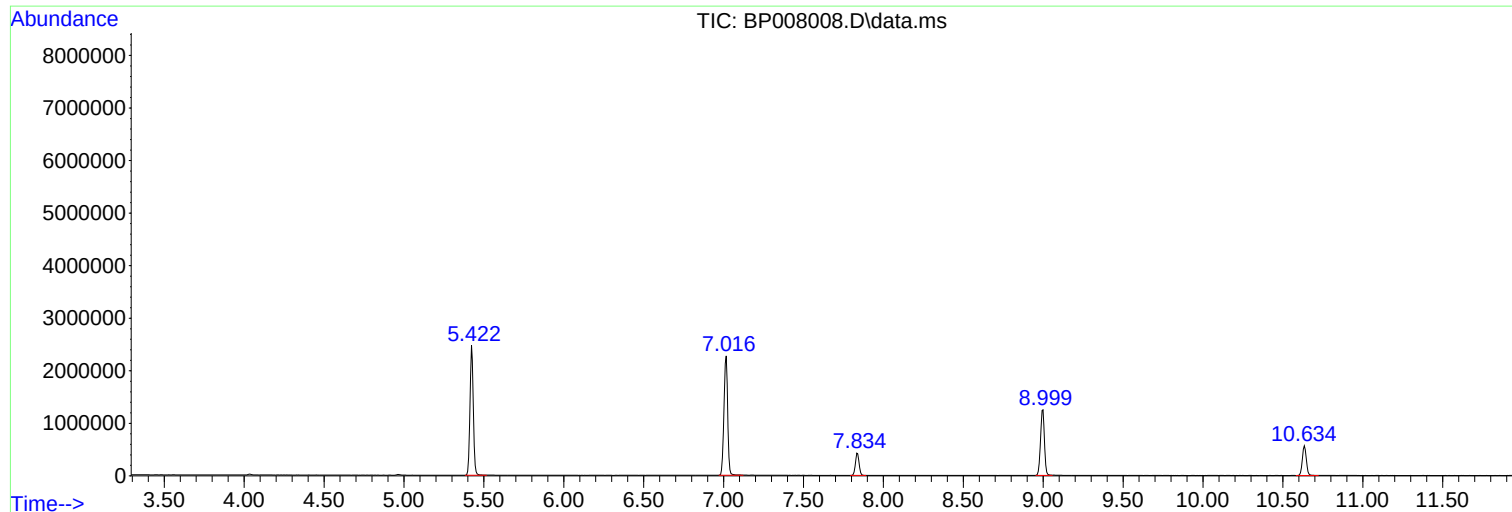

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111821\
Data File : BP008008.D
Acq On : 18 Nov 2021 10:03
Operator : CG/JU
Sample : PB140849BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB140849BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111821\
Data File : BP008008.D
Acq On : 18 Nov 2021 10:03
Operator : CG/JU
Sample : PB140849BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB140849BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------