
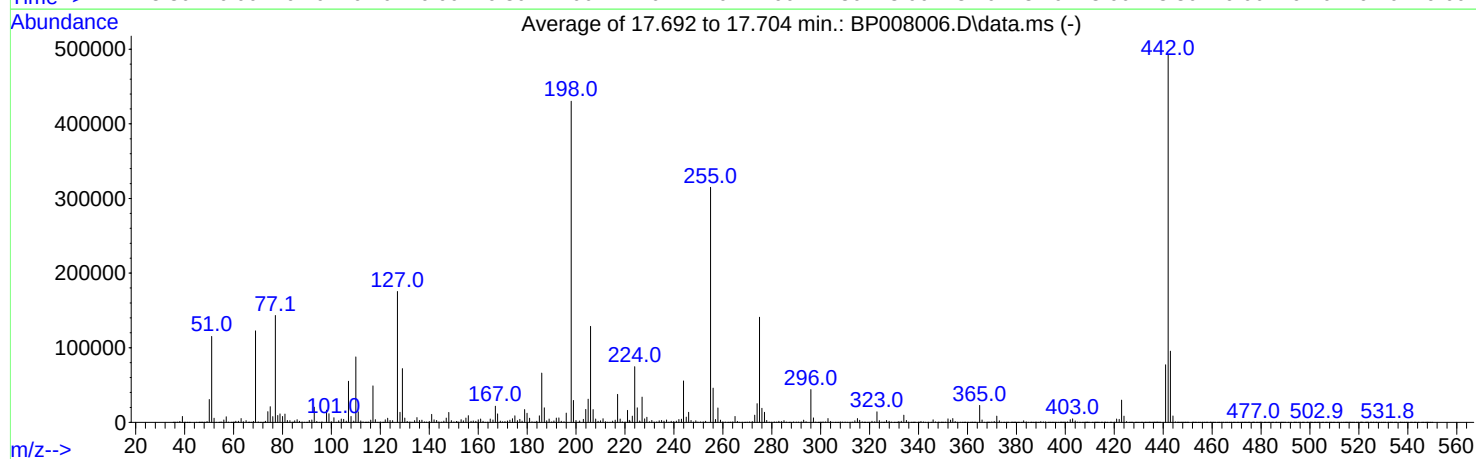


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111821\
 Data File : BP008006.D
 Acq On : 18 Nov 2021 08:53
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Nov 15 05:36:49 2021

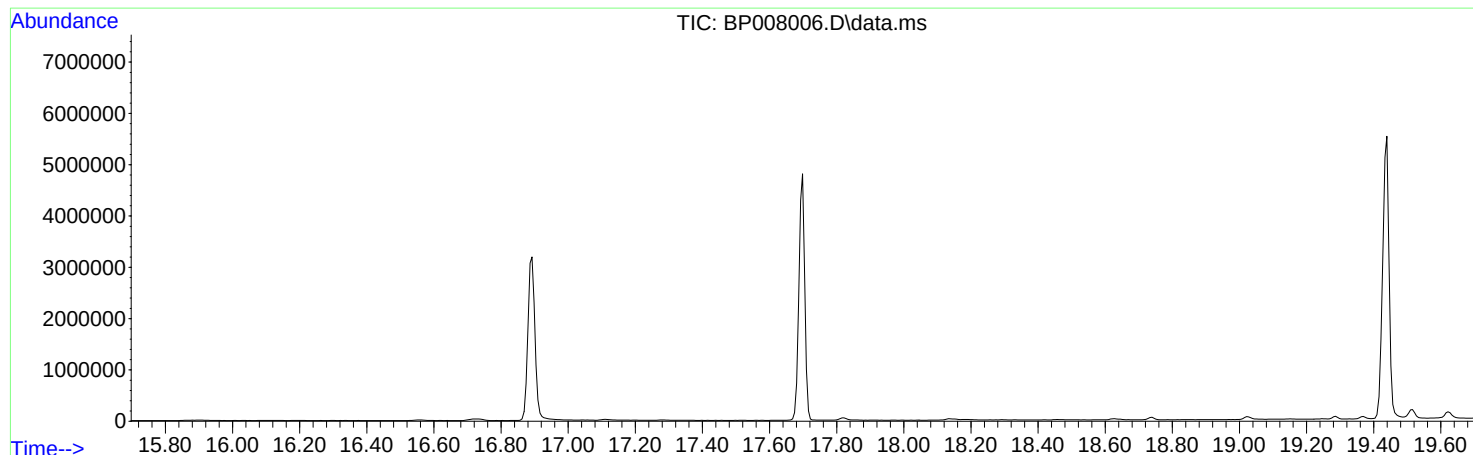




AutoFind: Scans 2449, 2450, 2451; Background Corrected with Scan 2440

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.8	115229	PASS
68	69	0.00	2	1.1	1352	PASS
69	198	0.00	100	28.5	122765	PASS
70	69	0.00	2	0.6	728	PASS
127	198	10	80	40.7	175331	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	430324	PASS
199	198	5	9	6.8	29307	PASS
275	198	10	60	32.8	140936	PASS
365	198	1	100	5.3	22720	PASS
441	198	0.01	100	17.9	77221	PASS
442	442	100	100	100.0	492928	PASS
443	442	15	24	19.4	95472	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111821\
Data File : BP008006.D
Acq On : 18 Nov 2021 08:53
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Nov 18 10:02:27 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 15 05:36:49 2021
Response via : Initial Calibration

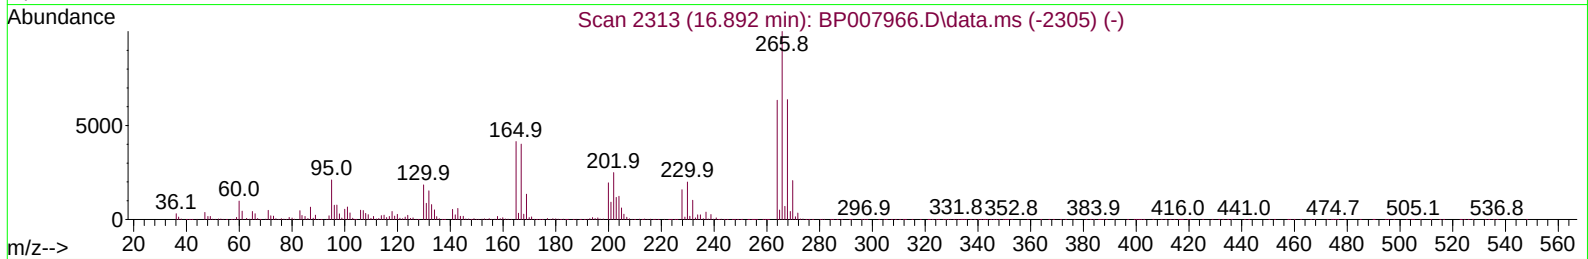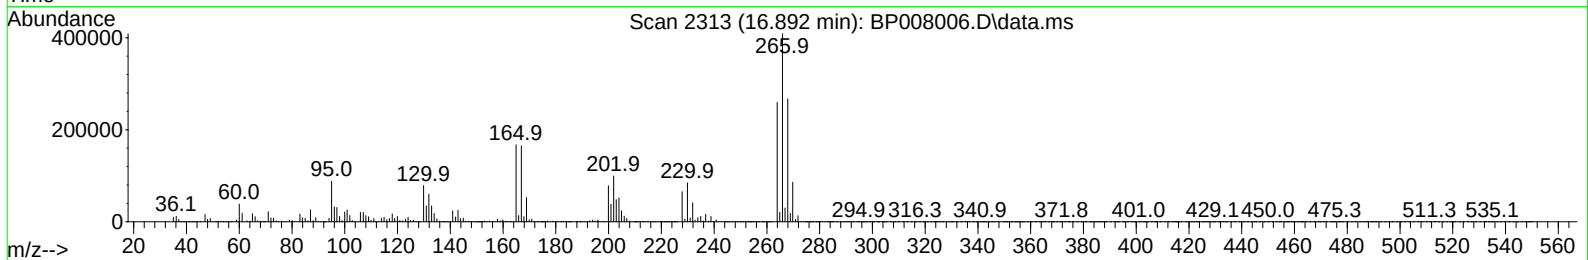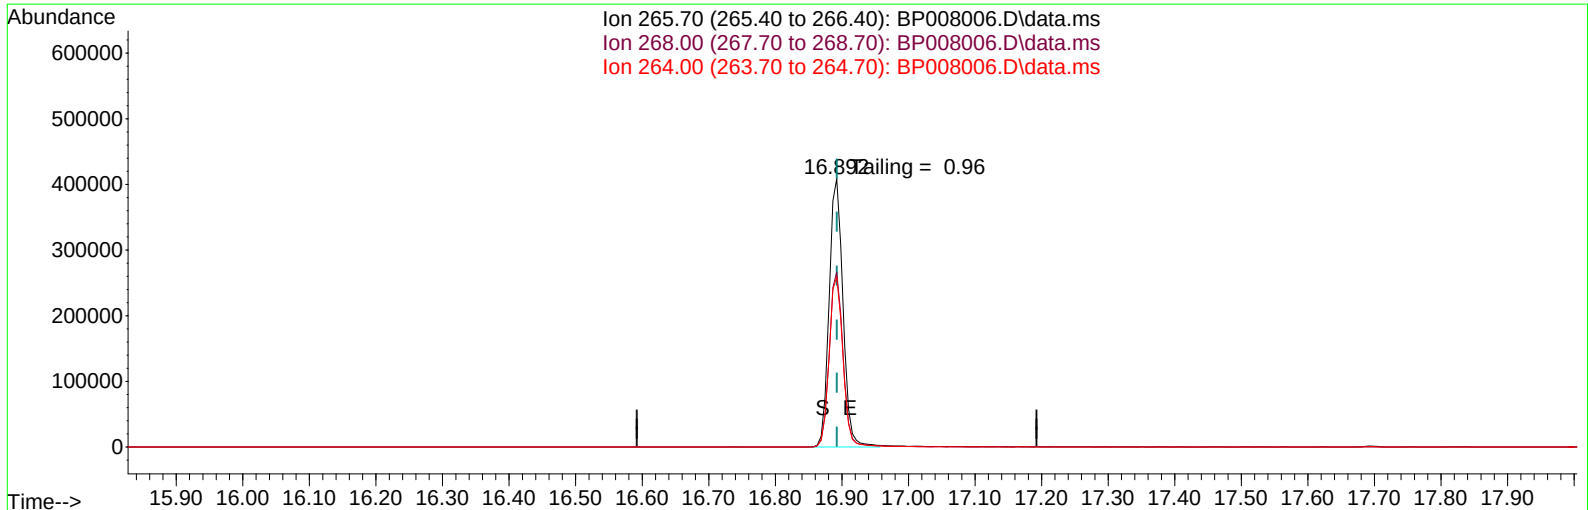

TIC: BP008006.D\data.ms

(70) Pentachlorophenol (C)

16.892min (+ 0.000) 121697.76 ng




response 594335

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.60	65.25
264.00	60.90	63.48
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111821\
Data File : BP008006.D
Acq On : 18 Nov 2021 08:53
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Nov 18 10:02:27 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 15 05:36:49 2021
Response via : Initial Calibration

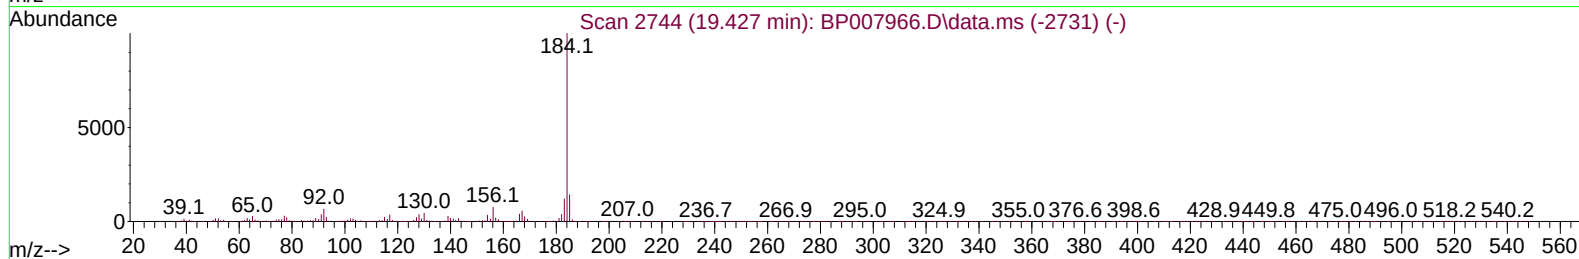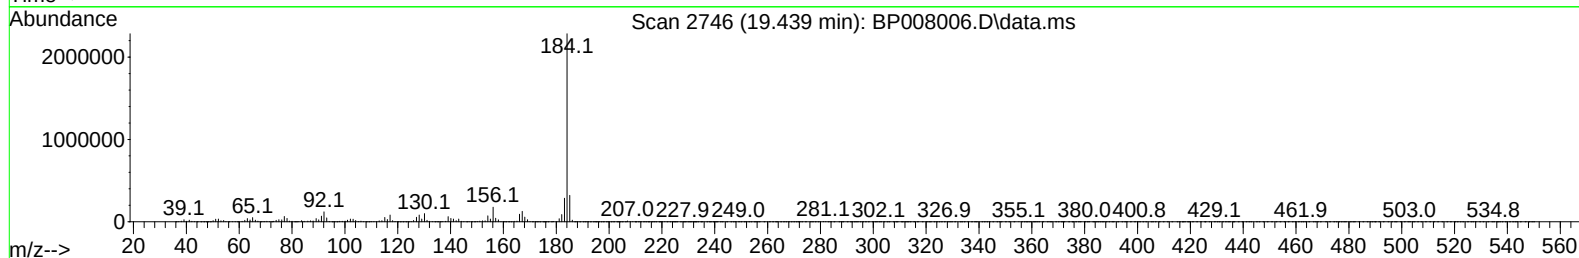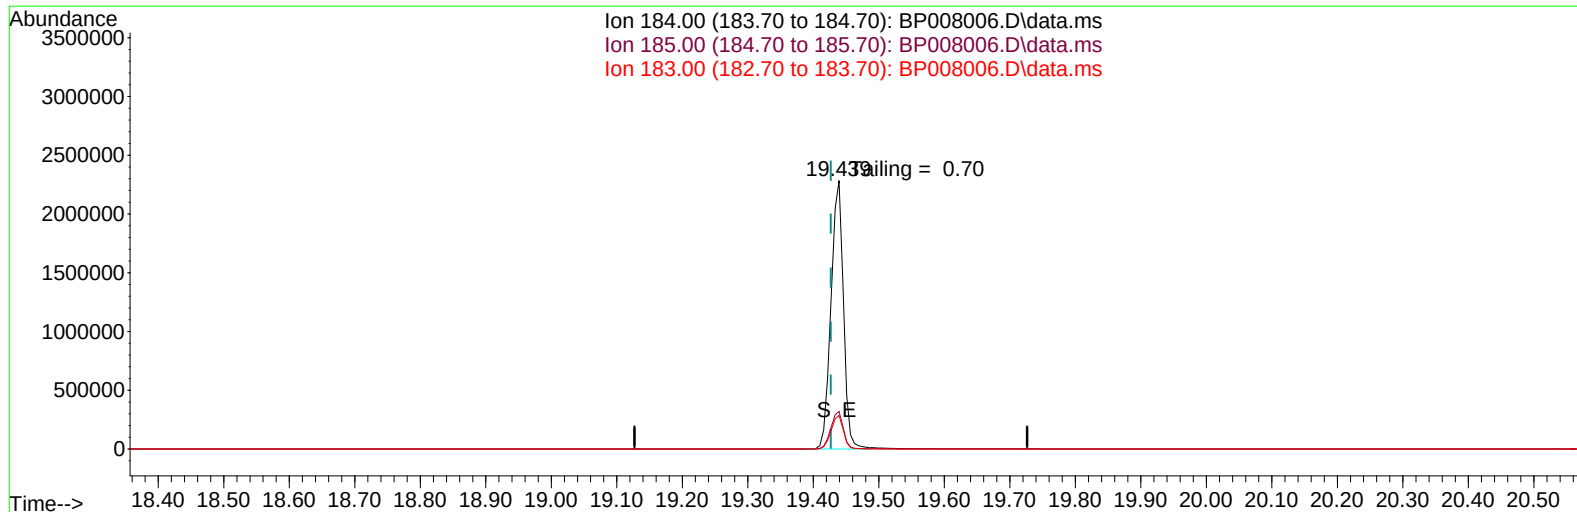

TIC: BP008006.D\data.ms

(77) Benzidine

19.439min (+ 0.012) 22312.33 ng

response 3047217

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	14.01
183.00	11.40	12.51
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/18/2021	BNA_P	<u>BP008006.D</u>
Compound Name	Response	Retention Time
DDT	1770424	20.63
DDD	21187	20.21
DDE	3603	19.71
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
24790	1795214	1.38

Instrument :
BNA_P
ClientSampleId :
DFTPP