


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111821\
 Data File : BP008016.D
 Acq On : 18 Nov 2021 14:56
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Nov 15 05:36:49 2021

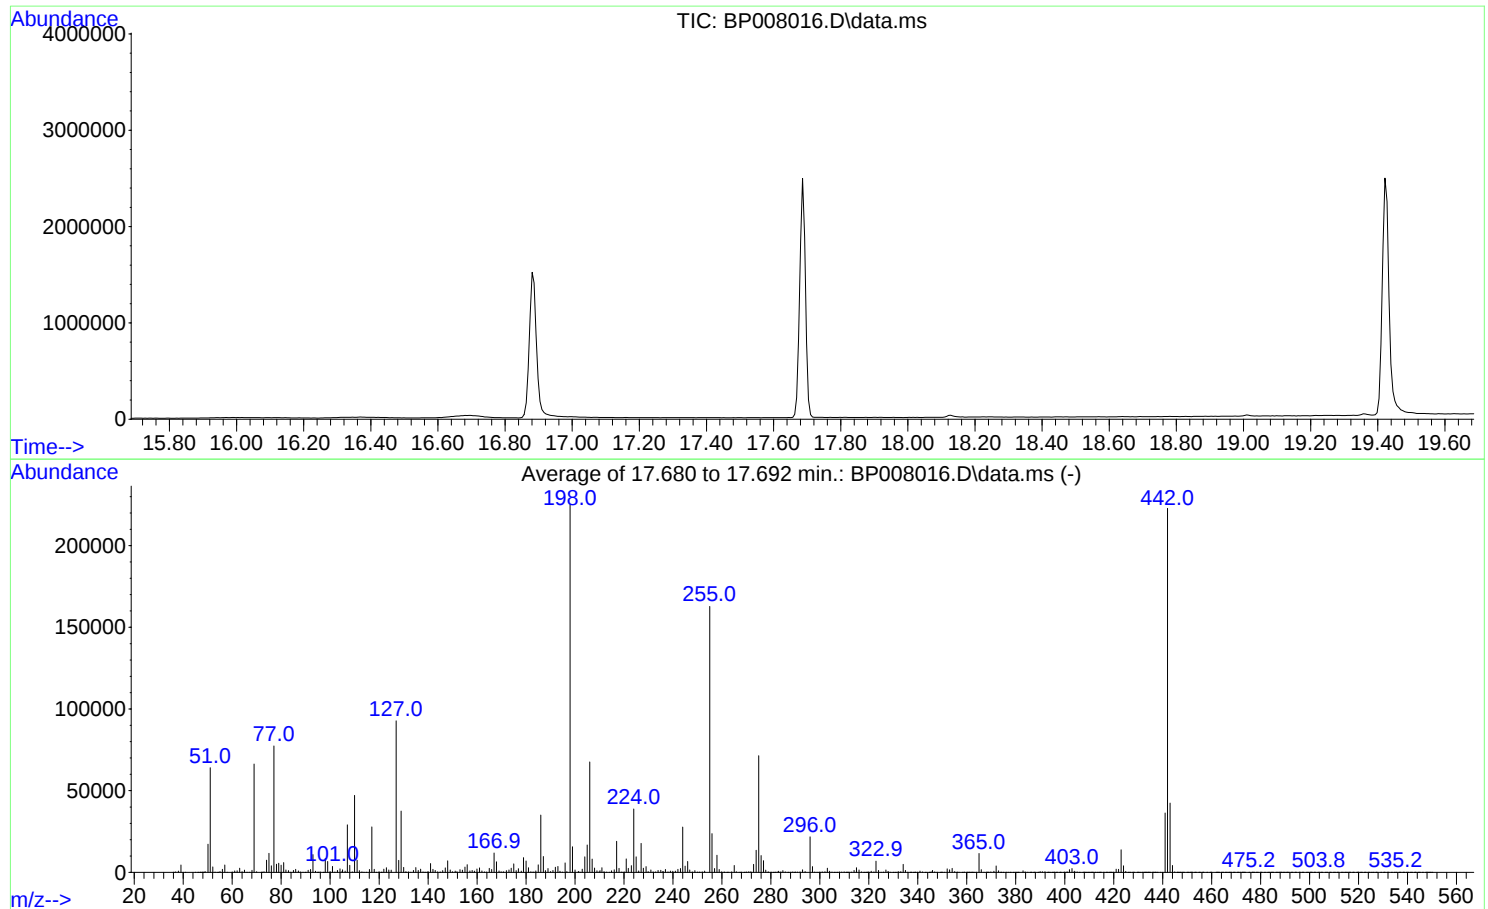




AutoFind: Scans 2447, 2448, 2449; Background Corrected with Scan 2440

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.4	64038	PASS
68	69	0.00	2	2.0	1302	PASS
69	198	0.00	100	29.5	66315	PASS
70	69	0.00	2	0.6	379	PASS
127	198	10	80	41.2	92727	PASS
197	198	0.00	2	0.2	458	PASS
198	198	100	100	100.0	225164	PASS
199	198	5	9	7.0	15702	PASS
275	198	10	60	31.7	71389	PASS
365	198	1	100	5.1	11591	PASS
441	198	0.01	100	16.1	36333	PASS
442	442	100	100	100.0	222763	PASS
443	442	15	24	19.1	42448	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111821\
 Data File : BP008016.D
 Acq On : 18 Nov 2021 14:56
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Nov 18 17:11:28 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 15 05:36:49 2021
 Response via : Initial Calibration

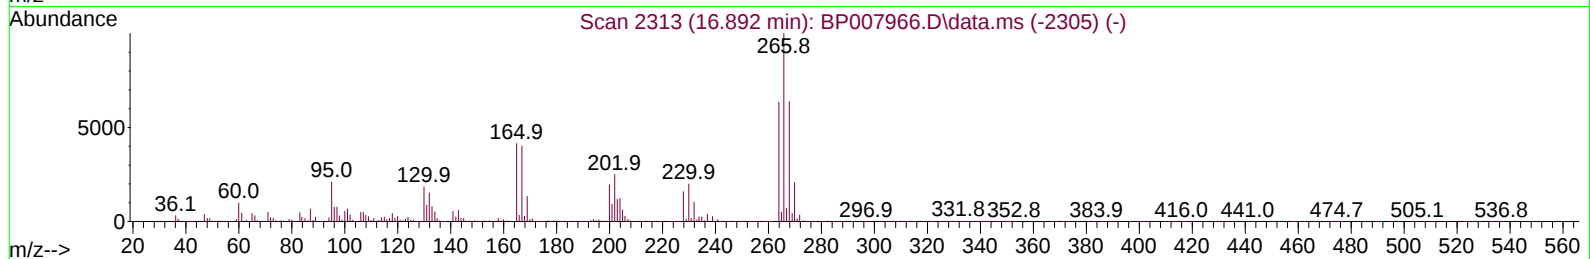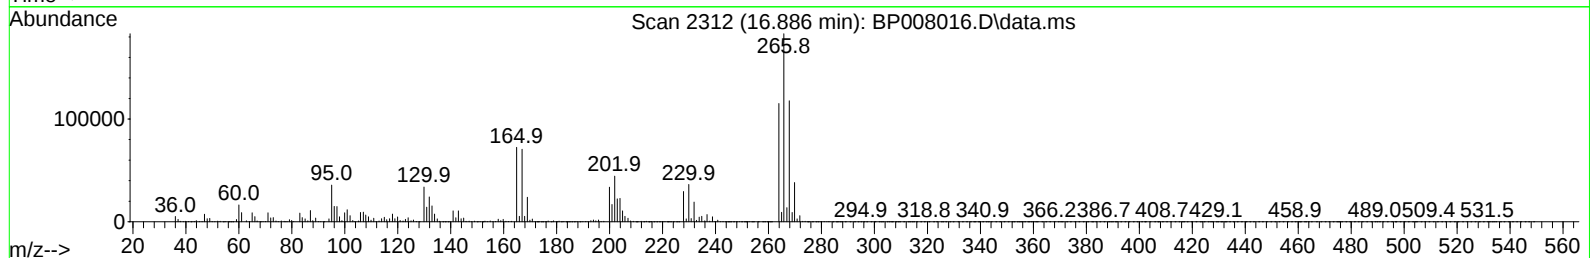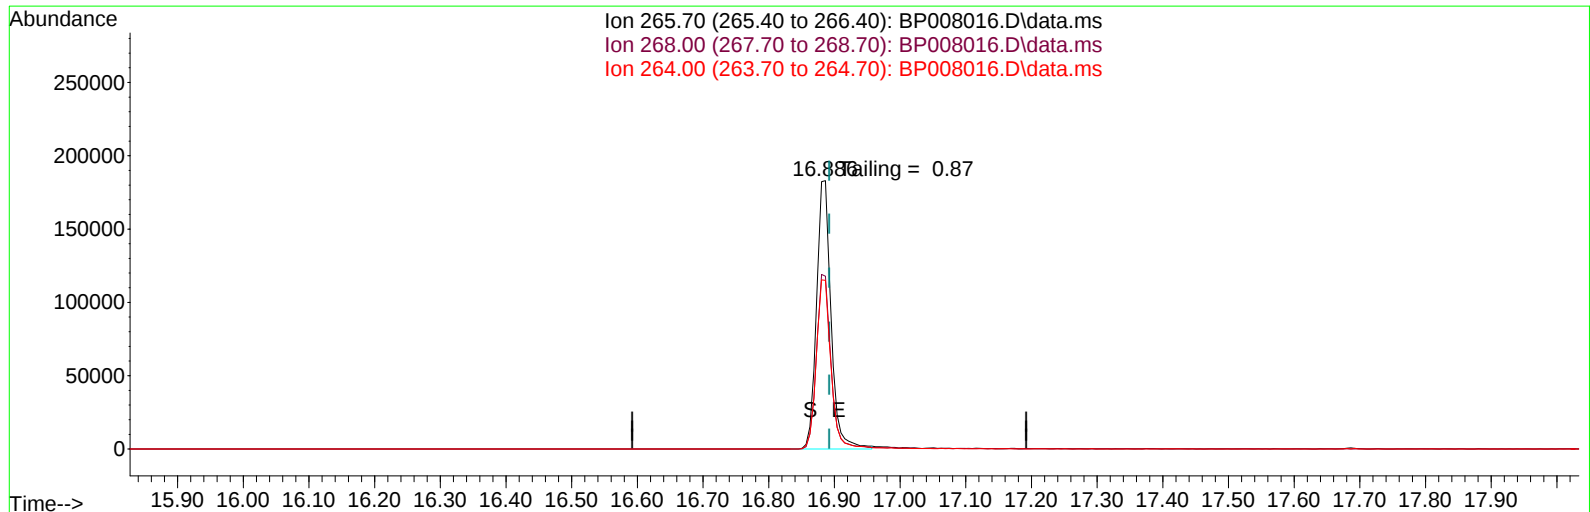

TIC: BP008016.D\data.ms

(70) Pentachlorophenol (C)

16.886min (-0.006) 2965937.09 ng




response 285883

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.60	64.38
264.00	60.90	62.85
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111821\
 Data File : BP008016.D
 Acq On : 18 Nov 2021 14:56
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Nov 18 17:11:28 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 15 05:36:49 2021
 Response via : Initial Calibration

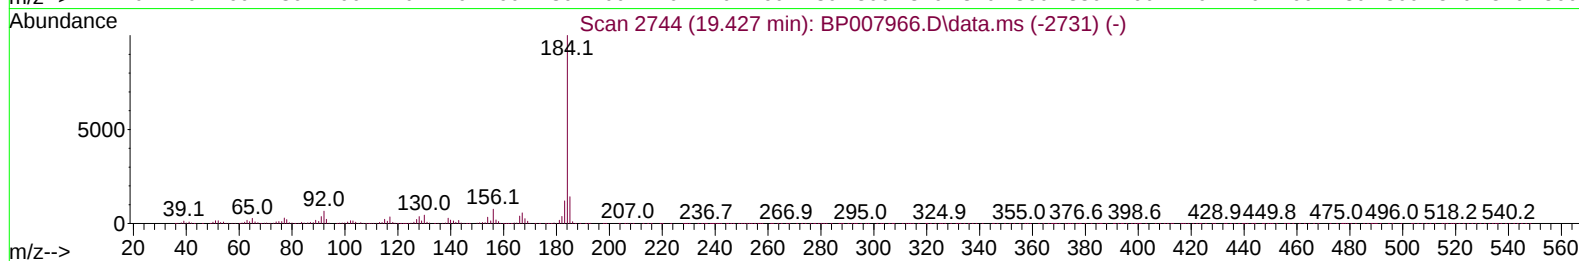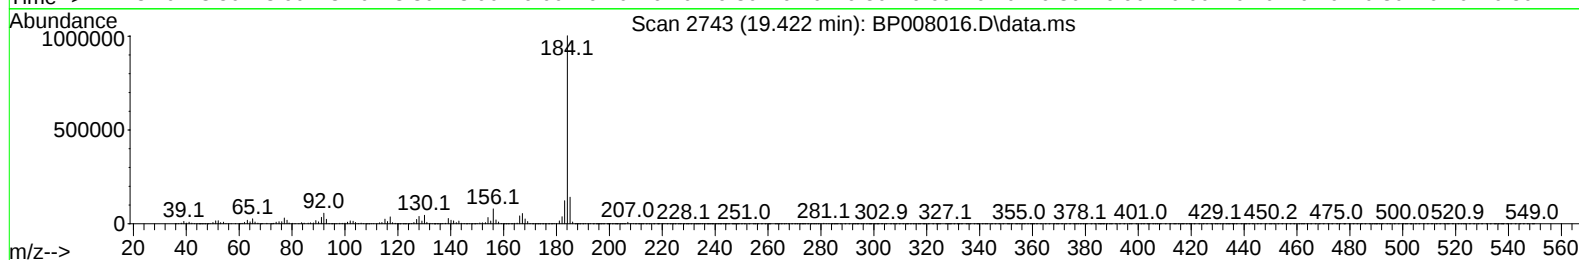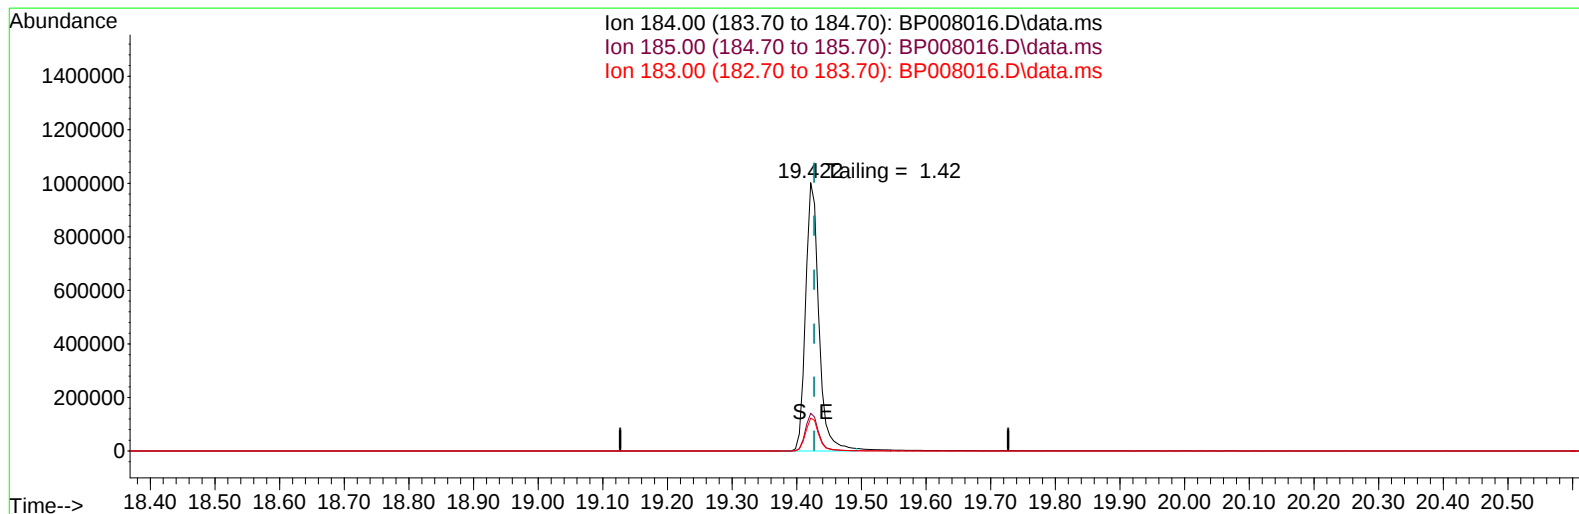

TIC: BP008016.D\data.ms

(77) Benzidine

19.422min (-0.005) 1719539.09 ng

response 1451090

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	14.09
183.00	11.40	12.29
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/18/2021	BNA_P	<u>BP008016.D</u>
Compound Name	Response	Retention Time
DDT	931292	20.63
DDD	6362	20.19
DDE	1218	19.71
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7580	938872	0.81

Instrument :
BNA_P
ClientSampleId :
DFTPP