
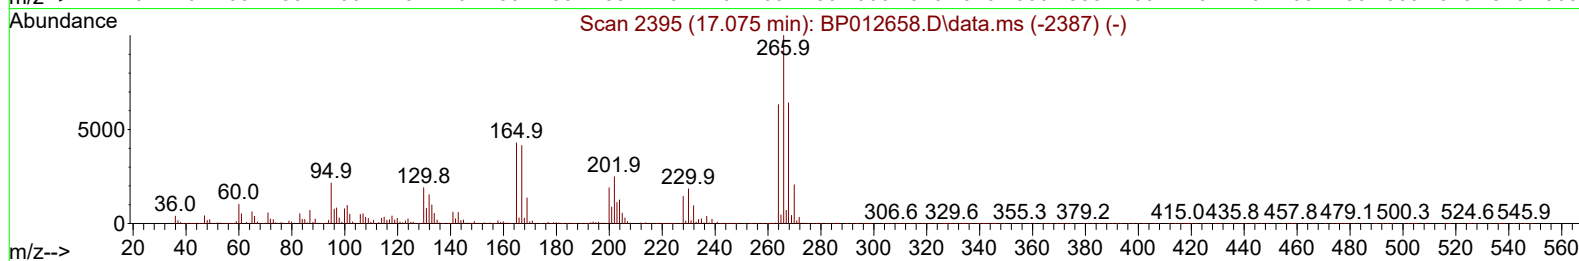
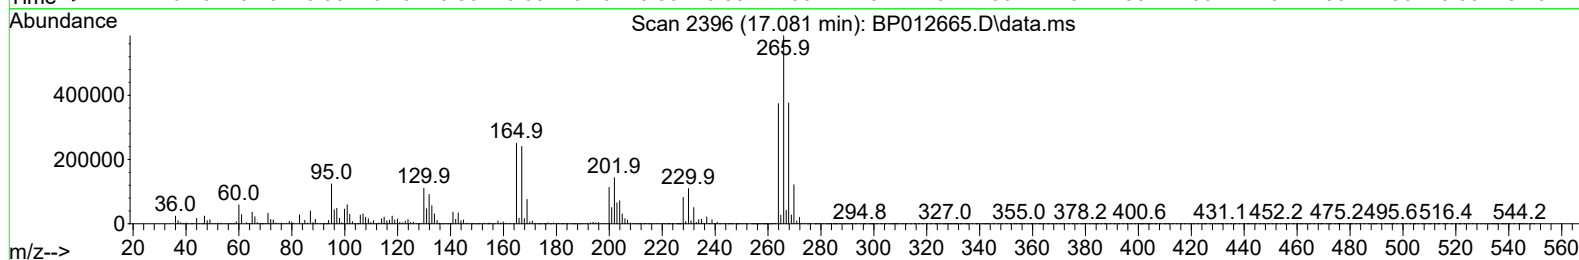


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111822\
Data File : BP012665.D
Acq On : 18 Nov 2022 08:41
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 19 05:08:32 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 18 00:16:03 2022
Response via : Initial Calibration

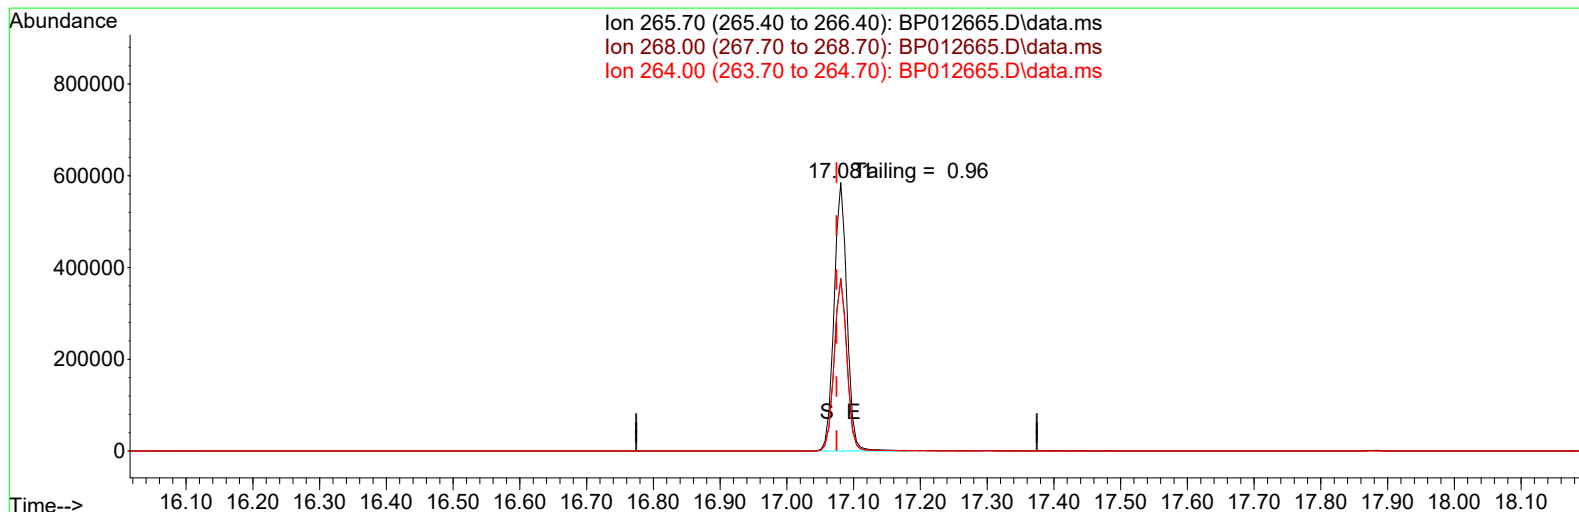

TIC: BP012665.D\data.ms

(70) Pentachlorophenol (C)




17.081min (+ 0.006) 1586025.42 ng

response 786430

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.20	64.26
264.00	63.20	63.93
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111822\
 Data File : BP012665.D
 Acq On : 18 Nov 2022 08:41
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 19 05:08:32 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 18 00:16:03 2022
 Response via : Initial Calibration

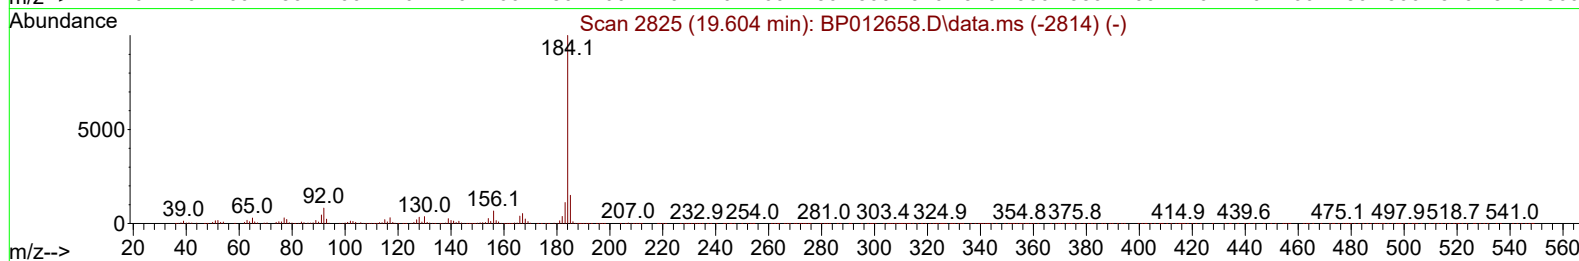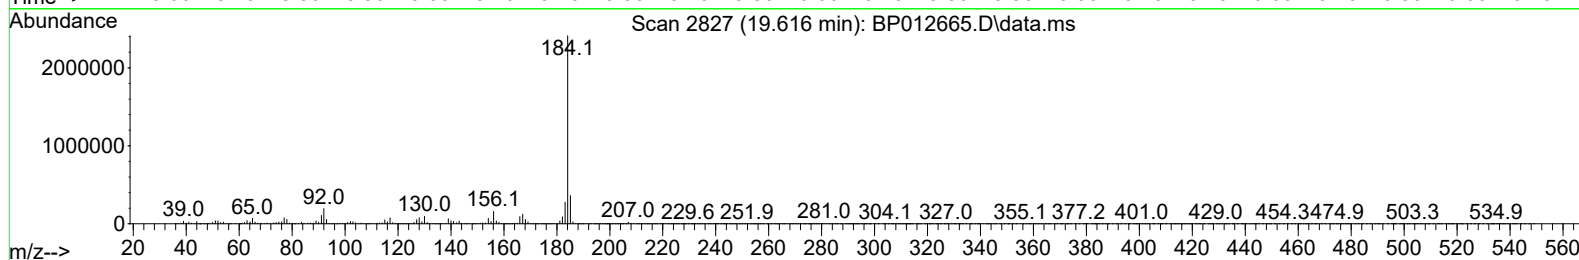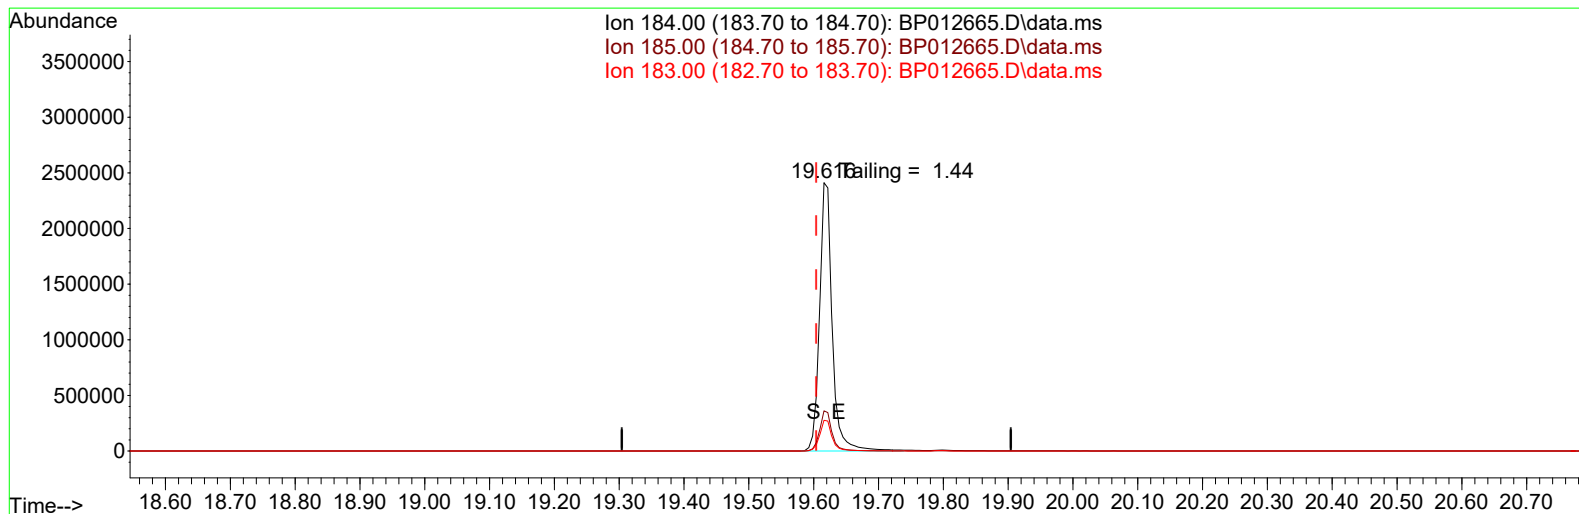

TIC: BP012665.D\data.ms

(77) Benzidine**19.616min (+ 0.012) 21388.77 ng****response 3299932**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.97
183.00	11.20	11.45
0.00	0.00	0.00