
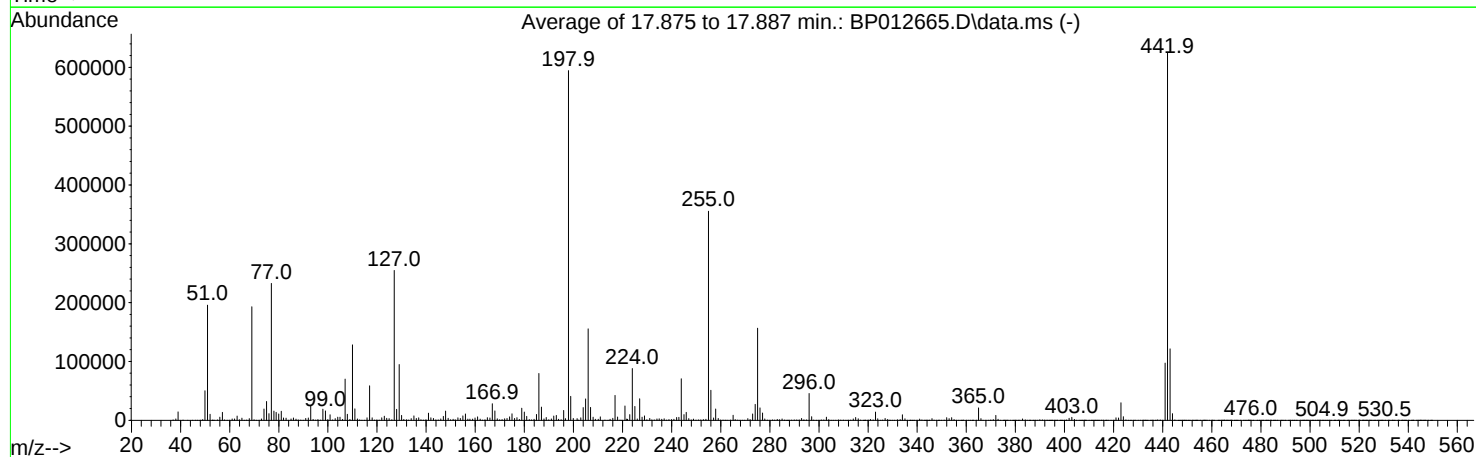


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111822\
 Data File : BP012665.D
 Acq On : 18 Nov 2022 08:41
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Nov 18 00:16:03 2022

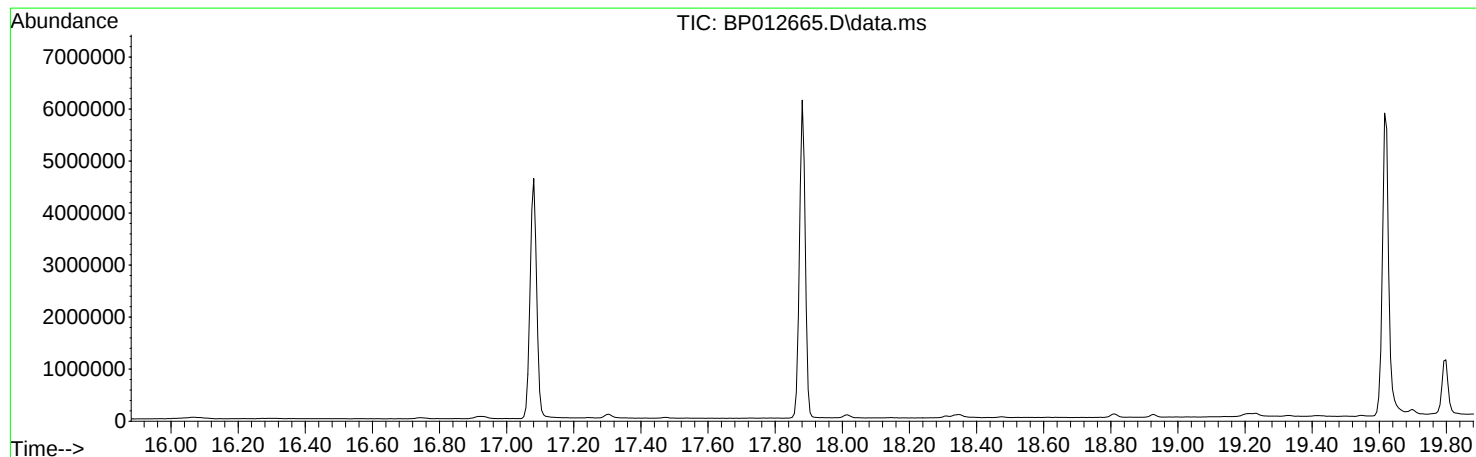




AutoFind: Scans 2531, 2532, 2533; Background Corrected with Scan 2522

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.9	195677	PASS
68	69	0.00	2	1.5	2859	PASS
69	198	0.00	100	32.5	193094	PASS
70	69	0.00	2	0.4	837	PASS
127	198	10	80	42.8	254763	PASS
197	198	0.00	2	0.5	2755	PASS
198	198	100	100	100.0	594553	PASS
199	198	5	9	6.8	40624	PASS
275	198	10	60	26.3	156592	PASS
365	198	1	100	3.5	21103	PASS
441	198	0.01	100	16.4	97267	PASS
442	442	100	100	100.0	625401	PASS
443	442	15	24	19.4	121397	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111822\
Data File : BP012665.D
Acq On : 18 Nov 2022 08:41
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Nov 19 05:08:32 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 18 00:16:03 2022
Response via : Initial Calibration

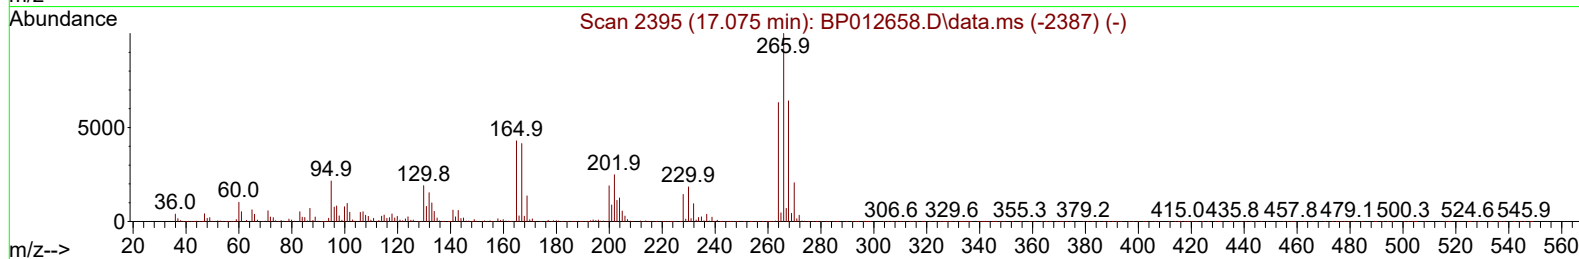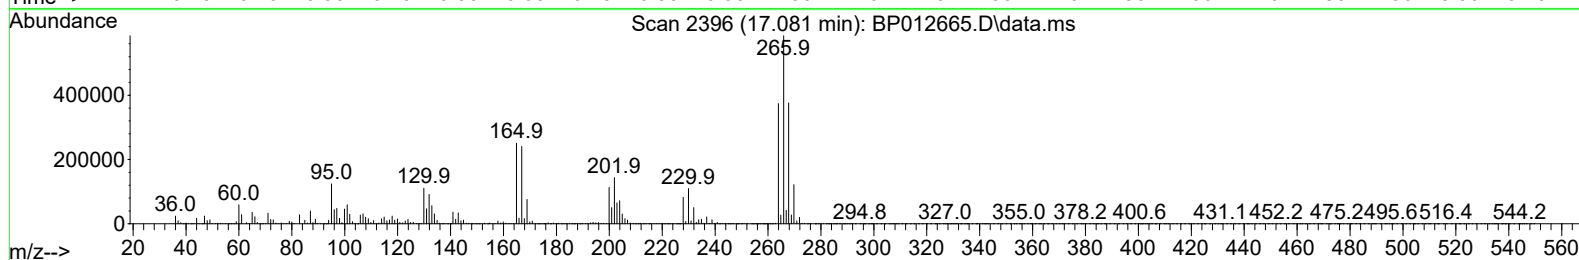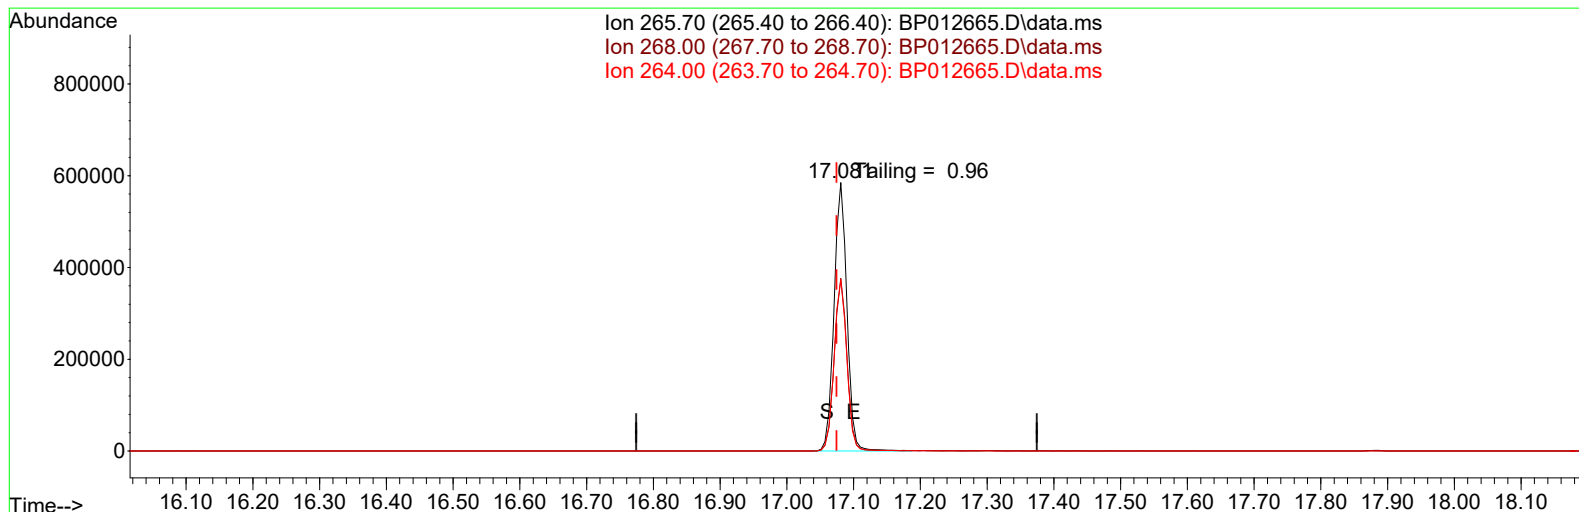

TIC: BP012665.D\data.ms

(70) Pentachlorophenol (C)

17.081min (+ 0.006) 1586025.42 ng




response 786430

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.20	64.26
264.00	63.20	63.93
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111822\
 Data File : BP012665.D
 Acq On : 18 Nov 2022 08:41
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Nov 19 05:08:32 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 18 00:16:03 2022
 Response via : Initial Calibration

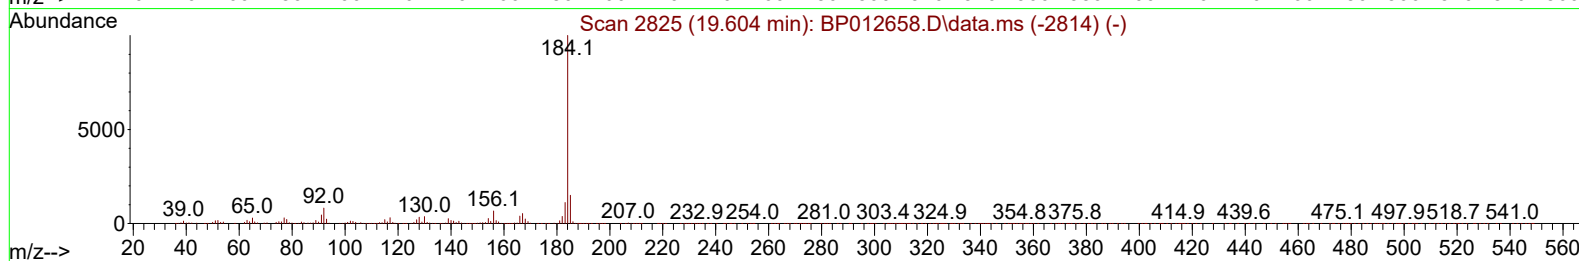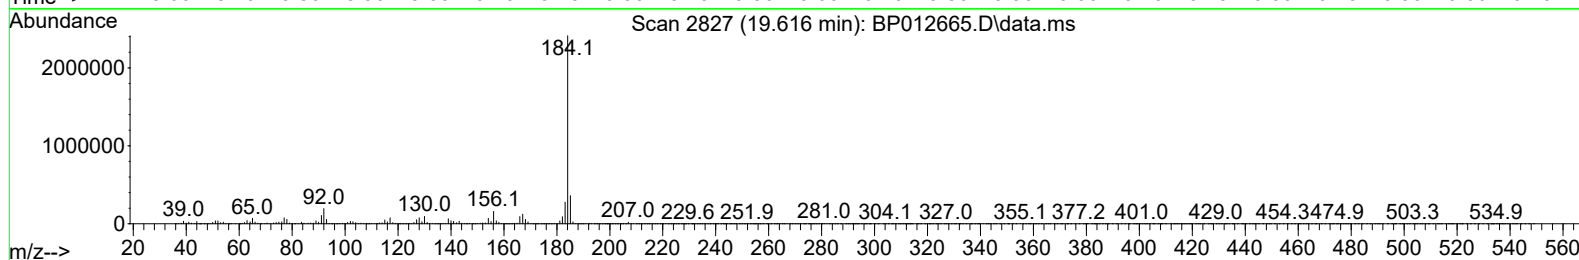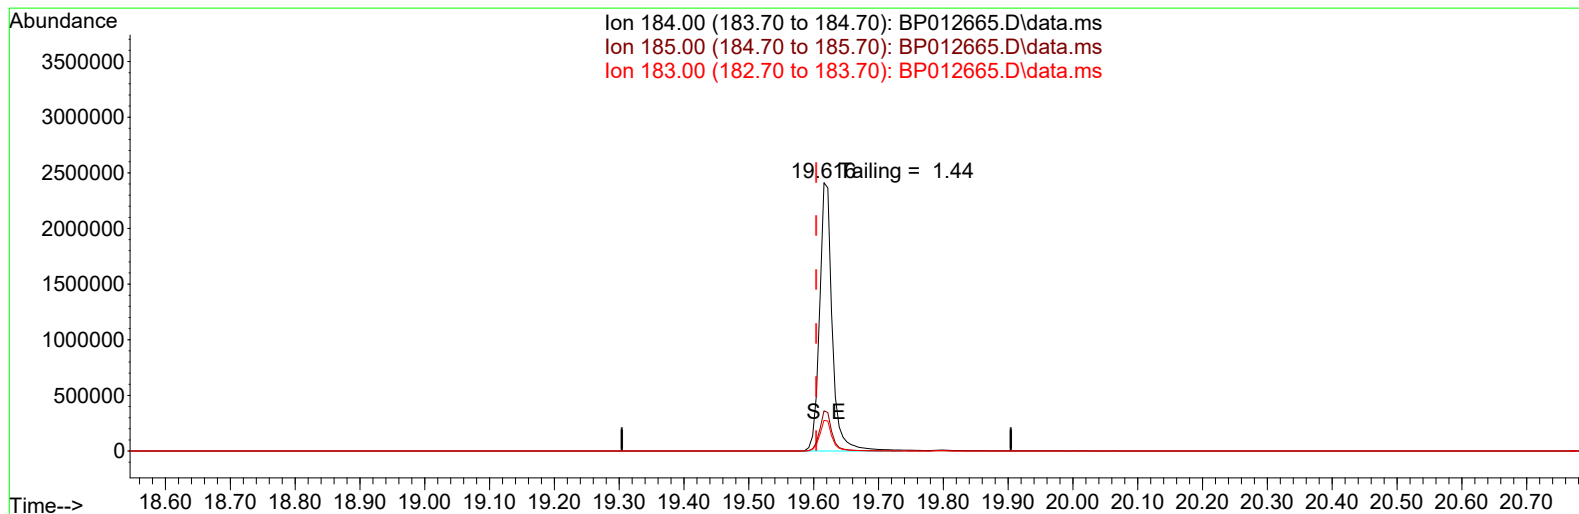

TIC: BP012665.D\data.ms

(77) Benzidine

19.616min (+ 0.012) 21388.77 ng

response 3299932

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.97
183.00	11.20	11.45
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/18/2022	BNA_P	<u>BP012665.D</u>
Compound Name	Response	Retention Time
DDT	1399302	20.822
DDD	26771	20.386
DDE	2227	19.892
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
28998	1428300	2.03

Instrument :
BNA_P
ClientSampleId :
DFTPP