




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111824\
Data File : BP023204.D
Acq On : 18 Nov 2024 19:24
Operator : RC/JU
Sample : P4882-14
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BG3J1

Manual IntegrationsAPPROVED

Quant Time: Nov 18 23:58:32 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 13 04:49:01 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/19/2024
Supervised By :mohammad ahmed 11/19/2024

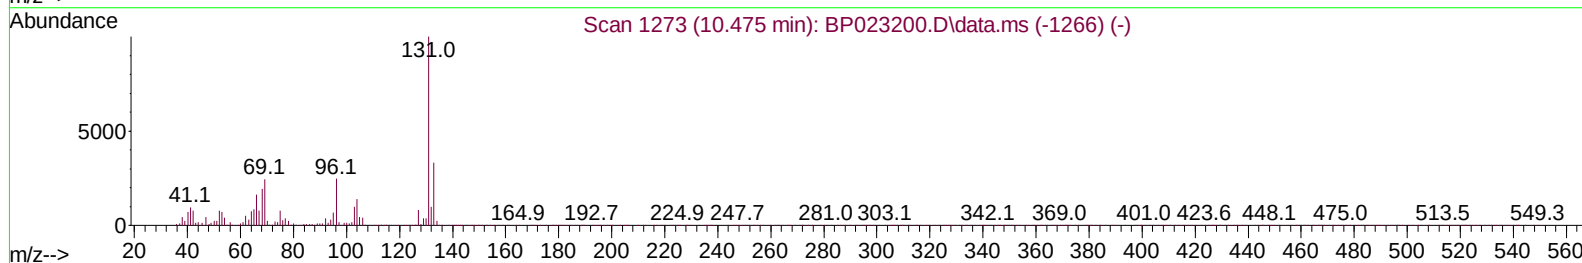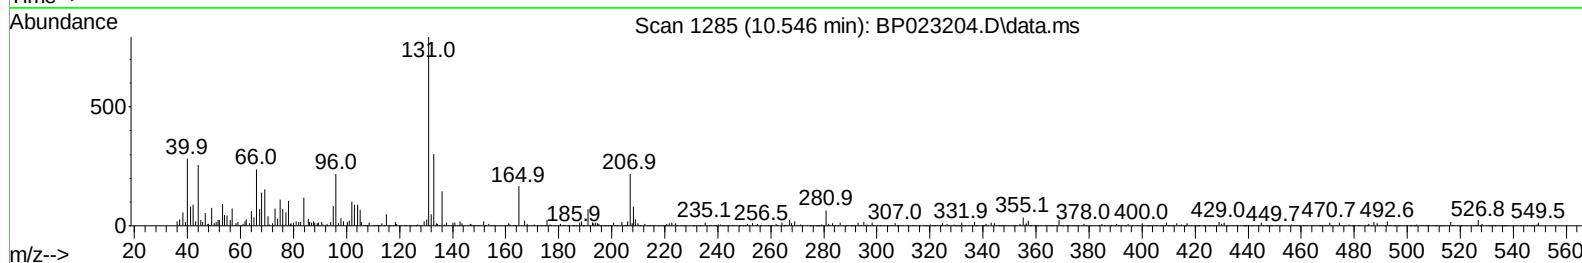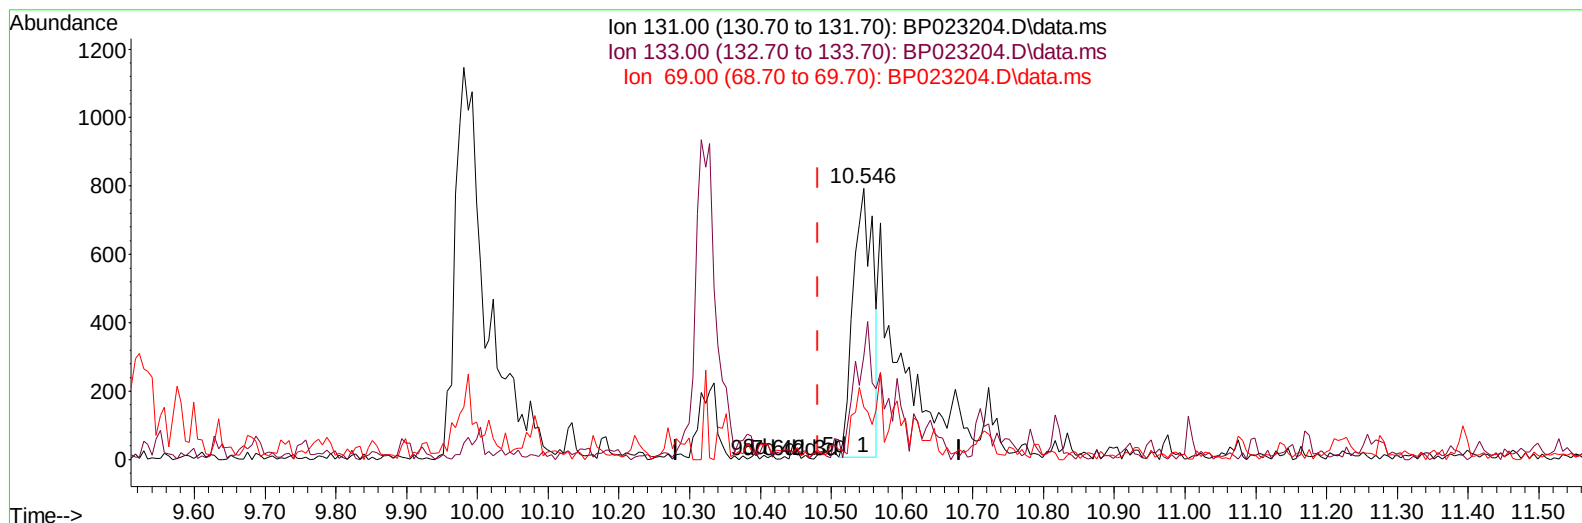

TIC: BP023204.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.546min (+ 0.065) 0.32 ng/u1

response 1540

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	33.90	38.04
69.00	23.10	19.40
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111824\
 Data File : BP023204.D
 Acq On : 18 Nov 2024 19:24
 Operator : RC/JU
 Sample : P4882-14
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BG3J1

Manual IntegrationsAPPROVED

Quant Time: Nov 18 23:58:32 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 13 04:49:01 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/19/2024
 Supervised By :mohammad ahmed 11/19/2024

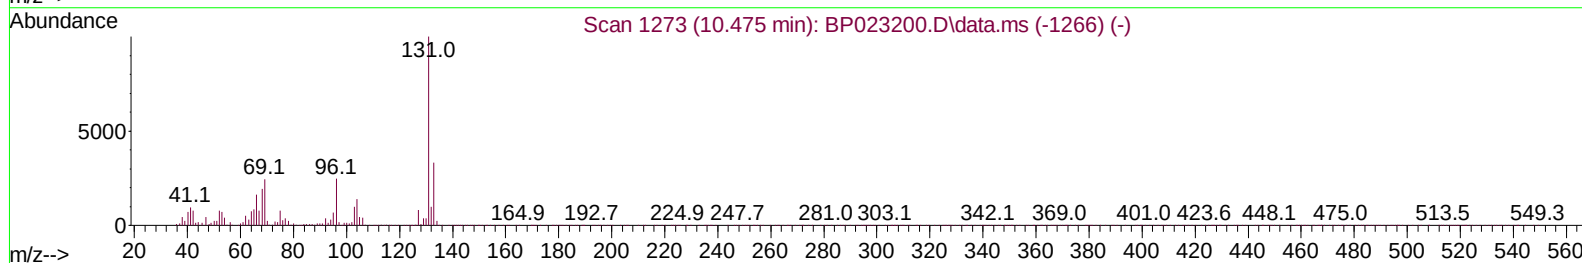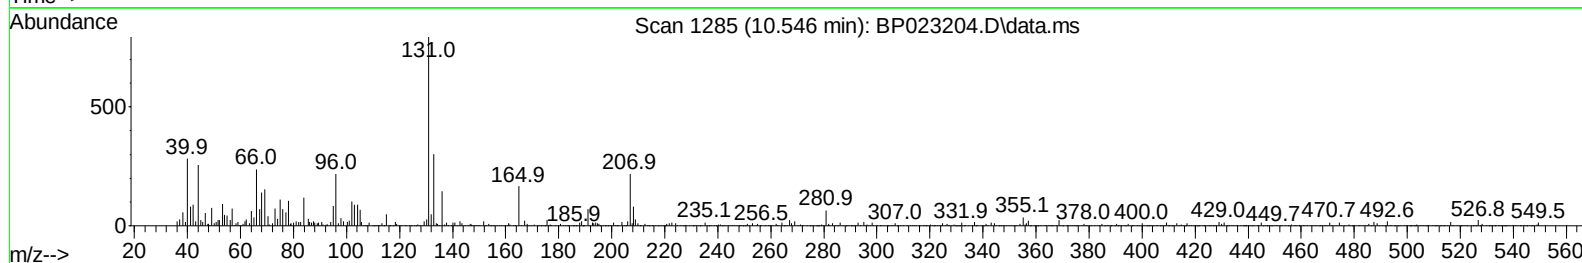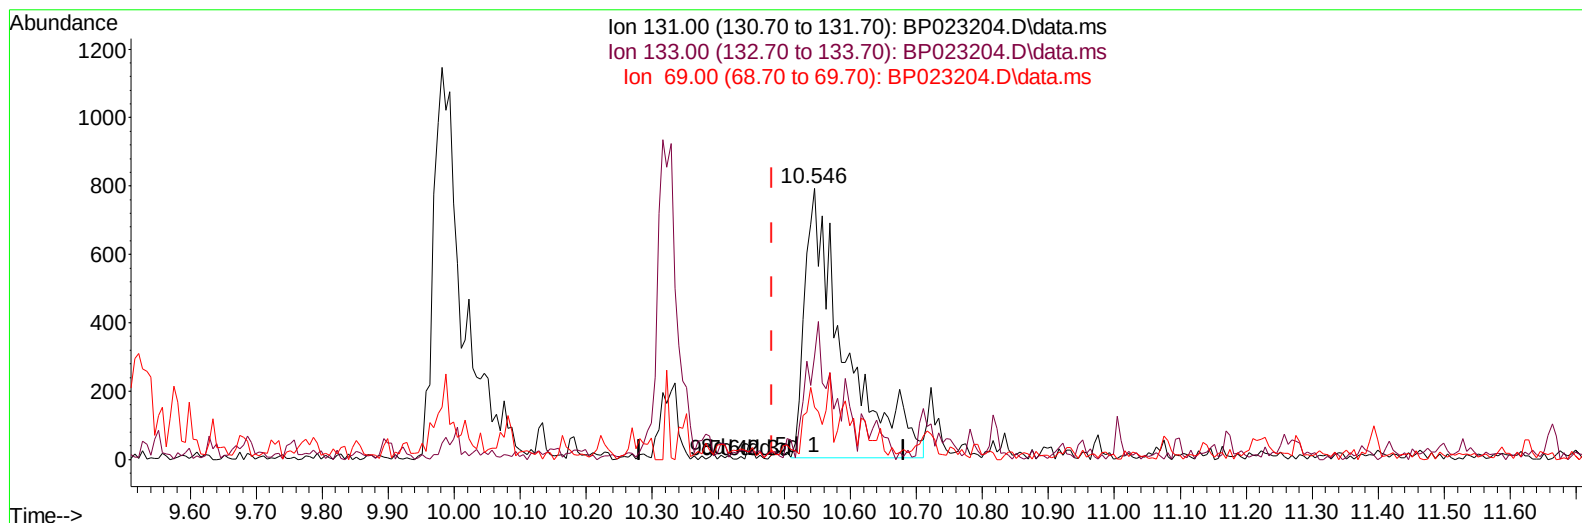

TIC: BP023204.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.546min (+ 0.065) 0.68 ng/ul m

response 3266

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	33.90	38.04
69.00	23.10	19.40
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111824\
Data File : BP023204.D
Acq On : 18 Nov 2024 19:24
Operator : RC/JU
Sample : P4882-14
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BG3J1

Manual IntegrationsAPPROVED

Quant Time: Nov 18 23:58:32 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 13 04:49:01 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/19/2024
Supervised By :mohammad ahmed 11/19/2024

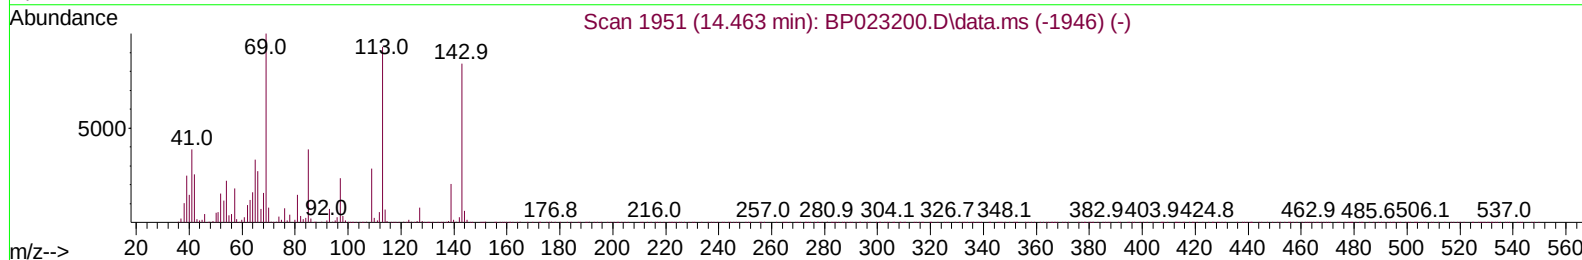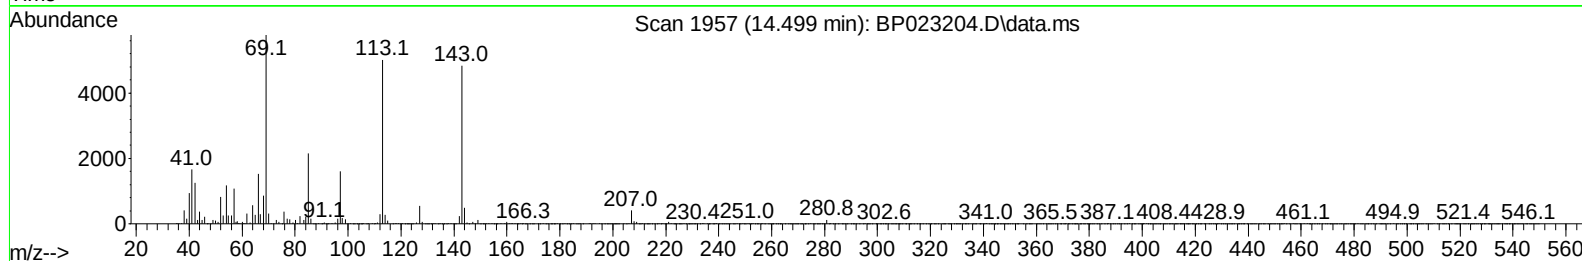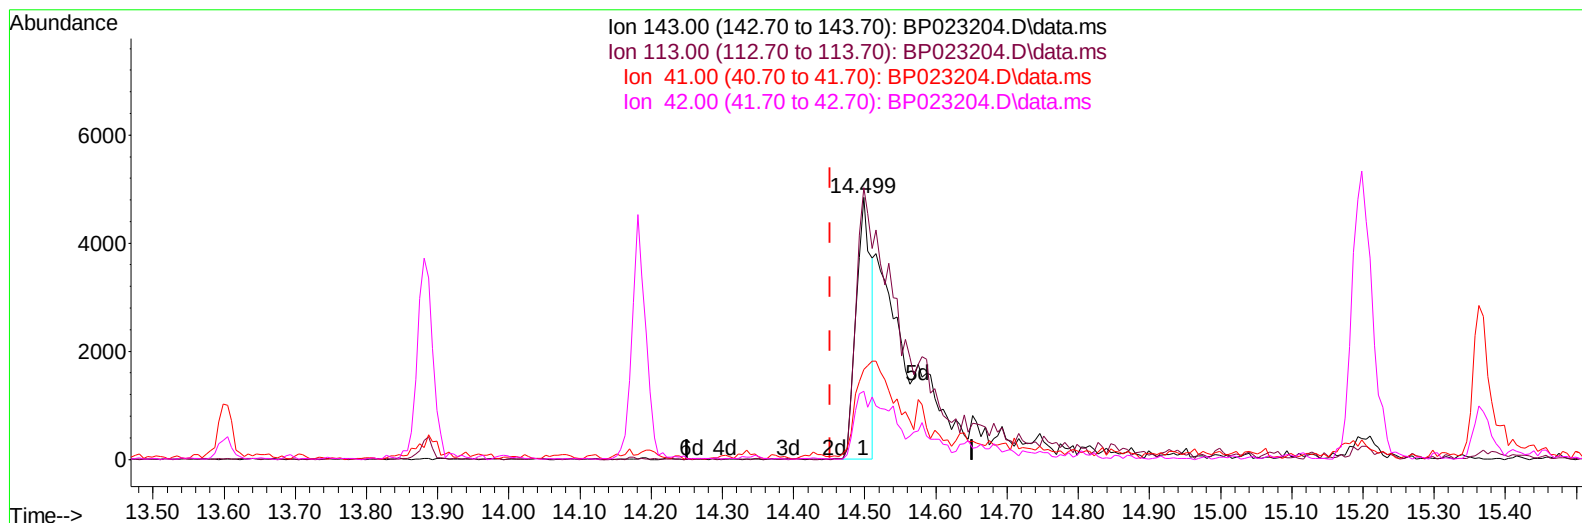

TIC: BP023204.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.499min (+ 0.047) 3.56 ng/ul

response 7107

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	107.90	103.70
41.00	39.20	34.26
42.00	25.90	26.04




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111824\
Data File : BP023204.D
Acq On : 18 Nov 2024 19:24
Operator : RC/JU
Sample : P4882-14
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BG3J1

Manual IntegrationsAPPROVED

Quant Time: Nov 18 23:58:32 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 13 04:49:01 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/19/2024
Supervised By :mohammad ahmed 11/19/2024

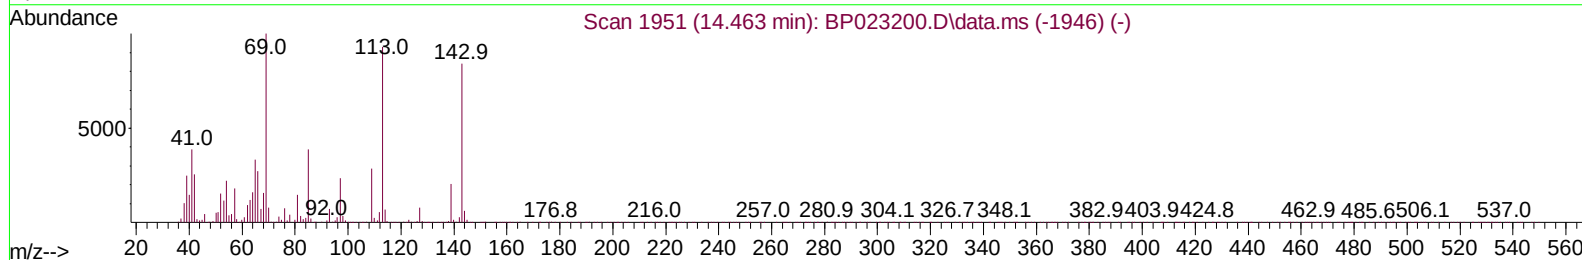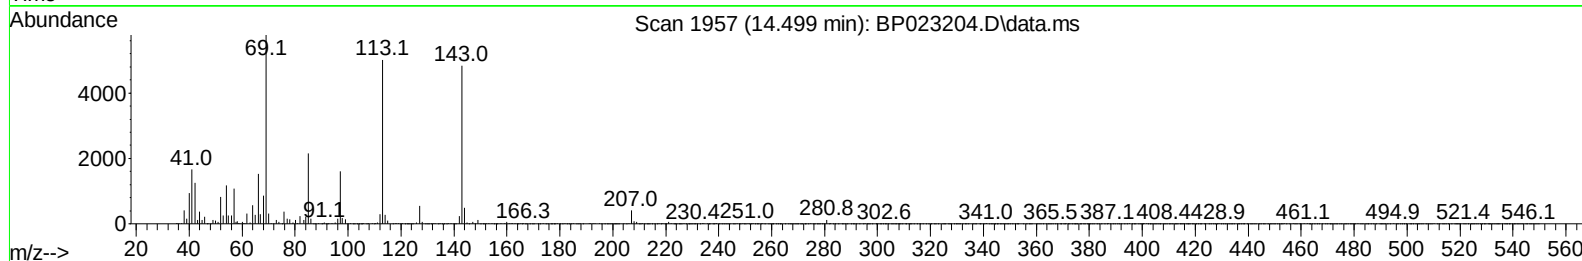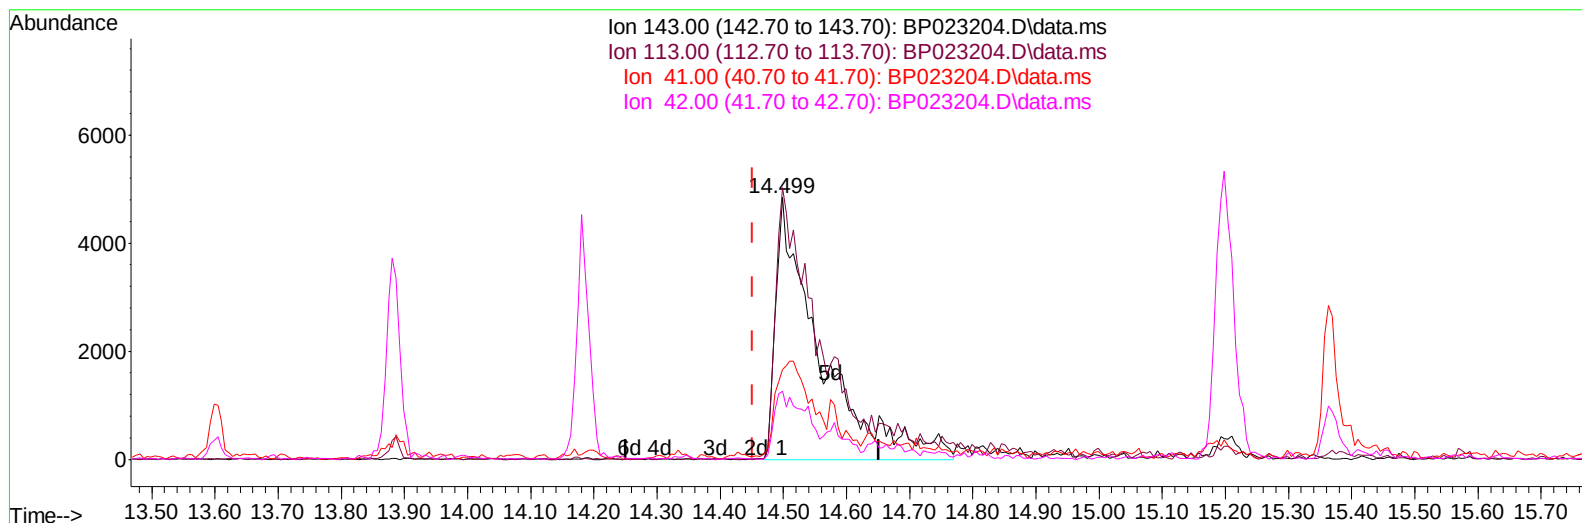

TIC: BP023204.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.499min (+ 0.047) 11.83 ng/ul m

response 23581

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	107.90	103.70
41.00	39.20	34.26
42.00	25.90	26.04

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111824\
 Data File : BP023204.D
 Acq On : 18 Nov 2024 19:24
 Operator : RC/JU
 Sample : P4882-14
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BG3J1

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/19/2024
 Supervised By :mohammad ahmed 11/19/2024

Quant Time: Nov 19 00:01:57 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 13 04:49:01 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.575	152	59758	20.000	ng/ul	0.00
20) Naphthalene-d8	10.322	136	230160	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.181	164	184093	20.000	ng/ul	-0.02
64) Phenanthrene-d10	16.992	188	469391	20.000	ng/ul	-0.02
79) Chrysene-d12	21.433	240	527246	20.000	ng/ul	-0.01
88) Perylene-d12	24.651	264	637934	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.134	96	6691	5.382	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.000	ng/ul	
7) Phenol-d5	6.787	99	53337	12.072	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.922	67	76441	29.449	ng/ul	0.00
11) 2-Chlorophenol-d4	7.122	132	94464	29.194	ng/ul	0.00
15) 4-Methylphenol-d8	8.293	113	86815	23.879	ng/ul	0.00
21) Nitrobenzene-d5	8.716	128	47421	29.595	ng/ul	0.00
24) 2-Nitrophenol-d4	9.428	143	55606	29.109	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.981	165	111415	27.851	ng/ul	0.01
31) 4-Chloroaniline-d4	10.546	131	3266m	0.684	ng/ul	0.06
46) Dimethylphthalate-d6	13.604	166	426682	32.158	ng/ul	0.00
49) Acenaphthylene-d8	13.881	160	385185	27.823	ng/ul	-0.02
54) 4-Nitrophenol-d4	14.499	143	23581m	11.826	ng/ul	0.05
60) Fluorene-d10	15.198	176	373915	32.143	ng/ul	-0.01
65) 4,6-Dinitro-2-methylph...	15.369	200	73647	26.191	ng/ul	0.00
73) Anthracene-d10	17.104	188	674697	33.948	ng/ul	-0.01
81) Pyrene-d10	19.486	212	865806	35.651	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.427	264	1023223	33.673	ng/ul	-0.02

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111824\
Data File : BP023204.D
Acq On : 18 Nov 2024 19:24
Operator : RC/JU
Sample : P4882-14
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BG3J1

Manual IntegrationsAPPROVED

Quant Time: Nov 19 00:01:57 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 13 04:49:01 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/19/2024
Supervised By :mohammad ahmed 11/19/2024

