




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111824\
Data File : BP023205.D
Acq On : 18 Nov 2024 20:04
Operator : RC/JU
Sample : P4884-01
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BG3M5

Manual IntegrationsAPPROVED

Quant Time: Nov 19 00:04:24 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 13 04:49:01 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/19/2024
Supervised By :mohammad ahmed 11/19/2024

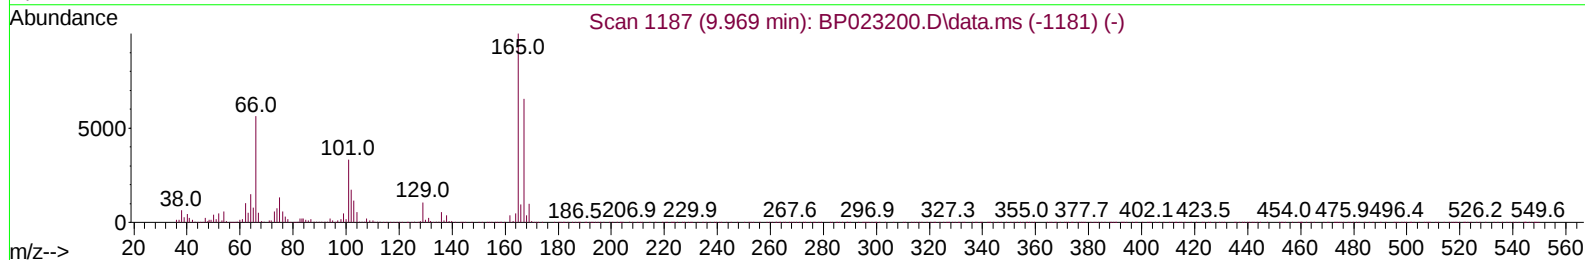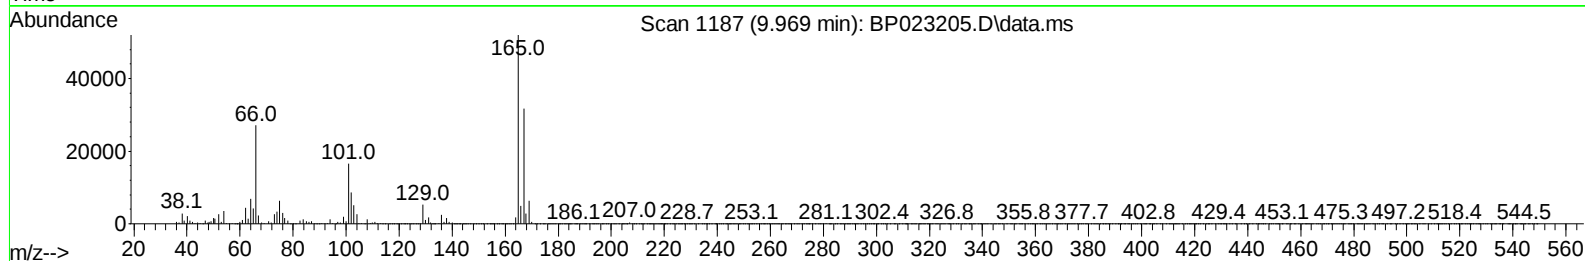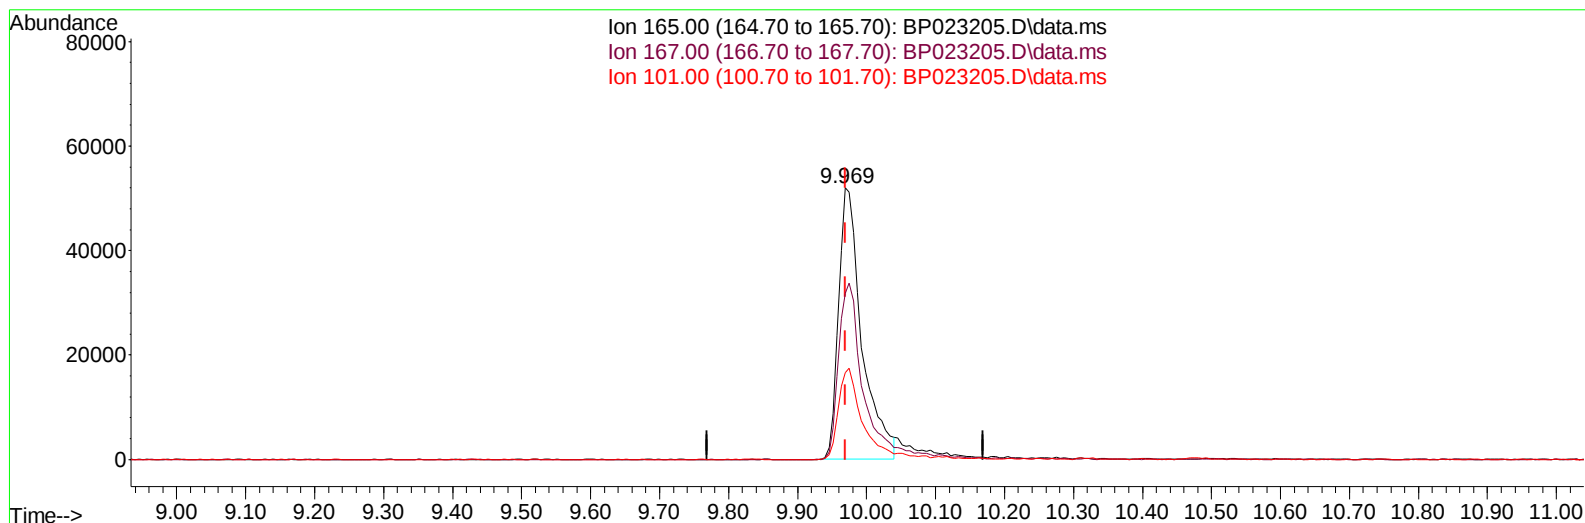

TIC: BP023205.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

9.969min (-0.000) 30.36 ng/u1

response 121834

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	65.80	61.18
101.00	32.60	32.04
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111824\
Data File : BP023205.D
Acq On : 18 Nov 2024 20:04
Operator : RC/JU
Sample : P4884-01
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BG3M5

Manual IntegrationsAPPROVED

Quant Time: Nov 19 00:04:24 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 13 04:49:01 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/19/2024
Supervised By :mohammad ahmed 11/19/2024

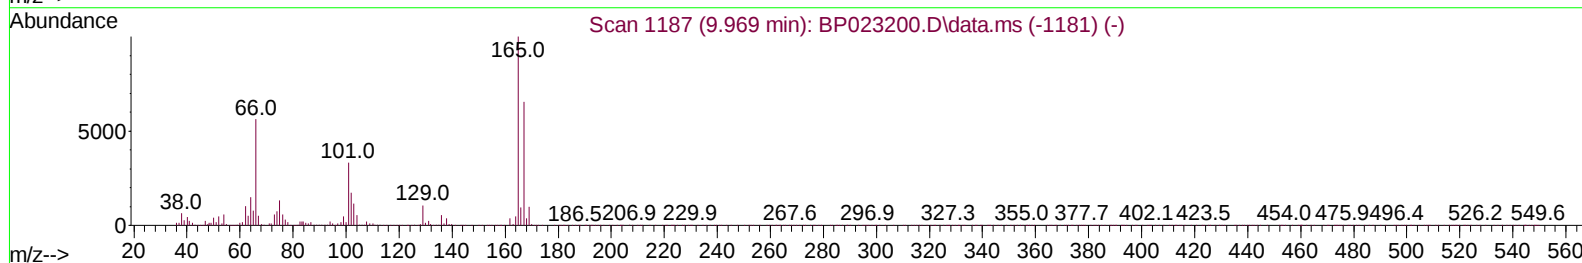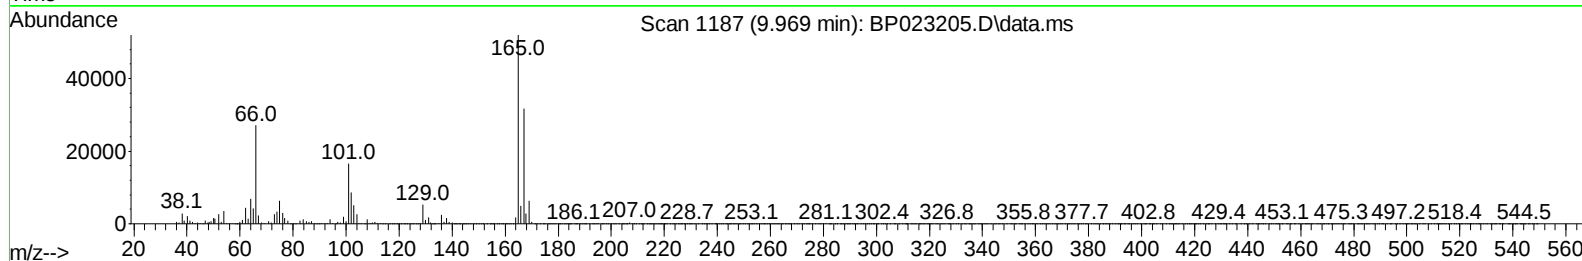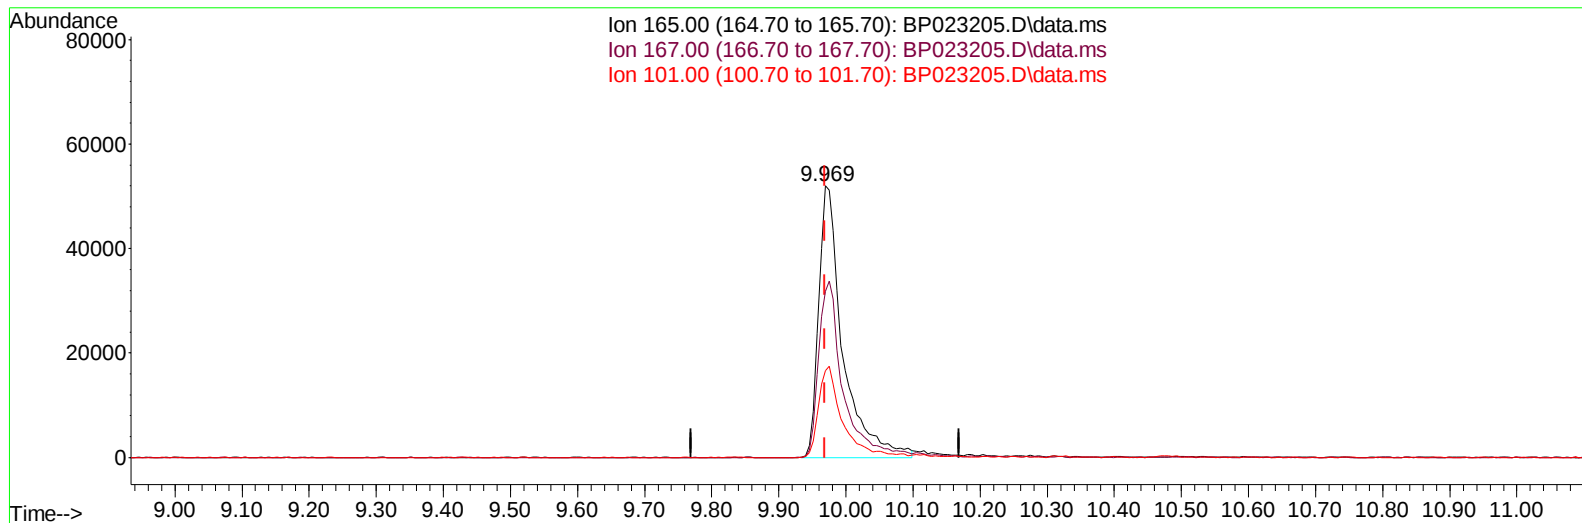

TIC: BP023205.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

9.969min (-0.000) 32.40 ng/u1 m

response 129990

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	65.80	61.18
101.00	32.60	32.04
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111824\
Data File : BP023205.D
Acq On : 18 Nov 2024 20:04
Operator : RC/JU
Sample : P4884-01
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BG3M5

Manual IntegrationsAPPROVED

Quant Time: Nov 19 00:04:24 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 13 04:49:01 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/19/2024
Supervised By :mohammad ahmed 11/19/2024

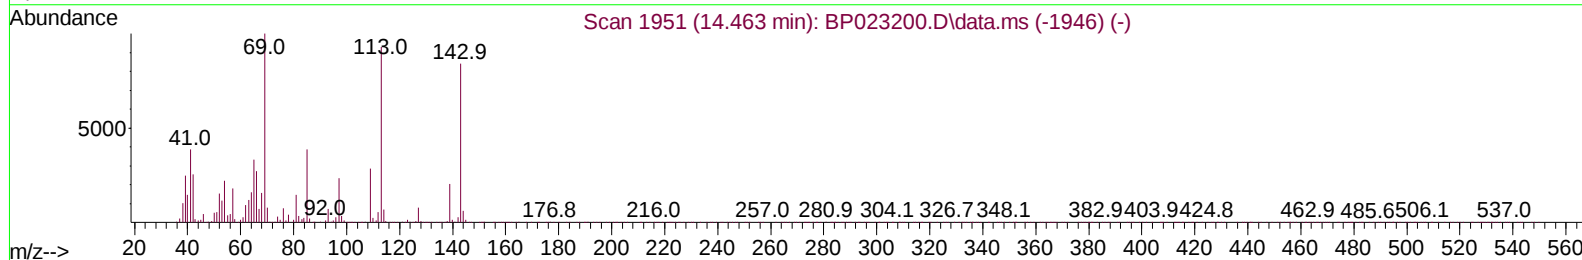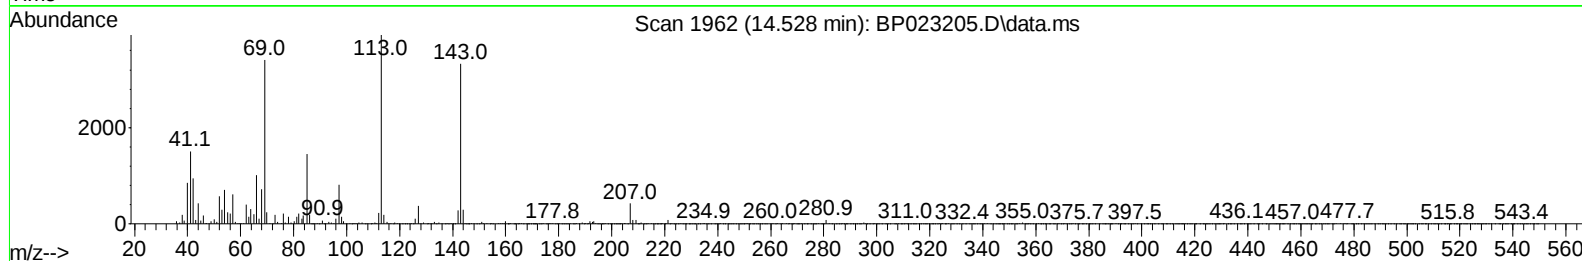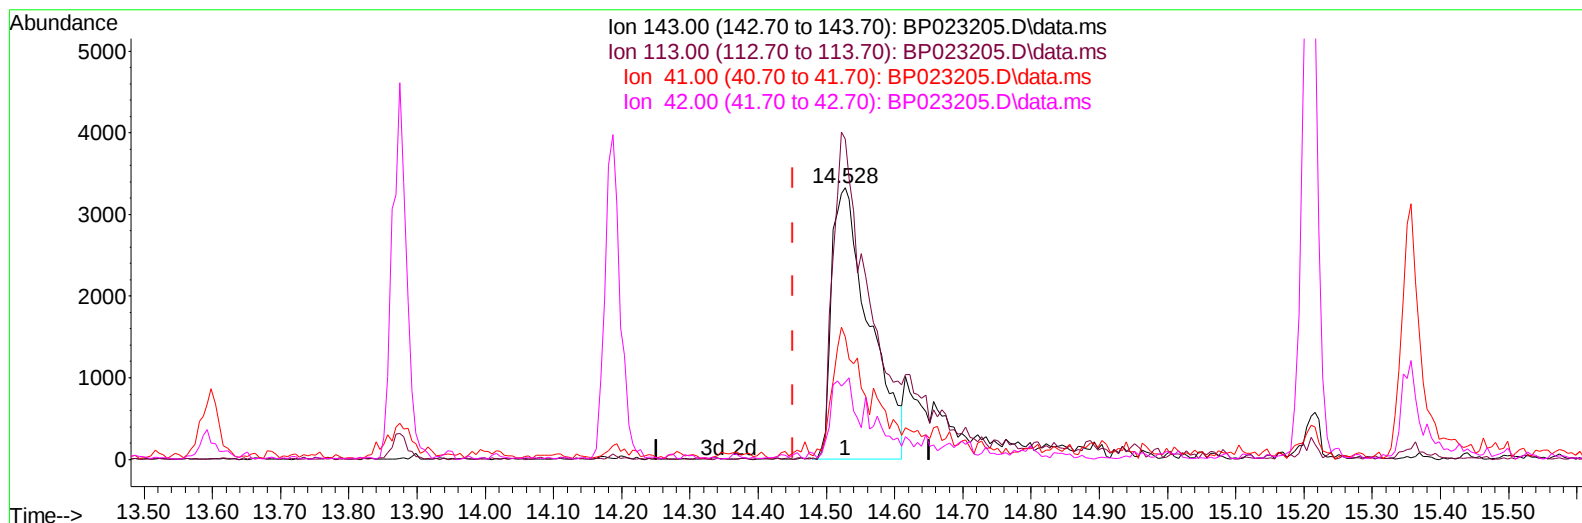

TIC: BP023205.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.528min (+ 0.076) 6.51 ng/ul

response 12673

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	107.90	118.01
41.00	39.20	45.22
42.00	25.90	28.32




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111824\
Data File : BP023205.D
Acq On : 18 Nov 2024 20:04
Operator : RC/JU
Sample : P4884-01
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BG3M5

Manual IntegrationsAPPROVED

Quant Time: Nov 19 00:04:24 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 13 04:49:01 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/19/2024
Supervised By :mohammad ahmed 11/19/2024

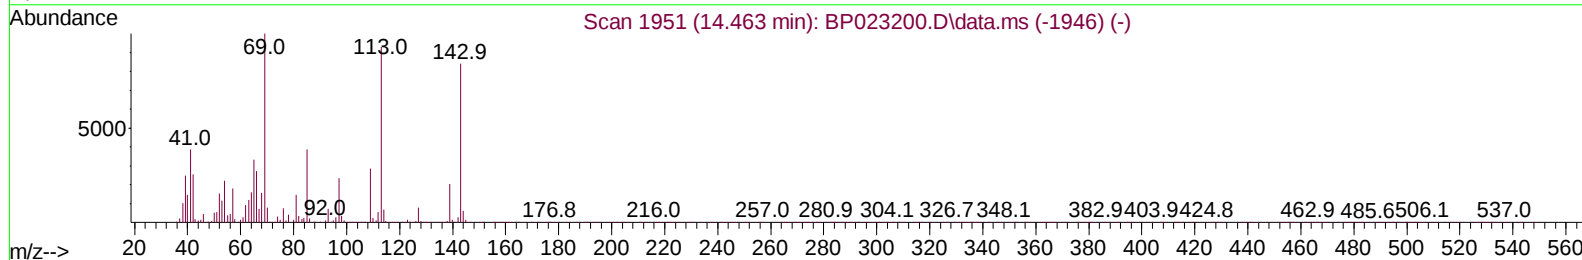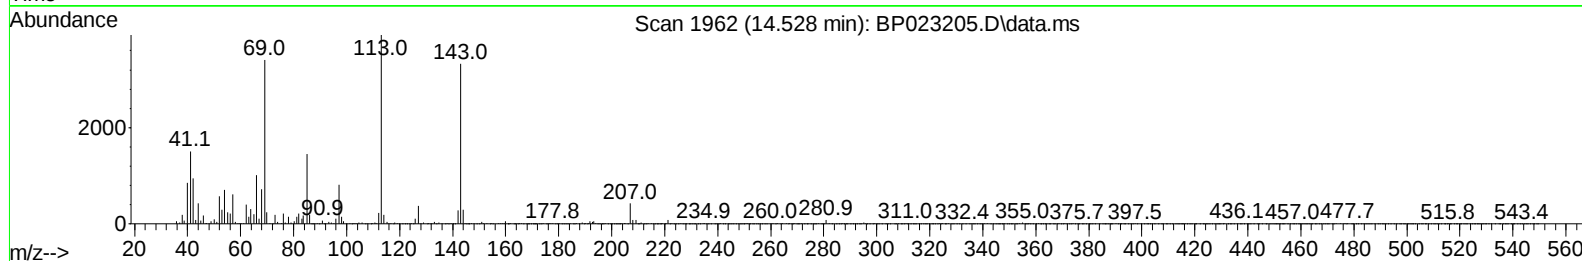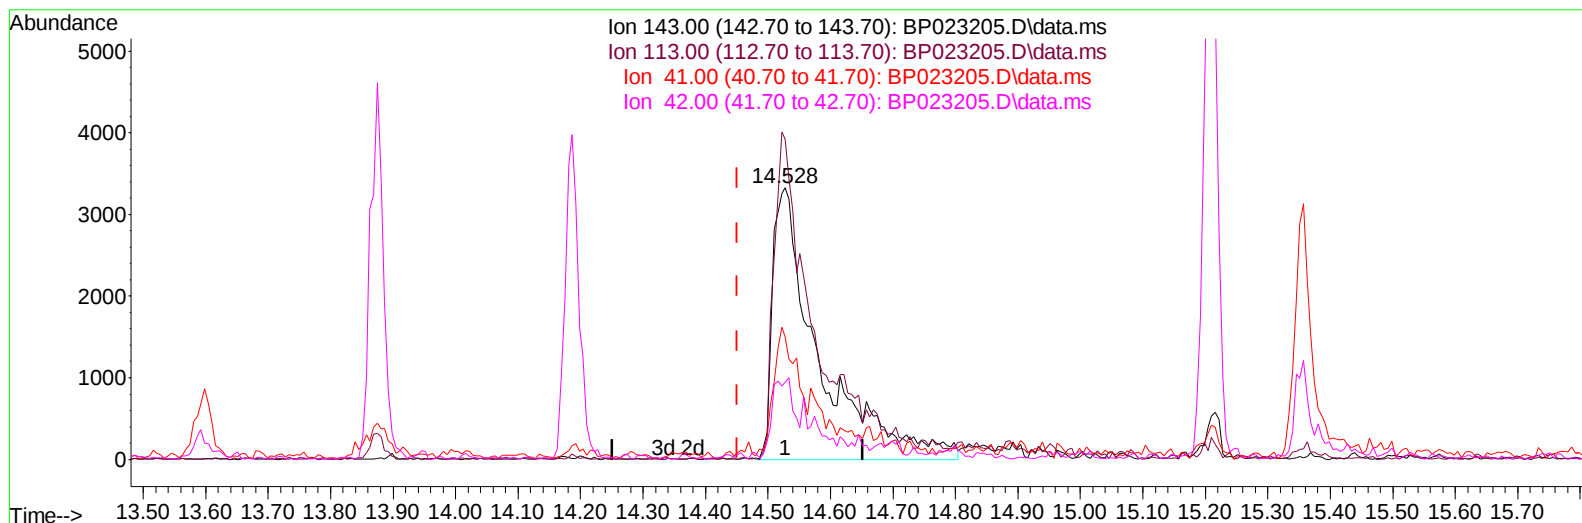

TIC: BP023205.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.528min (+ 0.076) 8.81 ng/ul m

response 17144

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	107.90	118.01
41.00	39.20	45.22
42.00	25.90	28.32

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111824\
 Data File : BP023205.D
 Acq On : 18 Nov 2024 20:04
 Operator : RC/JU
 Sample : P4884-01
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BG3M5

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/19/2024
 Supervised By :mohammad ahmed 11/19/2024

Quant Time: Nov 19 00:06:27 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 13 04:49:01 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.569	152	59564	20.000	ng/ul	-0.01
20) Naphthalene-d8	10.322	136	230854	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.187	164	179755	20.000	ng/ul	-0.02
64) Phenanthrene-d10	17.004	188	462257	20.000	ng/ul	-0.01
79) Chrysene-d12	21.433	240	540432	20.000	ng/ul	-0.01
88) Perylene-d12	24.651	264	641563	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.134	96	6585	5.314	ng/uL	0.00
4) Pyridine-d5	3.564	84	23738	6.448	ng/ul	0.02
7) Phenol-d5	6.787	99	55564	12.618	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.922	67	87332	33.754	ng/ul	0.00
11) 2-Chlorophenol-d4	7.116	132	96916	30.050	ng/ul	-0.01
15) 4-Methylphenol-d8	8.281	113	91290	25.191	ng/ul	-0.01
21) Nitrobenzene-d5	8.716	128	54304	33.789	ng/ul	0.00
24) 2-Nitrophenol-d4	9.434	143	64732	33.785	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.969	165	129990m	32.397	ng/ul	0.00
31) 4-Chloroaniline-d4	10.475	131	123472	25.794	ng/ul	0.00
46) Dimethylphthalate-d6	13.598	166	477587	36.864	ng/ul	-0.01
49) Acenaphthylene-d8	13.875	160	496050	36.695	ng/ul	-0.02
54) 4-Nitrophenol-d4	14.528	143	17144m	8.805	ng/ul	0.08
60) Fluorene-d10	15.210	176	435962	38.381	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.357	200	83480	30.146	ng/ul	0.00
73) Anthracene-d10	17.098	188	824023	42.101	ng/ul	-0.02
81) Pyrene-d10	19.486	212	1059221	42.551	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.433	264	1302414	42.618	ng/ul	-0.01

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111824\
Data File : BP023205.D
Acq On : 18 Nov 2024 20:04
Operator : RC/JU
Sample : P4884-01
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BG3M5

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/19/2024
Supervised By :mohammad ahmed 11/19/2024

Quant Time: Nov 19 00:06:27 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 13 04:49:01 2024
Response via : Initial Calibration

