

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111824\
 Data File : BP023199.D
 Acq On : 18 Nov 2024 16:01
 Operator : RC/JU
 Sample : P4784-18
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E27P6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP023199.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.134	21	25	35	rVB	10971	16967	1.25%	0.152%
2	3.481	80	84	87	rBV6	1316	1782	0.13%	0.016%
3	3.569	96	99	111	rBV	18644	43809	3.23%	0.392%
4	3.858	144	148	154	rVB4	3491	5197	0.38%	0.046%
5	5.022	344	346	349	rBV3	1171	1604	0.12%	0.014%
6	5.987	509	510	516	rVB6	1185	1516	0.11%	0.014%
7	6.134	531	535	538	rBV6	1379	1523	0.11%	0.014%
8	6.799	642	648	664	rVV2	43282	119757	8.84%	1.071%
9	6.928	665	670	684	rVB	69783	123757	9.13%	1.107%
10	7.134	696	705	717	rBV	81666	161136	11.89%	1.441%
11	7.575	774	780	794	rBV	201306	366673	27.05%	3.280%
12	8.210	885	888	893	rVB7	814	1389	0.10%	0.012%
13	8.310	898	905	927	rBV	75294	202537	14.94%	1.812%
14	8.728	970	976	993	rVV	84072	175715	12.96%	1.572%
15	9.099	1035	1039	1042	rBV6	1172	1755	0.13%	0.016%
16	9.252	1060	1065	1071	rBV10	1160	3261	0.24%	0.029%
17	9.440	1089	1097	1116	rBV	67558	159758	11.79%	1.429%
18	9.781	1153	1155	1159	rVB5	1362	1595	0.12%	0.014%
19	9.863	1164	1169	1172	rVV7	903	1456	0.11%	0.013%
20	10.004	1184	1193	1209	rBV	65718	223424	16.48%	1.998%
21	10.322	1239	1247	1259	rBV	294052	514009	37.92%	4.597%
22	10.499	1269	1277	1302	rBV	70400	217115	16.02%	1.942%
23	10.716	1311	1314	1317	rVB5	1501	1668	0.12%	0.015%
24	10.740	1317	1318	1324	rBV5	1082	1443	0.11%	0.013%
25	12.522	1618	1621	1625	rBV6	1070	1931	0.14%	0.017%
26	13.187	1728	1734	1740	rBV7	2482	4684	0.35%	0.042%
27	13.604	1800	1805	1826	rBV	263392	422491	31.17%	3.779%
28	13.740	1826	1828	1830	rVV3	1281	1507	0.11%	0.013%
29	13.787	1833	1836	1840	rVB6	1278	2056	0.15%	0.018%
30	13.887	1846	1853	1862	rBV	254962	435107	32.10%	3.892%
31	14.057	1878	1882	1887	rVB7	926	1742	0.13%	0.016%
32	14.187	1897	1904	1918	rBV	494897	794927	58.65%	7.110%
33	14.545	1960	1965	1971	rBV5	13564	37928	2.80%	0.339%
34	14.939	2027	2032	2034	rBV5	1054	1512	0.11%	0.014%
35	15.057	2050	2052	2057	rVB5	1664	1680	0.12%	0.015%
36	15.204	2069	2077	2091	rBV2	270849	620966	45.81%	5.554%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111824\
Data File : BP023199.D
Acq On : 18 Nov 2024 16:01
Operator : RC/JU
Sample : P4784-18
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E27P6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Title : SVOA CALIBRATION

37	15.381	2100	2107	2118	rBV2	52968	126741	9.35%	1.134%
38	15.604	2138	2145	2153	rBV2	2828	6251	0.46%	0.056%
39	15.798	2176	2178	2183	rVB6	1355	1888	0.14%	0.017%
40	15.934	2199	2201	2203	rBV3	1239	1385	0.10%	0.012%
41	16.751	2339	2340	2343	rBV3	1217	1484	0.11%	0.013%
42	16.804	2346	2349	2351	rVV4	2513	2936	0.22%	0.026%
43	16.845	2353	2356	2358	rBV4	1214	1570	0.12%	0.014%
44	16.998	2375	2382	2395	rBV	626020	1072241	79.11%	9.590%
45	17.116	2395	2402	2418	rVV	436456	732615	54.05%	6.553%
46	17.716	2502	2504	2507	rVB4	2012	1398	0.10%	0.013%
47	17.951	2540	2544	2550	rBV8	8737	17601	1.30%	0.157%
48	18.016	2553	2555	2558	rVB3	2612	1840	0.14%	0.016%
49	18.239	2591	2593	2595	rBV3	1777	1785	0.13%	0.016%
50	18.745	2677	2679	2681	rVB3	2621	1975	0.15%	0.018%
51	19.039	2726	2729	2730	rBV3	7120	5968	0.44%	0.053%
52	19.075	2733	2735	2739	rVB4	6518	5669	0.42%	0.051%
53	19.280	2768	2770	2774	rBV5	4465	4916	0.36%	0.044%
54	19.492	2800	2806	2822	rBV	597574	968117	71.42%	8.659%
55	21.439	3131	3137	3150	rBV2	687843	1324069	97.68%	11.843%
56	24.433	3637	3646	3657	rVB	351083	868963	64.11%	7.772%
57	24.651	3675	3683	3701	rVB	466555	1355452	100.00%	12.124%




Sum of corrected areas: 11180241

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111824\
Data File : BP023199.D
Acq On : 18 Nov 2024 16:01
Operator : RC/JU
Sample : P4784-18
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E27P6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

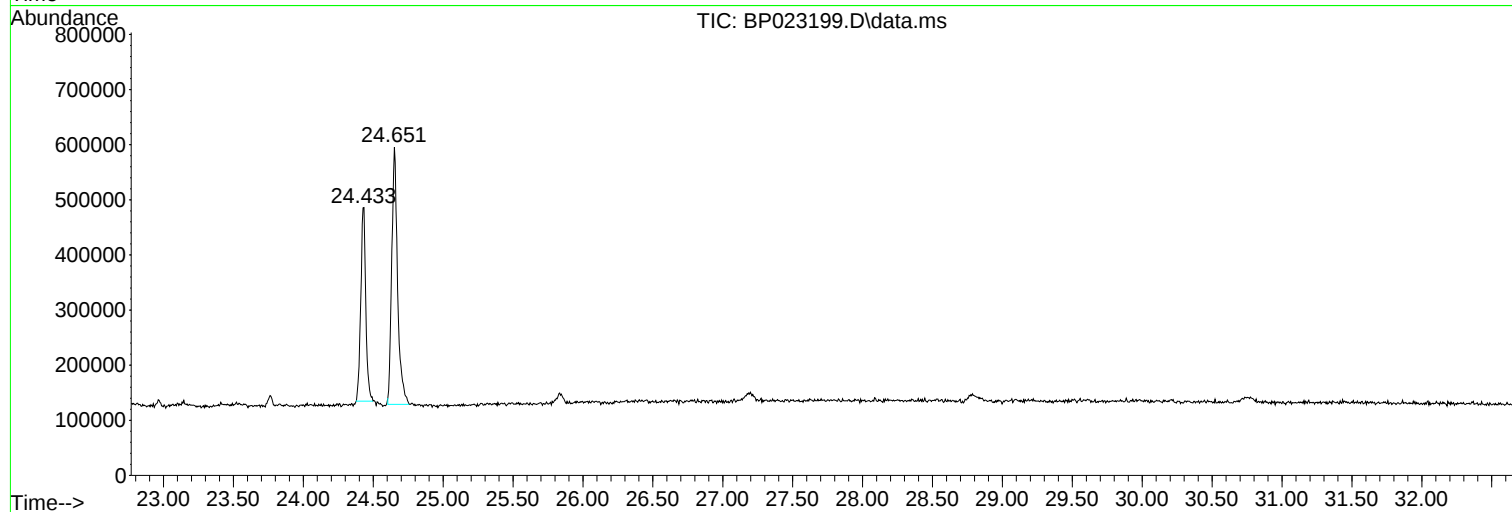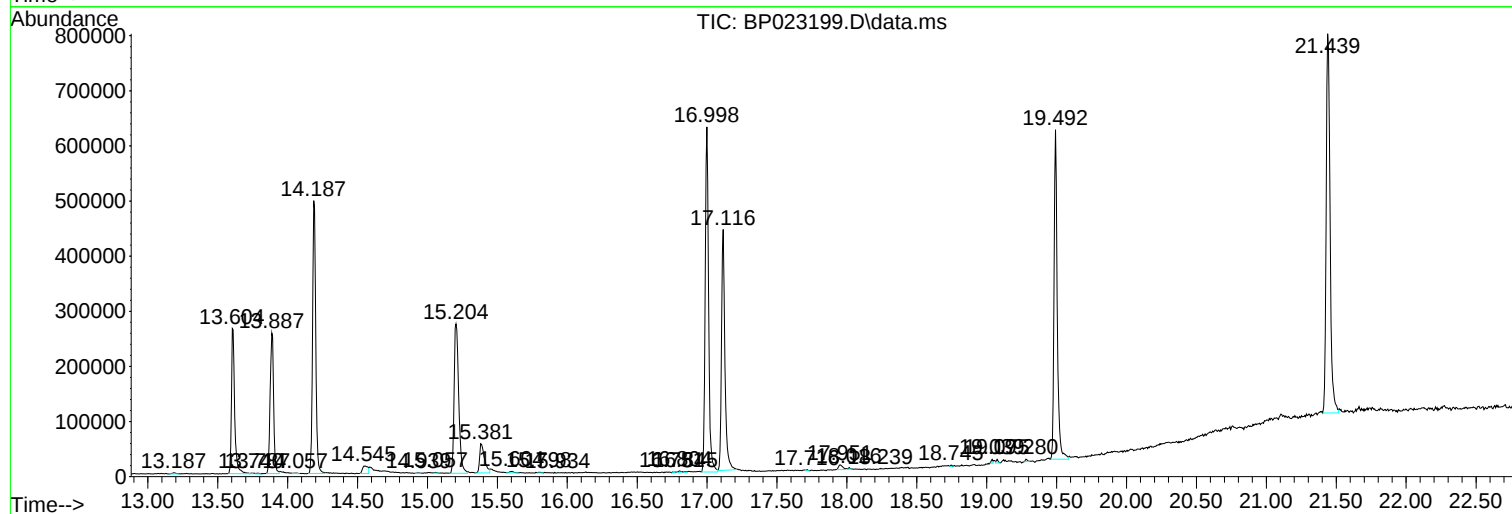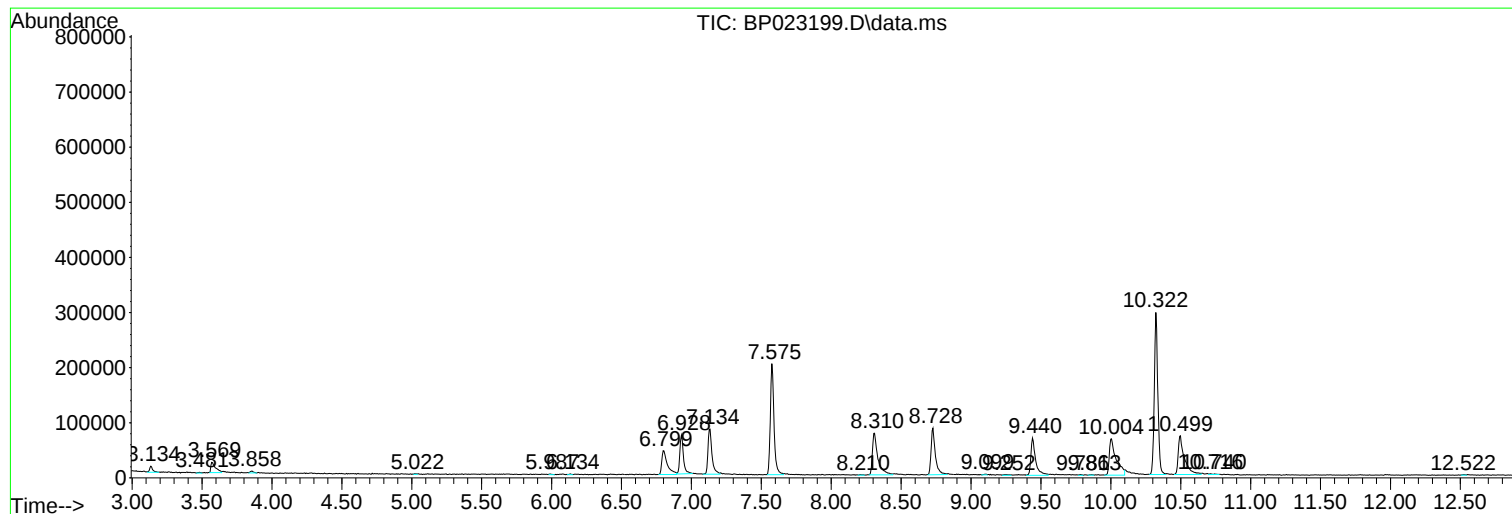

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111824\
Data File : BP023199.D
Acq On : 18 Nov 2024 16:01
Operator : RC/JU
Sample : P4784-18
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E27P6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111824\
Data File : BP023199.D
Acq On : 18 Nov 2024 16:01
Operator : RC/JU
Sample : P4784-18
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E27P6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
