

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111824\
 Data File : BP023201.D
 Acq On : 18 Nov 2024 17:22
 Operator : RC/JU
 Sample : PB165051BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK051

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP023201.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.134	22	25	33	rVB	21213	27212	0.99%	0.112%
2	3.546	92	95	115	rBV	225967	398218	14.51%	1.634%
3	3.852	144	147	153	rVB3	5733	8778	0.32%	0.036%
4	6.781	639	645	662	rBV	258026	523710	19.08%	2.149%
5	6.922	663	669	688	rVB	227130	389337	14.19%	1.598%
6	7.122	696	703	717	rBV	297564	522163	19.03%	2.143%
7	7.575	770	780	798	rBV	258990	465391	16.96%	1.910%
8	8.287	893	901	929	rBV2	303833	685879	24.99%	2.815%
9	8.722	968	975	993	rBV	288542	556940	20.30%	2.286%
10	8.857	993	998	1012	rVB3	15032	38701	1.41%	0.159%
11	9.434	1088	1096	1118	rBV	246934	488777	17.81%	2.006%
12	9.969	1179	1187	1209	rBV	320694	734091	26.75%	3.013%
13	10.316	1237	1246	1260	rBV	353223	627282	22.86%	2.574%
14	10.481	1266	1274	1291	rBV	235379	656764	23.93%	2.695%
15	11.963	1519	1526	1534	rBV6	3812	10986	0.40%	0.045%
16	13.598	1796	1804	1819	rBV	597139	1171150	42.68%	4.806%
17	13.875	1844	1851	1865	rBV	859441	1311125	47.78%	5.381%
18	14.187	1897	1904	1922	rBV	716714	961405	35.04%	3.945%
19	14.475	1947	1953	1971	rBV2	116039	454332	16.56%	1.864%
20	14.604	1971	1975	1981	rVB7	8983	22502	0.82%	0.092%
21	15.045	2046	2050	2054	rVB6	1866	2975	0.11%	0.012%
22	15.204	2071	2077	2092	rBV	1341639	1784671	65.04%	7.324%
23	15.357	2096	2103	2112	rBV	251728	474267	17.28%	1.946%
24	15.586	2138	2142	2151	rVB	2734	5691	0.21%	0.023%
25	16.004	2211	2213	2220	rVB7	2673	3237	0.12%	0.013%
26	16.669	2321	2326	2330	rBV6	2455	4474	0.16%	0.018%
27	16.992	2373	2381	2392	rBV	1011201	1315259	47.93%	5.398%
28	17.092	2392	2398	2416	rVV	1245493	2057132	74.97%	8.442%
29	17.692	2496	2500	2505	rBV8	3509	5046	0.18%	0.021%
30	17.963	2540	2546	2550	rBV9	2885	5714	0.21%	0.023%
31	19.039	2724	2729	2732	rBV4	16294	26135	0.95%	0.107%
32	19.122	2739	2743	2750	rBV2	15769	25113	0.92%	0.103%
33	19.492	2800	2806	2820	rBV	1935522	2602073	94.82%	10.678%
34	21.439	3131	3137	3144	rBV	972608	1613203	58.79%	6.620%
35	24.415	3635	3643	3661	rVB	1110002	2744104	100.00%	11.261%
36	24.651	3673	3683	3700	rBV	547475	1643937	59.91%	6.746%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111824\
Data File : BP023201.D
Acq On : 18 Nov 2024 17:22
Operator : RC/JU
Sample : PB165051BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK051

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 24367774

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111824\
Data File : BP023201.D
Acq On : 18 Nov 2024 17:22
Operator : RC/JU
Sample : PB165051BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK051

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

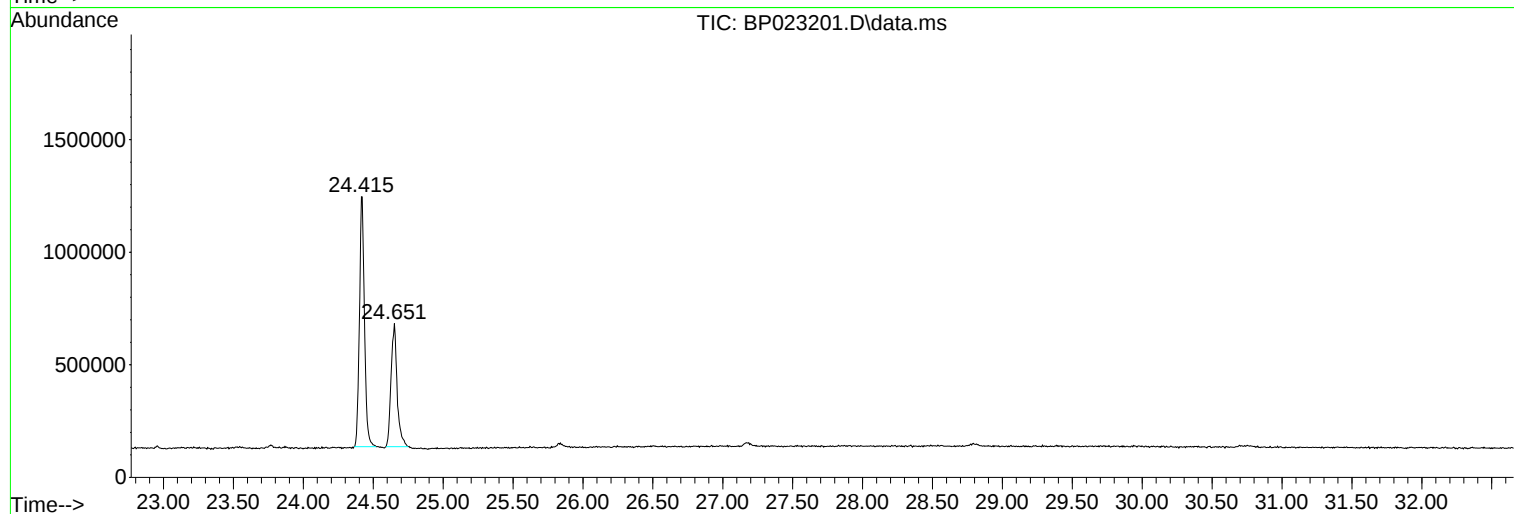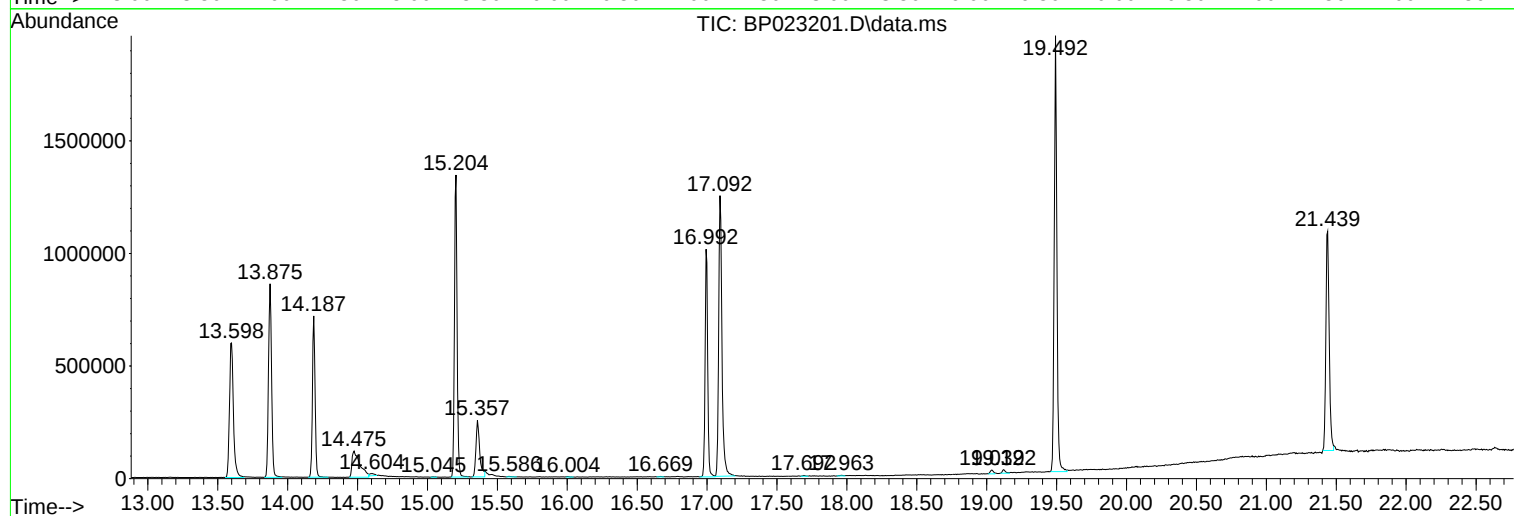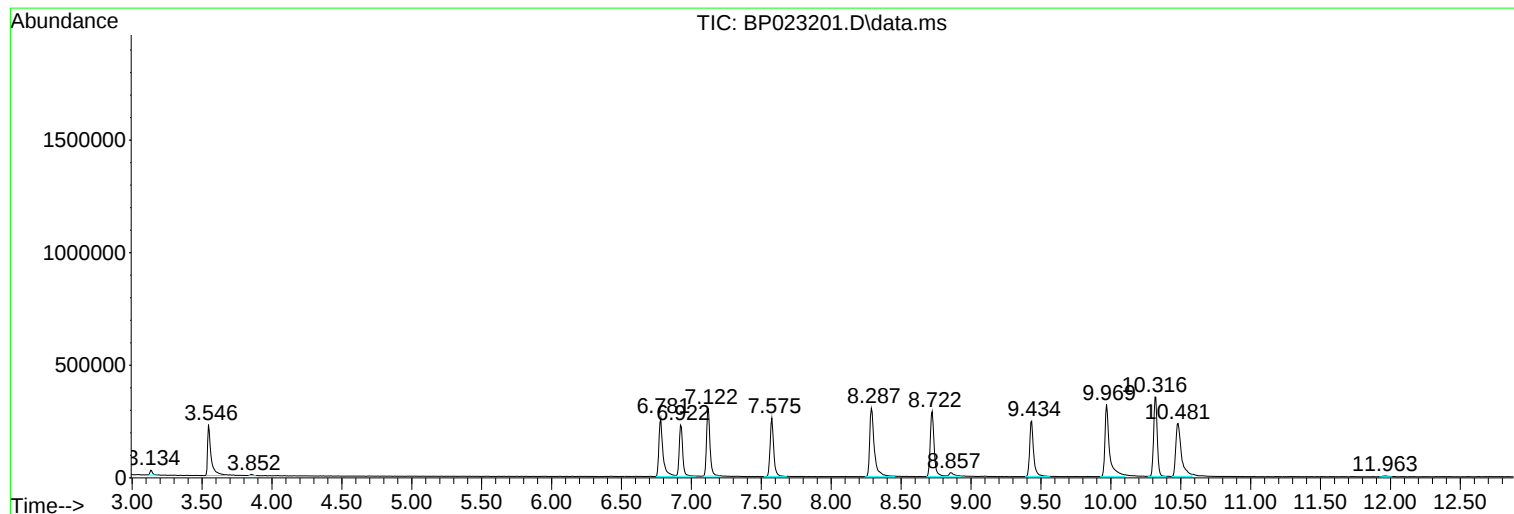

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111824\
Data File : BP023201.D
Acq On : 18 Nov 2024 17:22
Operator : RC/JU
Sample : PB165051BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK051

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111824\
Data File : BP023201.D
Acq On : 18 Nov 2024 17:22
Operator : RC/JU
Sample : PB165051BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK051

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc