

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111824\
 Data File : BP023203.D
 Acq On : 18 Nov 2024 18:43
 Operator : RC/JU
 Sample : P4882-13
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BG3J0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP023203.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.099	15	19	23	rBV	102101	132729	5.25%	0.678%
2	3.858	144	148	157	rBV3	4198	6784	0.27%	0.035%
3	4.281	215	220	225	rVB5	3079	5518	0.22%	0.028%
4	4.370	229	235	248	rVB	23104	38685	1.53%	0.198%
5	6.717	628	634	639	rVB3	4570	7616	0.30%	0.039%
6	6.787	639	646	663	rBV	69693	171150	6.76%	0.874%
7	6.922	663	669	681	rVB	162967	276469	10.93%	1.412%
8	7.122	696	703	724	rBV	228286	404156	15.97%	2.064%
9	7.575	772	780	790	rBV	220049	393640	15.56%	2.011%
10	7.652	791	793	803	rVB8	4333	8763	0.35%	0.045%
11	8.287	895	901	923	rBV	195338	424369	16.77%	2.168%
12	8.716	968	974	998	rBV	221037	435200	17.20%	2.223%
13	9.105	1035	1040	1046	rBV8	2732	4725	0.19%	0.024%
14	9.428	1085	1095	1112	rBV	183776	382432	15.11%	1.954%
15	9.975	1180	1188	1213	rBV2	195951	587828	23.23%	3.003%
16	10.316	1239	1246	1261	rVB	296096	528023	20.87%	2.697%
17	10.493	1266	1276	1297	rBV2	51067	157685	6.23%	0.805%
18	11.887	1507	1513	1519	rBV8	3041	6963	0.28%	0.036%
19	11.946	1519	1523	1533	rVB6	3248	7818	0.31%	0.040%
20	13.593	1795	1803	1818	rBV	560364	928932	36.71%	4.745%
21	13.869	1842	1850	1865	rBV	632324	1003247	39.65%	5.125%
22	14.187	1897	1904	1920	rVB	535439	788067	31.14%	4.026%
23	14.504	1952	1958	1975	rBV3	34752	146866	5.80%	0.750%
24	14.687	1984	1989	1995	rVB8	5167	10930	0.43%	0.056%
25	15.045	2045	2050	2055	rBV4	2412	3687	0.15%	0.019%
26	15.198	2069	2076	2089	rBV	1020502	1385137	54.74%	7.075%
27	15.357	2096	2103	2118	rBV	216028	453810	17.93%	2.318%
28	15.581	2136	2141	2146	rBV	19223	27684	1.09%	0.141%
29	15.793	2173	2177	2180	rBV6	1376	2654	0.10%	0.014%
30	16.163	2231	2240	2244	rBV4	7003	12880	0.51%	0.066%
31	16.675	2322	2327	2329	rBV5	1782	3039	0.12%	0.016%
32	16.792	2342	2347	2351	rBV6	2236	3558	0.14%	0.018%
33	16.998	2376	2382	2392	rBV	840038	1088418	43.01%	5.560%
34	17.098	2392	2399	2417	rVV	1107443	1746447	69.02%	8.921%
35	17.616	2484	2487	2490	rBV5	1898	2739	0.11%	0.014%
36	17.934	2537	2541	2551	rVV6	19643	36689	1.45%	0.187%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111824\
Data File : BP023203.D
Acq On : 18 Nov 2024 18:43
Operator : RC/JU
Sample : P4882-13
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BG3J0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Title : SVOA CALIBRATION

37	18.804	2685	2689	2694	rBV7	7559	14022	0.55%	0.072%
38	18.934	2707	2711	2718	rVB2	15036	20013	0.79%	0.102%
39	19.039	2725	2729	2734	rBV3	14479	22406	0.89%	0.114%
40	19.122	2739	2743	2748	rBV2	15884	24925	0.99%	0.127%
41	19.216	2755	2759	2765	rBV	48385	51463	2.03%	0.263%
42	19.275	2766	2769	2775	rVB7	10683	14490	0.57%	0.074%
43	19.492	2800	2806	2820	rBV	1745483	2267167	89.60%	11.581%
44	21.439	3131	3137	3148	rBV	795752	1394618	55.11%	7.124%
45	24.427	3635	3645	3658	rBV	953299	2530429	100.00%	12.926%
46	24.657	3674	3684	3704	rVB2	487711	1611782	63.70%	8.233%




Sum of corrected areas: 19576652

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111824\
Data File : BP023203.D
Acq On : 18 Nov 2024 18:43
Operator : RC/JU
Sample : P4882-13
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BG3J0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

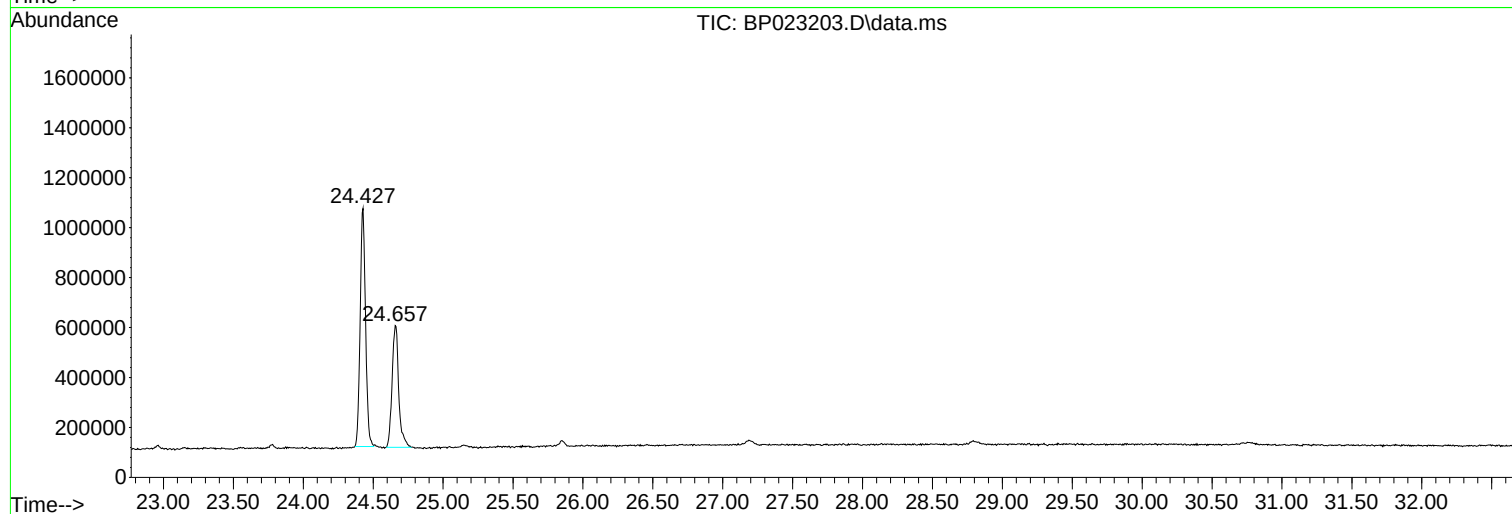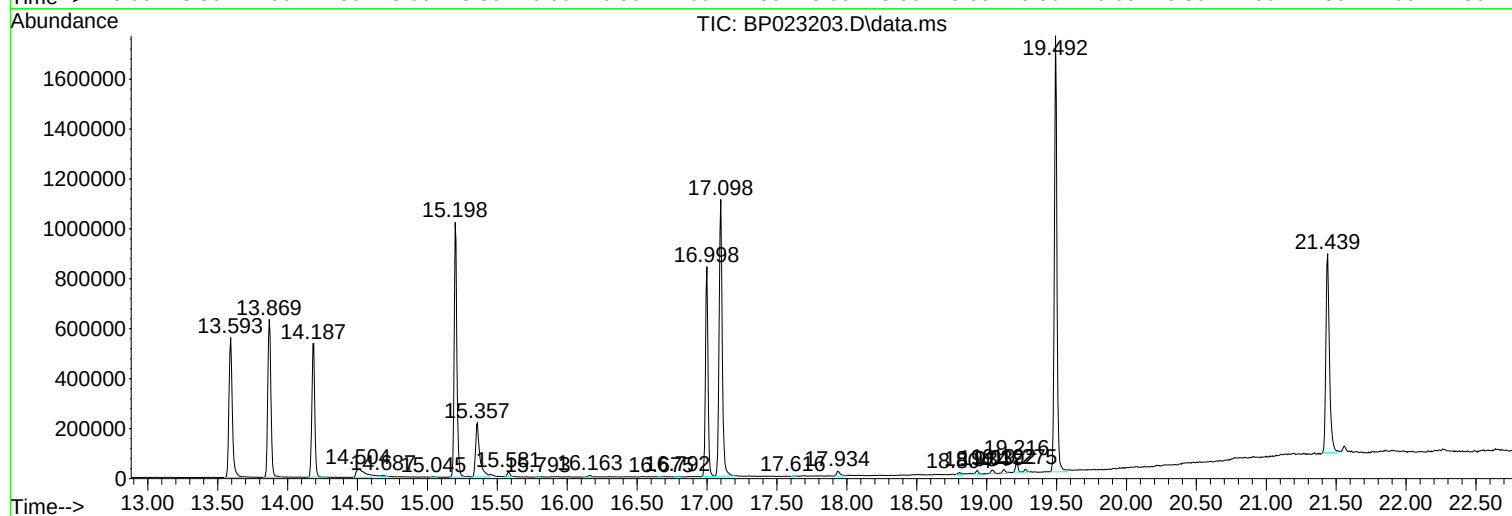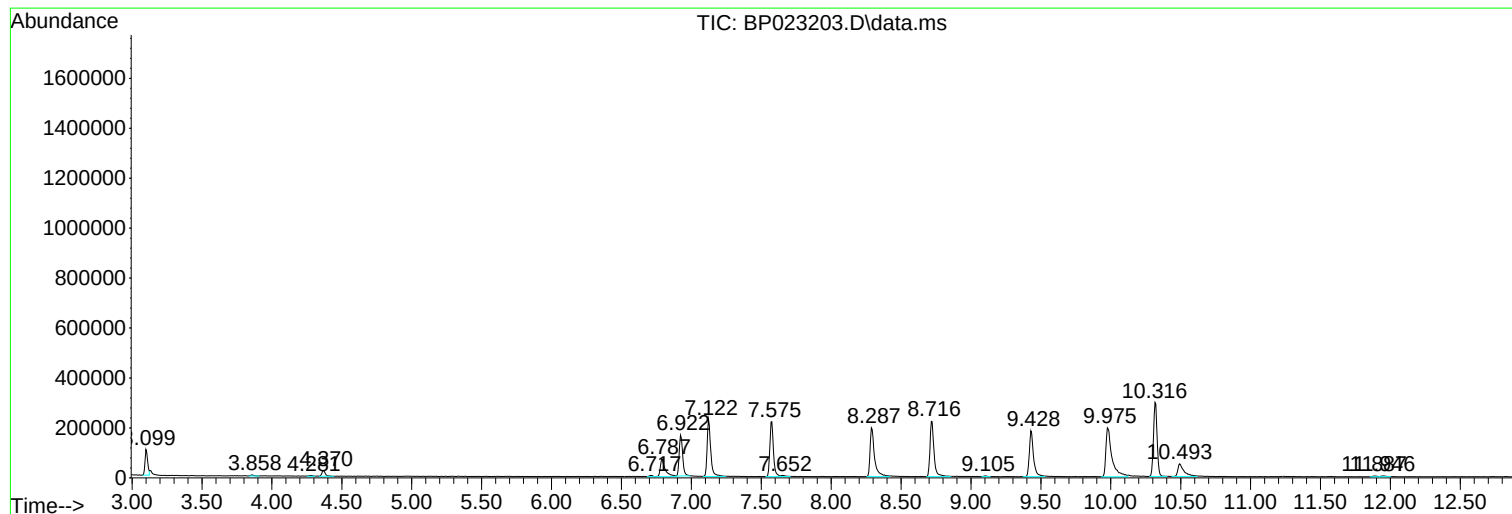

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111824\
Data File : BP023203.D
Acq On : 18 Nov 2024 18:43
Operator : RC/JU
Sample : P4882-13
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BG3J0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111824\
Data File : BP023203.D
Acq On : 18 Nov 2024 18:43
Operator : RC/JU
Sample : P4882-13
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BG3J0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc