

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111824\
 Data File : BP023206.D
 Acq On : 18 Nov 2024 20:45
 Operator : RC/JU
 Sample : P4884-11
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BG3N5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP023206.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.105	16	20	23	rBV	17852	24029	0.89%	0.116%
2	3.134	23	25	30	rVB	14581	15755	0.58%	0.076%
3	3.858	144	148	152	rBV4	3920	6482	0.24%	0.031%
4	4.275	216	219	225	rVB	4948	7652	0.28%	0.037%
5	4.364	227	234	246	rBV	60640	98508	3.63%	0.475%
6	6.716	629	634	640	rVB4	4828	7659	0.28%	0.037%
7	6.793	640	647	664	rBV	77924	188215	6.94%	0.908%
8	6.922	664	669	689	rVB	192226	319010	11.76%	1.539%
9	7.122	697	703	722	rBV	240093	444223	16.37%	2.143%
10	7.575	773	780	792	rBV	221607	397219	14.64%	1.916%
11	8.293	893	902	923	rBV2	218352	470811	17.35%	2.271%
12	8.722	968	975	988	rBV	273565	470916	17.35%	2.271%
13	9.104	1035	1040	1042	rBV4	2639	3582	0.13%	0.017%
14	9.434	1089	1096	1114	rBV	219288	433053	15.96%	2.089%
15	9.981	1182	1189	1208	rBV	211088	615357	22.68%	2.968%
16	10.322	1239	1247	1261	rVB	318845	533062	19.64%	2.571%
17	10.563	1282	1288	1296	rBV6	3156	7921	0.29%	0.038%
18	11.222	1394	1400	1401	rBV6	2568	3476	0.13%	0.017%
19	11.957	1516	1525	1528	rBV9	3682	9351	0.34%	0.045%
20	13.592	1796	1803	1818	rBV	682078	1069972	39.43%	5.161%
21	13.875	1841	1851	1867	rBV2	706461	1041079	38.37%	5.022%
22	14.187	1897	1904	1915	rBV	654552	830004	30.59%	4.003%
23	14.434	1939	1946	1951	rBV10	1107	3519	0.13%	0.017%
24	14.498	1951	1957	1971	rBV2	48448	159961	5.89%	0.772%
25	15.051	2046	2051	2055	rVB5	2175	4064	0.15%	0.020%
26	15.204	2070	2077	2087	rBV	1061358	1603763	59.10%	7.736%
27	15.287	2087	2091	2095	rVB7	3814	6648	0.24%	0.032%
28	15.363	2097	2104	2118	rBV	261080	519534	19.15%	2.506%
29	16.428	2280	2285	2288	rBV7	2367	3437	0.13%	0.017%
30	16.669	2322	2326	2331	rVB8	1927	3622	0.13%	0.017%
31	16.998	2376	2382	2392	rBV	894779	1158139	42.68%	5.586%
32	17.092	2392	2398	2420	rVB	1279815	1932859	71.23%	9.323%
33	17.698	2496	2501	2504	rBV5	2739	4671	0.17%	0.023%
34	17.933	2537	2541	2548	rBV2	27398	47204	1.74%	0.228%
35	18.004	2551	2553	2557	rVB4	3150	3603	0.13%	0.017%
36	19.027	2722	2727	2733	rBV3	16637	30228	1.11%	0.146%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111824\
Data File : BP023206.D
Acq On : 18 Nov 2024 20:45
Operator : RC/JU
Sample : P4884-11
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BG3N5

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Title : SVOA CALIBRATION

37	19.122	2738	2743	2747	rBV	19302	31881	1.17%	0.154%
38	19.210	2755	2758	2761	rBV4	12546	14717	0.54%	0.071%
39	19.269	2765	2768	2773	rVB7	10847	16271	0.60%	0.078%
40	19.486	2799	2805	2819	rBV	1694517	2441191	89.96%	11.775%
41	21.427	3130	3135	3149	rBV2	913066	1428139	52.63%	6.889%
42	24.421	3634	3644	3663	rVB	978679	2713546	100.00%	13.089%
43	24.639	3673	3681	3701	rVB	490487	1607657	59.25%	7.754%




Sum of corrected areas: 20731990

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111824\
Data File : BP023206.D
Acq On : 18 Nov 2024 20:45
Operator : RC/JU
Sample : P4884-11
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BG3N5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

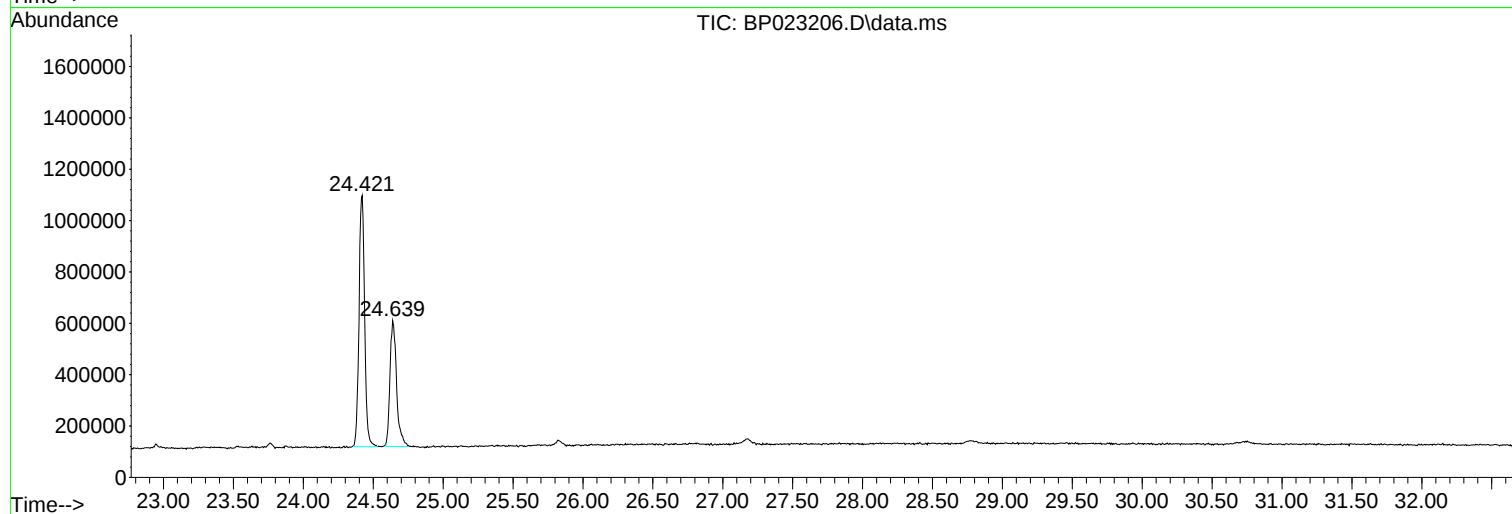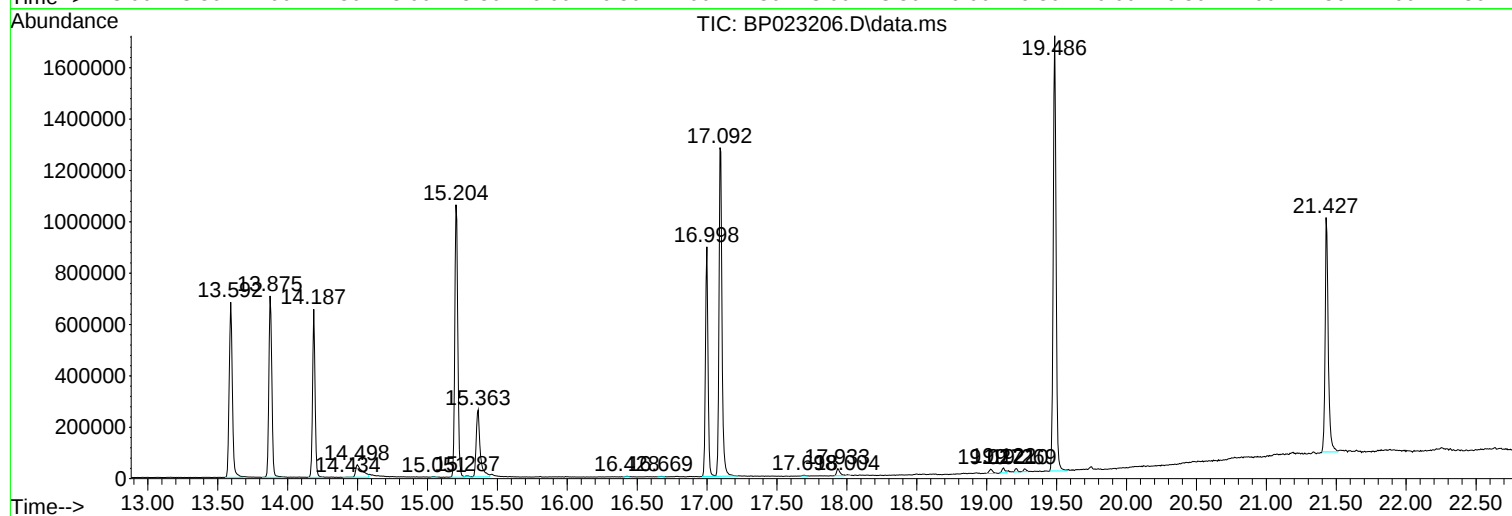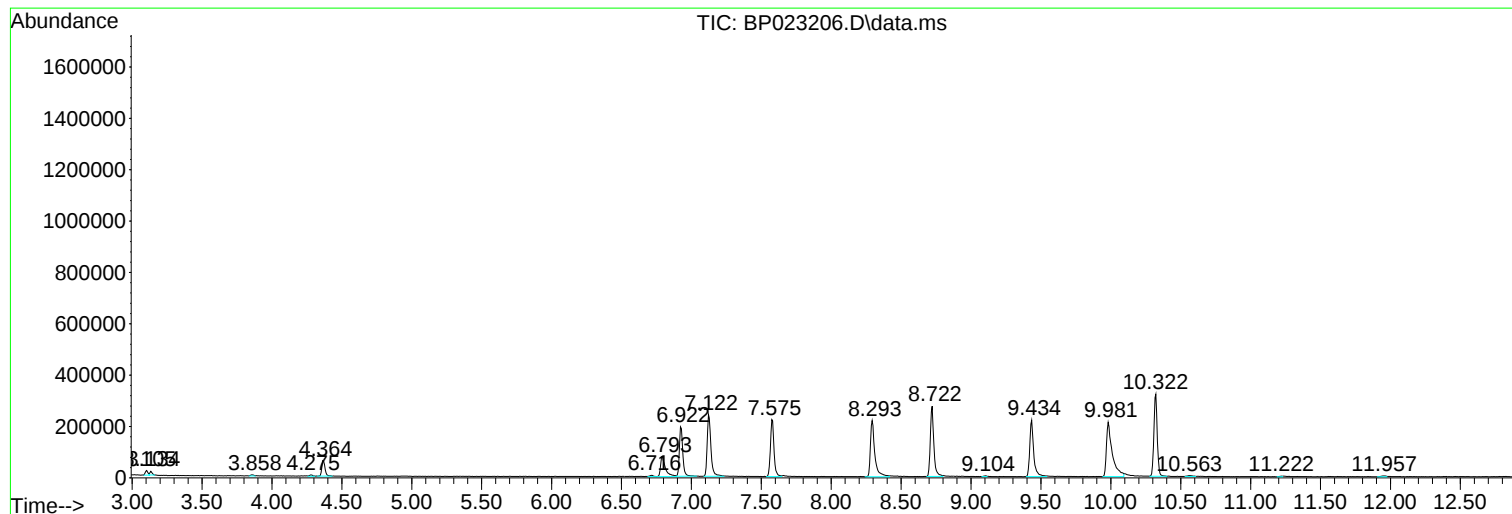

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111824\
Data File : BP023206.D
Acq On : 18 Nov 2024 20:45
Operator : RC/JU
Sample : P4884-11
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BG3N5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111824\
Data File : BP023206.D
Acq On : 18 Nov 2024 20:45
Operator : RC/JU
Sample : P4884-11
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BG3N5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc