




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111924\
Data File : BP023237.D
Acq On : 20 Nov 2024 04:49
Operator : RC/JU
Sample : PB165071BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK071

Manual IntegrationsAPPROVED

Quant Time: Nov 20 05:14:12 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 20 04:34:35 2024
Response via : Initial Calibration

Reviewed By :Yogesh
Patel

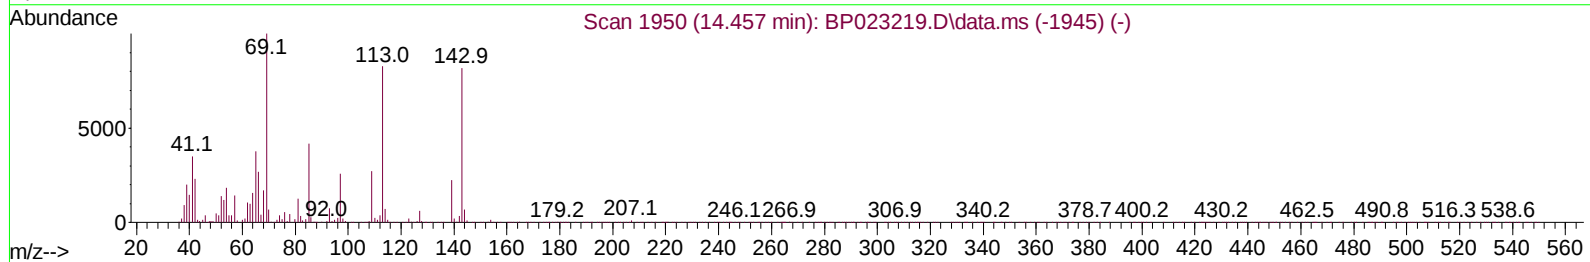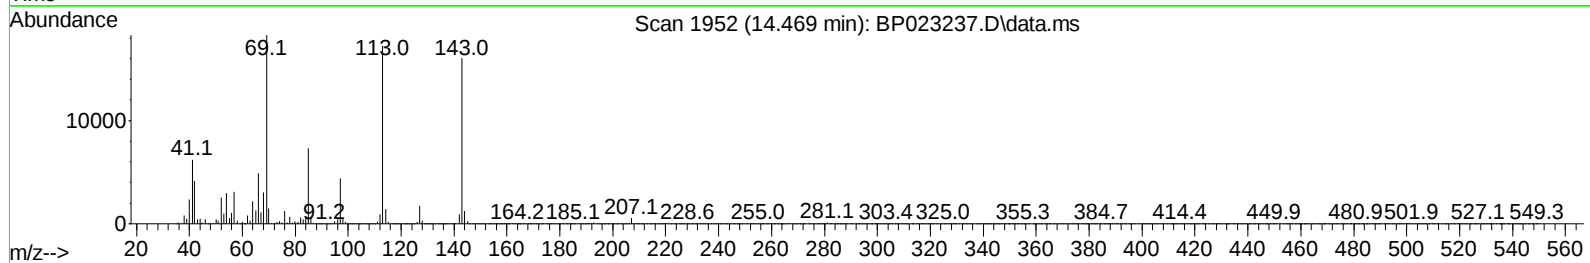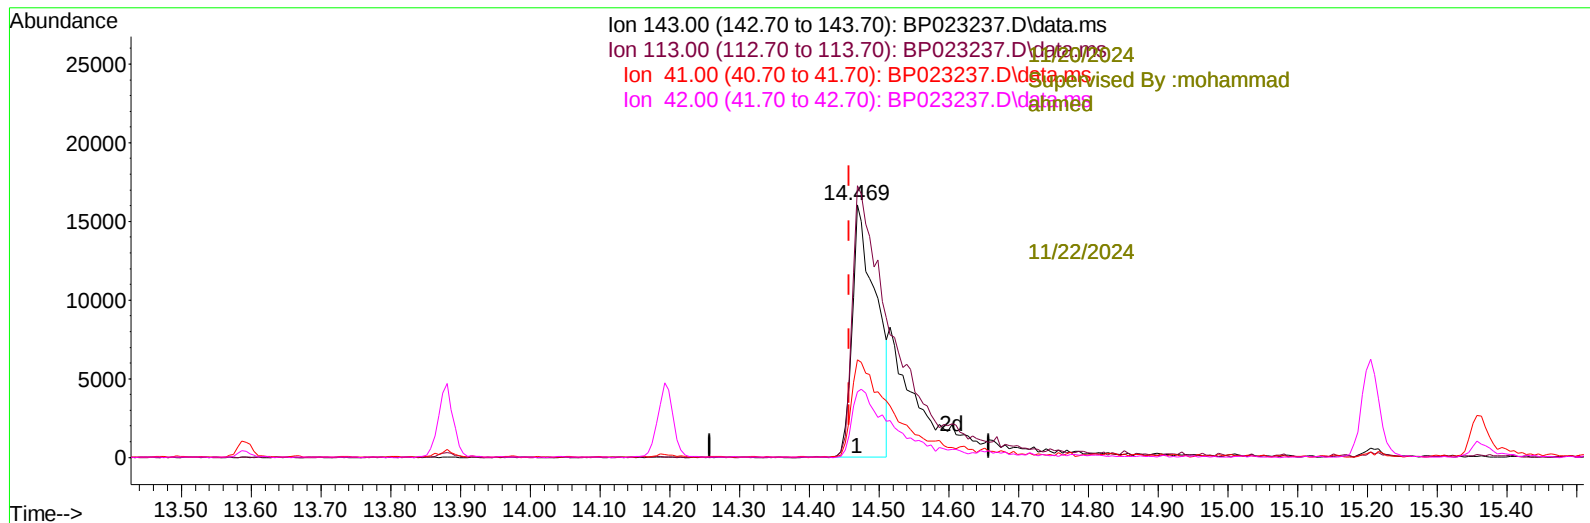

TIC: BP023237.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.469min (+ 0.012) 15.94 ng/u1

response 38196

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	107.90	107.64
41.00	39.20	38.78
42.00	25.90	25.92




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111924\
Data File : BP023237.D
Acq On : 20 Nov 2024 04:49
Operator : RC/JU
Sample : PB165071BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK071

Manual IntegrationsAPPROVED

Quant Time: Nov 20 05:14:12 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 20 04:34:35 2024
Response via : Initial Calibration

Reviewed By :Yogesh
Patel

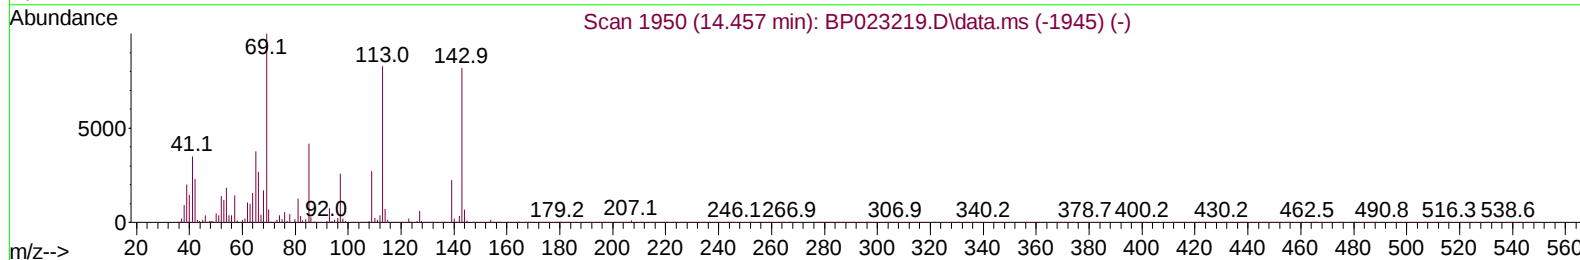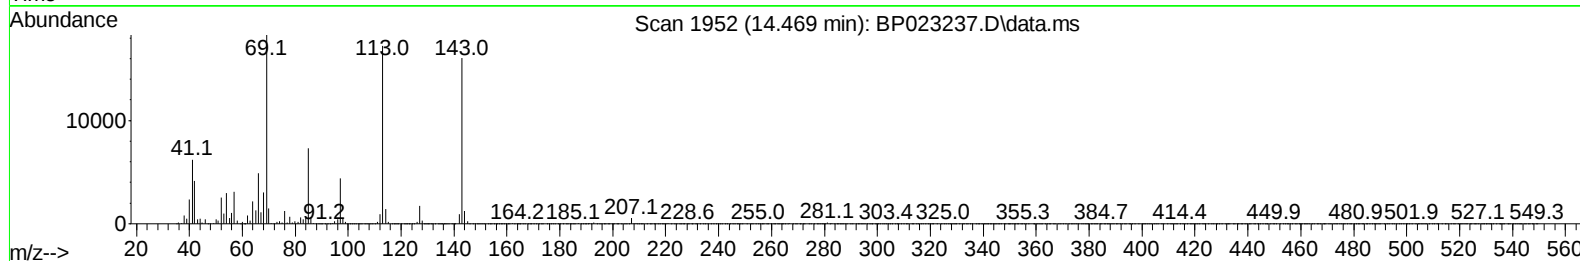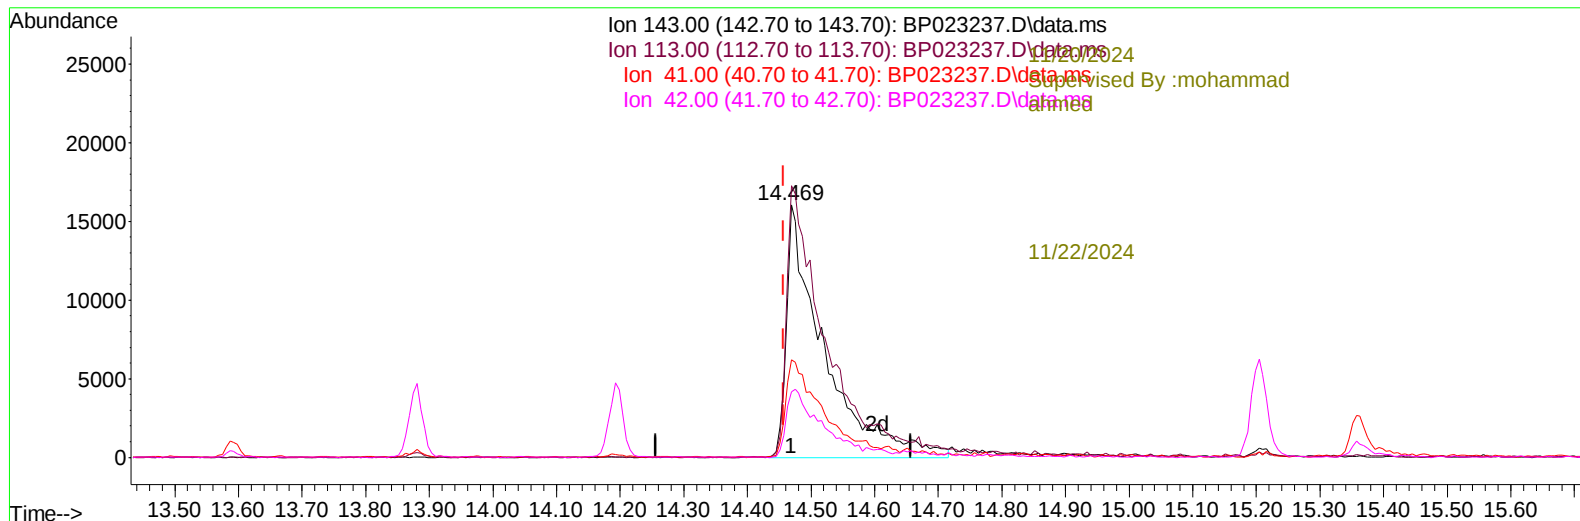

TIC: BP023237.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.469min (+ 0.012) 27.22 ng/ul m

response 65226

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	107.90	107.64
41.00	39.20	38.78
42.00	25.90	25.92

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111924\
 Data File : BP023237.D
 Acq On : 20 Nov 2024 04:49
 Operator : RC/JU
 Sample : PB165071BL
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK071

Manual IntegrationsAPPROVED

Quant Time: Nov 20 05:15:23 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 20 04:34:35 2024
 Response via : Initial Calibration

Reviewed By :Yogesh
 Patel

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
-----11/20/2024						
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.569	152	81062	20.000	ng/ul	0.00
20) Naphthalene-d8	10.316	136	290273	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.198	164	221257	20.000	ng/ul	0.01
64) Phenanthrene-d10	16.998	188	538148	20.000	ng/ul	0.00
79) Chrysene-d12	21.439	240	645439	20.000	ng/ul	0.02
88) Perylene-d12	24.668	264	766452	20.000	ng/ul	0.04
-----12/22/2024						
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.134	96	11274	6.685	ng/uL	0.00
4) Pyridine-d5	3.546	84	135718	27.087	ng/ul	0.00
7) Phenol-d5	6.775	99	165669	27.643	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.916	67	105244	29.890	ng/ul	0.00
11) 2-Chlorophenol-d4	7.116	132	130503	29.733	ng/ul	0.00
15) 4-Methylphenol-d8	8.281	113	131051	26.573	ng/ul	0.00
21) Nitrobenzene-d5	8.716	128	62763	31.058	ng/ul	0.00
24) 2-Nitrophenol-d4	9.422	143	74007	30.719	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.969	165	144247	28.591	ng/ul	0.00
31) 4-Chloroaniline-d4	10.469	131	158791	26.382	ng/ul	0.00
46) Dimethylphthalate-d6	13.593	166	516292	32.376	ng/ul	0.00
49) Acenaphthylene-d8	13.881	160	532138	31.981	ng/ul	0.00
54) 4-Nitrophenol-d4	14.469	143	65226m	27.217	ng/ul	0.01
60) Fluorene-d10	15.204	176	437447	31.288	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.363	200	78049	24.210	ng/ul	0.01
73) Anthracene-d10	17.104	188	770553	33.817	ng/ul	0.00
81) Pyrene-d10	19.480	212	970252	32.636	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.439	264	1188925	32.565	ng/ul	0.02

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111924\
Data File : BP023237.D
Acq On : 20 Nov 2024 04:49
Operator : RC/JU
Sample : PB165071BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK071

Manual IntegrationsAPPROVED

Quant Time: Nov 20 05:15:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 20 04:34:35 2024
Response via : Initial Calibration

Reviewed By :Yogesh
Patel

