




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111924\
Data File : BP023255.D
Acq On : 20 Nov 2024 17:43
Operator : RC/JU
Sample : P4875-21
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E2A20

Manual IntegrationsAPPROVED

Quant Time: Nov 21 03:31:19 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 20 04:34:35 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/22/2024
Supervised By :mohammad ahmed 11/22/2024

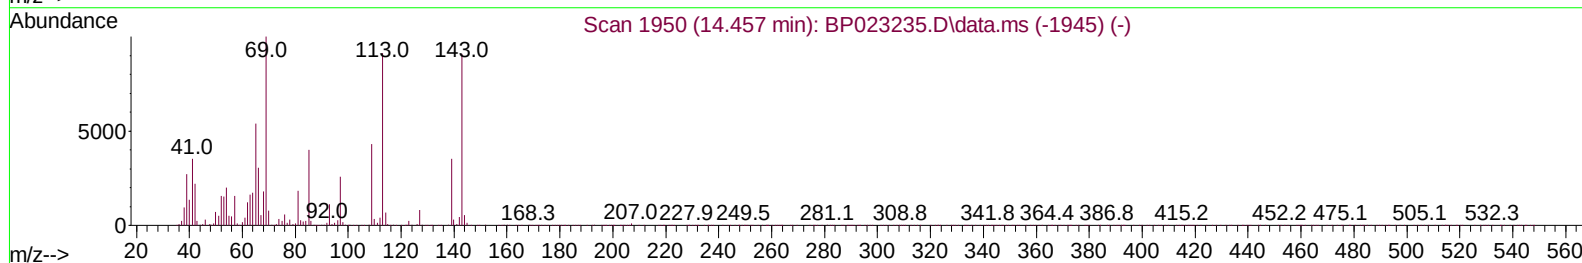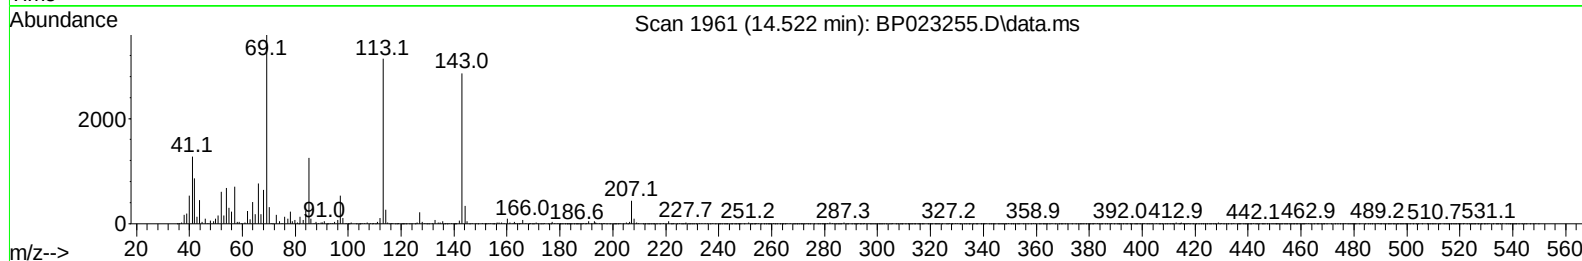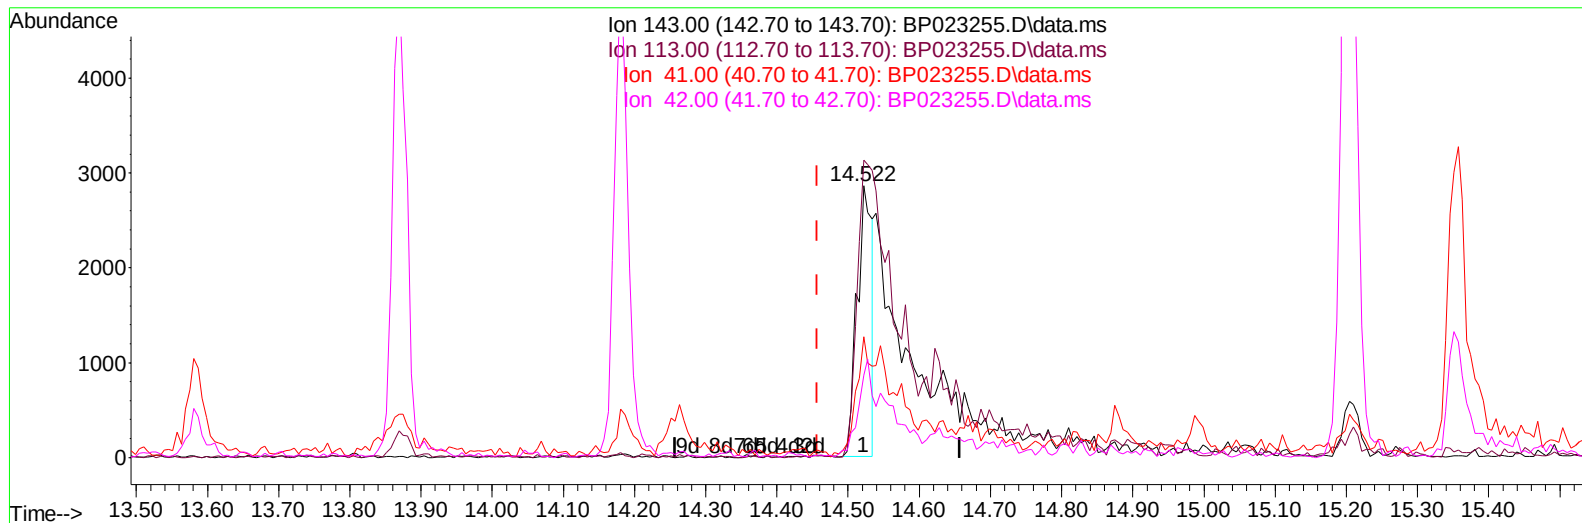

TIC: BP023255.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.522min (+ 0.065) 1.88 ng/ul

response 4179

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	107.90	109.60
41.00	39.20	44.52
42.00	25.90	30.31




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111924\
Data File : BP023255.D
Acq On : 20 Nov 2024 17:43
Operator : RC/JU
Sample : P4875-21
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E2A20

Manual IntegrationsAPPROVED

Quant Time: Nov 21 03:31:19 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 20 04:34:35 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/22/2024
Supervised By :mohammad ahmed 11/22/2024

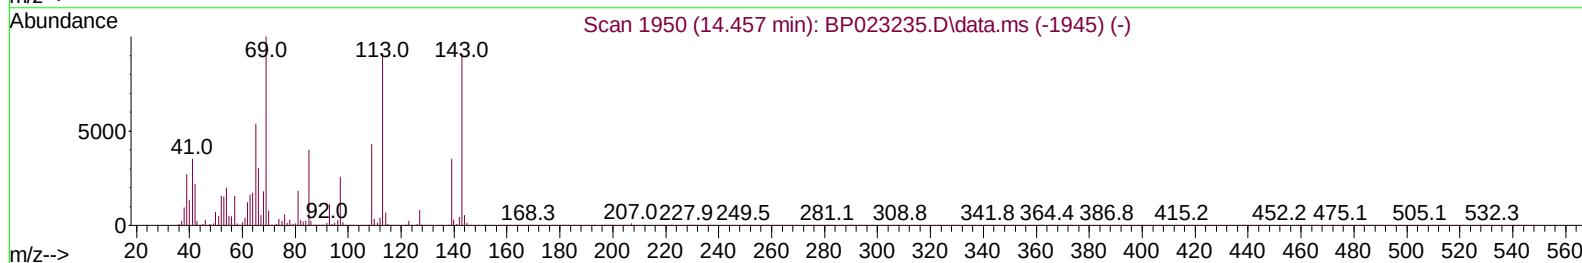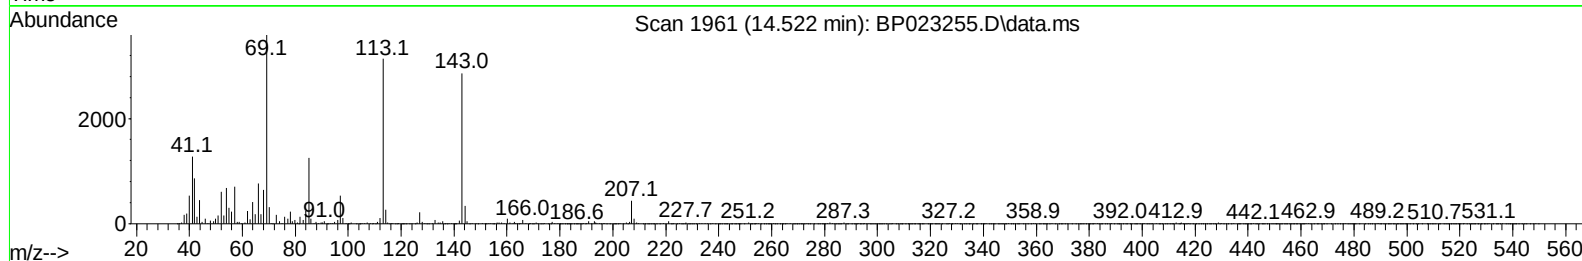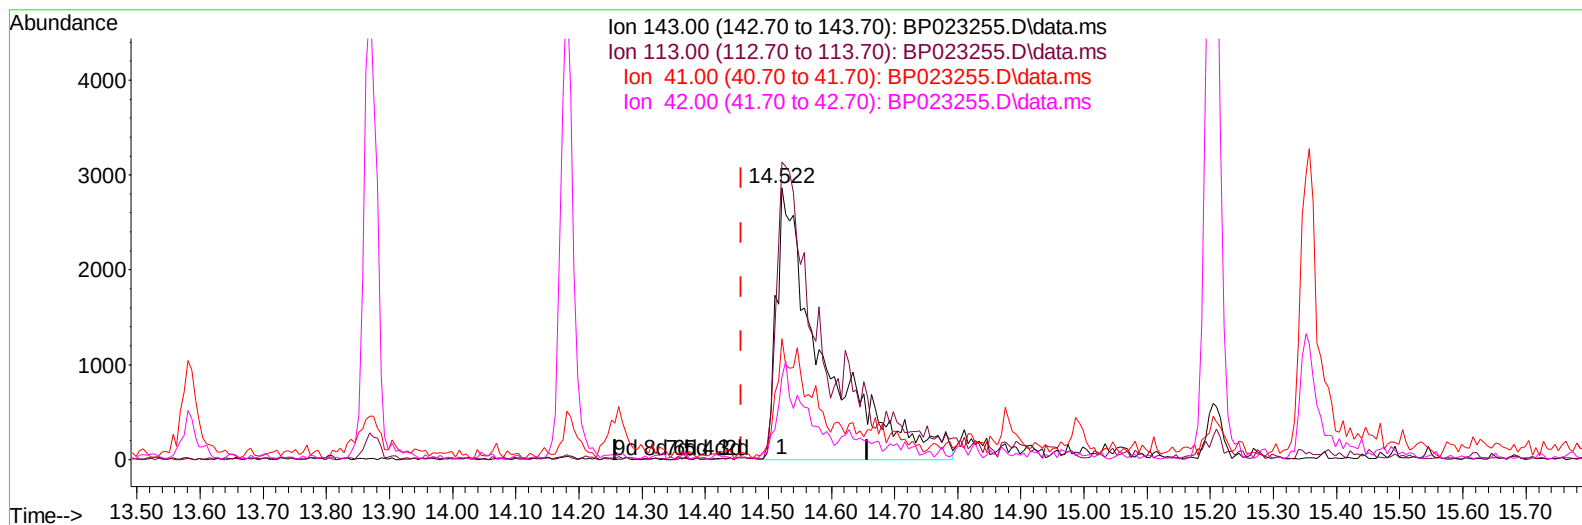

TIC: BP023255.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.522min (+ 0.065) 6.60 ng/ul m

response 14675

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	107.90	109.60
41.00	39.20	44.52
42.00	25.90	30.31

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111924\
 Data File : BP023255.D
 Acq On : 20 Nov 2024 17:43
 Operator : RC/JU
 Sample : P4875-21
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E2A20

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/22/2024
 Supervised By :mohammad ahmed 11/22/2024

Quant Time: Nov 21 03:32:12 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 20 04:34:35 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.563	152	72118	20.000	ng/ul	0.00
20) Naphthalene-d8	10.310	136	262832	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.181	164	205386	20.000	ng/ul	0.00
64) Phenanthrene-d10	16.998	188	515908	20.000	ng/ul	0.00
79) Chrysene-d12	21.433	240	578253	20.000	ng/ul	0.01
88) Perylene-d12	24.645	264	675081	20.000	ng/ul	0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.134	96	6927	4.617	ng/uL	0.00
4) Pyridine-d5	3.564	84	32336	7.254	ng/ul	0.02
7) Phenol-d5	6.787	99	34997	6.564	ng/ul	0.01
9) Bis-(2-Chloroethyl)eth...	6.916	67	97392	31.090	ng/ul	0.00
11) 2-Chlorophenol-d4	7.116	132	101449	25.980	ng/ul	0.00
15) 4-Methylphenol-d8	8.287	113	71874	16.381	ng/ul	0.00
21) Nitrobenzene-d5	8.710	128	56551	30.906	ng/ul	0.00
24) 2-Nitrophenol-d4	9.422	143	68881	31.576	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.963	165	135304	29.618	ng/ul	0.00
31) 4-Chloroaniline-d4	10.469	131	137352	25.202	ng/ul	0.00
46) Dimethylphthalate-d6	13.581	166	531737	35.921	ng/ul	0.00
49) Acenaphthylene-d8	13.869	160	517230	33.487	ng/ul	0.00
54) 4-Nitrophenol-d4	14.522	143	14675m	6.597	ng/ul	0.06
60) Fluorene-d10	15.204	176	463185	35.689	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.351	200	97501	31.548	ng/ul	0.00
73) Anthracene-d10	17.092	188	885202	40.524	ng/ul	0.00
81) Pyrene-d10	19.486	212	1169186	43.897	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.427	264	1382417	42.990	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111924\
Data File : BP023255.D
Acq On : 20 Nov 2024 17:43
Operator : RC/JU
Sample : P4875-21
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E2A20

Manual IntegrationsAPPROVED

Quant Time: Nov 21 03:32:12 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 20 04:34:35 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/22/2024
Supervised By :mohammad ahmed 11/22/2024

