




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111924\
Data File : BP023267.D
Acq On : 21 Nov 2024 02:31
Operator : RC/JU
Sample : P4872-15
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E29Y2

Manual IntegrationsAPPROVED

Quant Time: Nov 21 03:19:38 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 20 04:34:35 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/22/2024
Supervised By :mohammad ahmed 11/22/2024

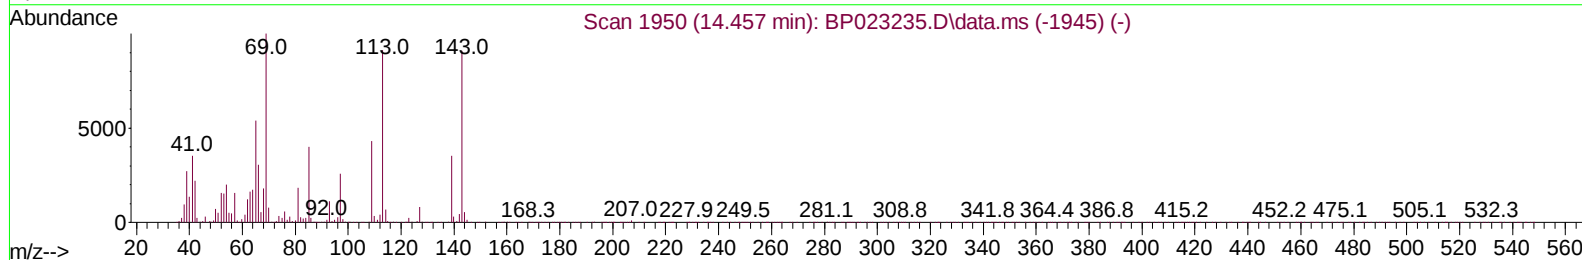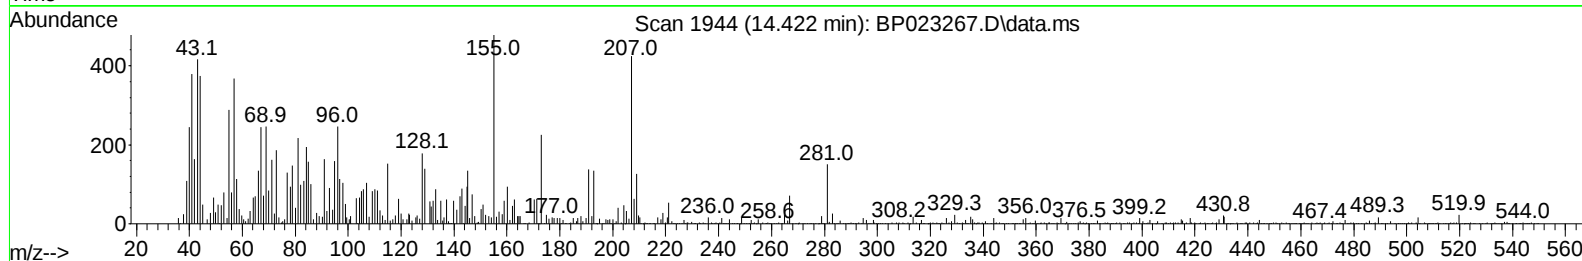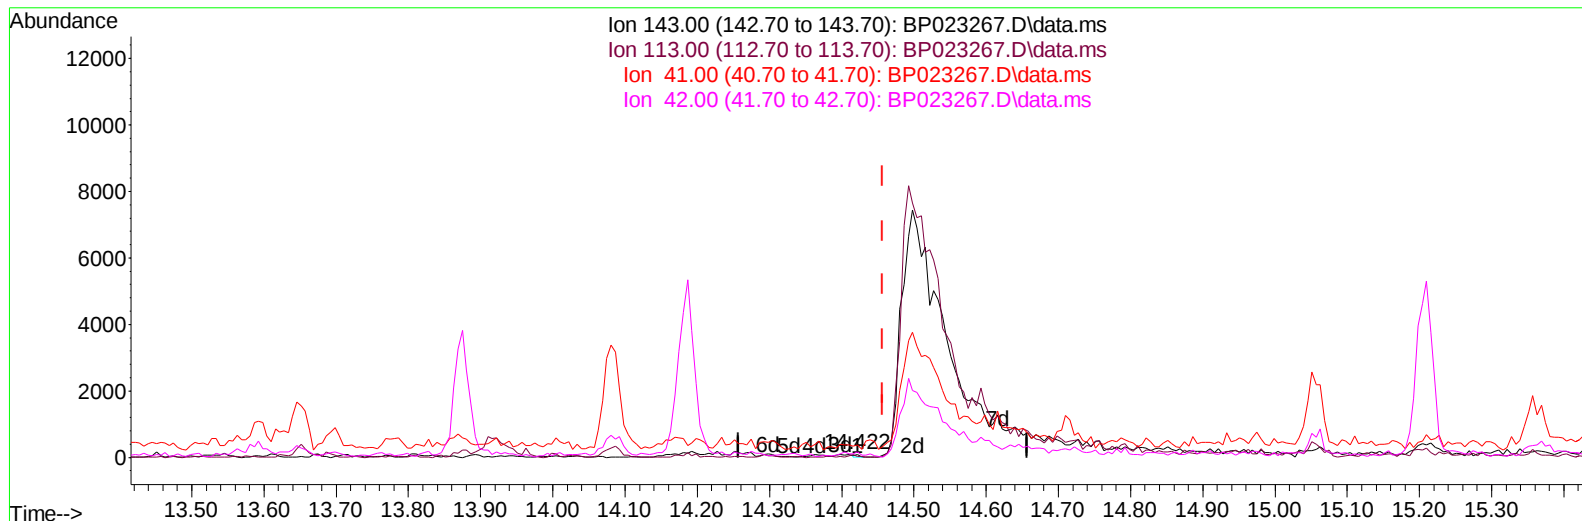

TIC: BP023267.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.422min (-0.035) 0.01 ng/u1

response 28

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	107.90	23.33#
41.00	39.20	421.11#
42.00	25.90	181.11#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111924\
Data File : BP023267.D
Acq On : 21 Nov 2024 02:31
Operator : RC/JU
Sample : P4872-15
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E29Y2

Manual IntegrationsAPPROVED

Quant Time: Nov 21 03:19:38 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 20 04:34:35 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/22/2024
Supervised By :mohammad ahmed 11/22/2024

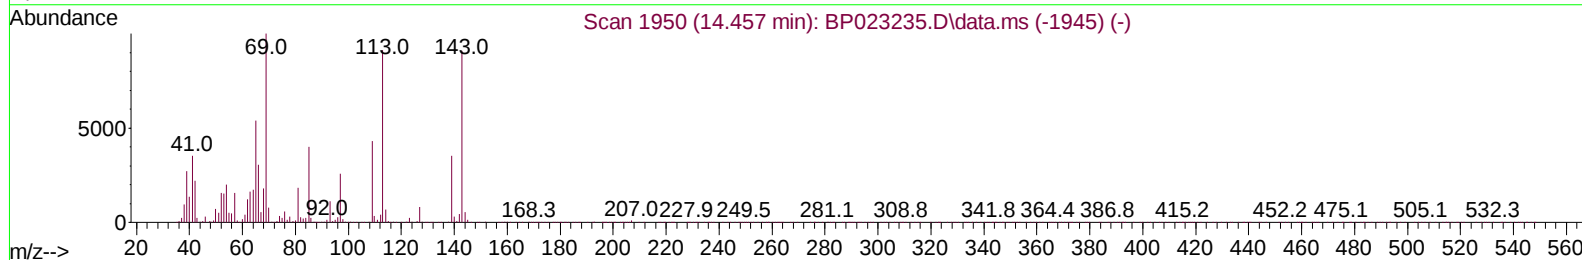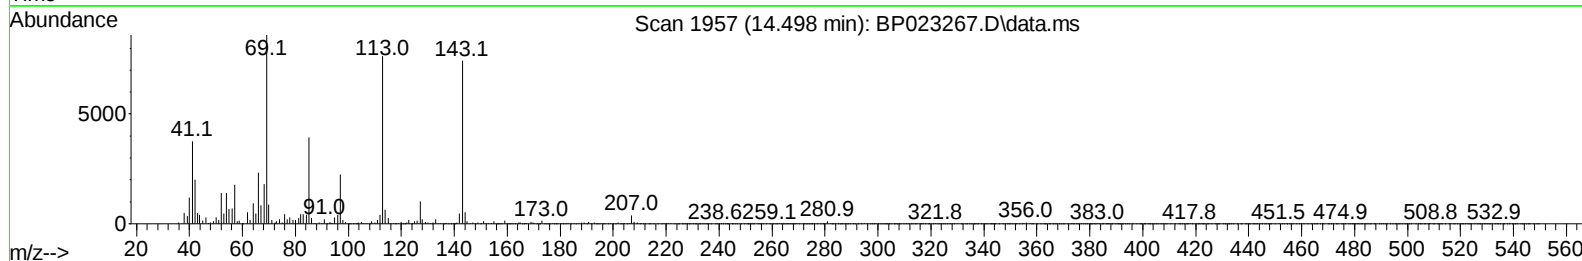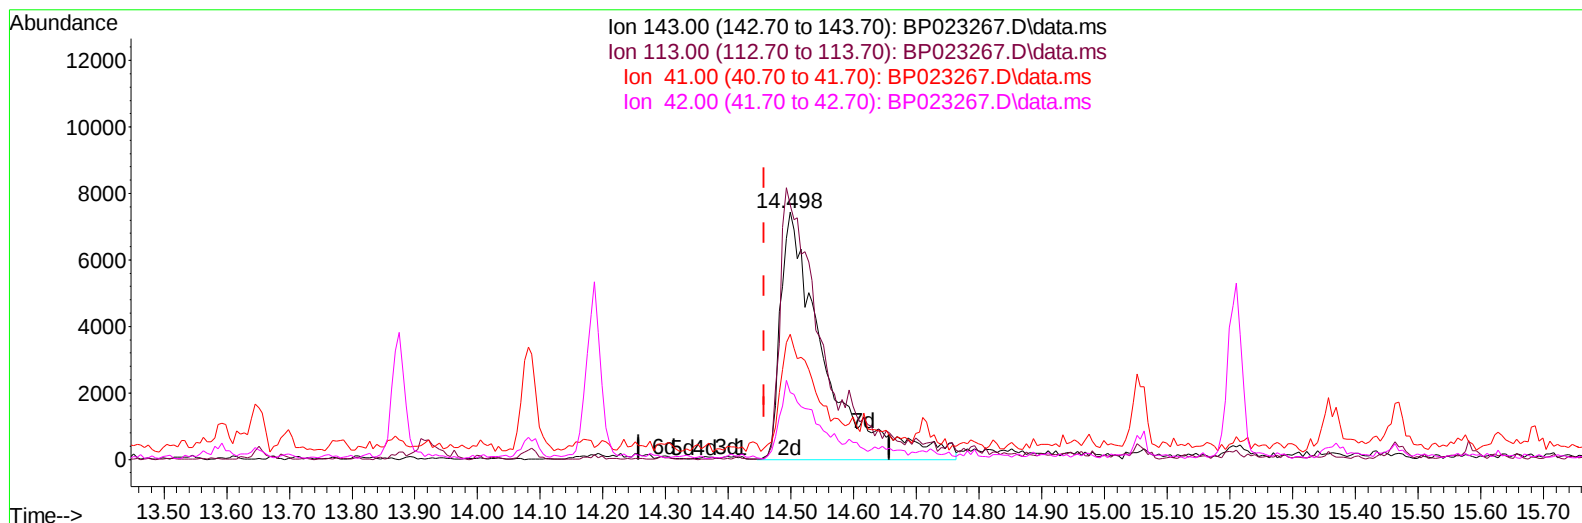

TIC: BP023267.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.498min (+ 0.041) 12.85 ng/ul m

response 36277

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	107.90	102.96
41.00	39.20	50.71#
42.00	25.90	27.19

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111924\
 Data File : BP023267.D
 Acq On : 21 Nov 2024 02:31
 Operator : RC/JU
 Sample : P4872-15
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E29Y2

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/22/2024
 Supervised By :mohammad ahmed 11/22/2024

Quant Time: Nov 21 03:20:30 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 20 04:34:35 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.569	152	93074	20.000	ng/ul	0.00
20) Naphthalene-d8	10.310	136	337634	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.186	164	260702	20.000	ng/ul	0.00
64) Phenanthrene-d10	16.998	188	620108	20.000	ng/ul	0.00
79) Chrysene-d12	21.427	240	744055	20.000	ng/ul	0.00
88) Perylene-d12	24.662	264	901706	20.000	ng/ul	0.03
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.134	96	6063	3.131	ng/uL	0.00
4) Pyridine-d5	3.552	84	64502	11.212	ng/ul	0.00
7) Phenol-d5	6.775	99	112961	16.416	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.916	67	70468	17.430	ng/ul	0.00
11) 2-Chlorophenol-d4	7.116	132	85672	17.000	ng/ul	0.00
15) 4-Methylphenol-d8	8.287	113	93650	16.538	ng/ul	0.00
21) Nitrobenzene-d5	8.710	128	42739	18.183	ng/ul	0.00
24) 2-Nitrophenol-d4	9.422	143	49191	17.554	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.969	165	99744	16.997	ng/ul	0.00
31) 4-Chloroaniline-d4	10.469	131	117718	16.814	ng/ul	0.00
46) Dimethylphthalate-d6	13.592	166	395608	21.055	ng/ul	0.00
49) Acenaphthylene-d8	13.875	160	393452	20.068	ng/ul	0.00
54) 4-Nitrophenol-d4	14.498	143	36277m	12.847	ng/ul	0.04
60) Fluorene-d10	15.210	176	343959	20.879	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.363	200	35483	9.552	ng/ul	0.01
73) Anthracene-d10	17.098	188	604450	23.021	ng/ul	0.00
81) Pyrene-d10	19.486	212	785194	22.911	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.439	264	1000385	23.291	ng/ul	0.02

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111924\
Data File : BP023267.D
Acq On : 21 Nov 2024 02:31
Operator : RC/JU
Sample : P4872-15
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E29Y2

Manual IntegrationsAPPROVED

Quant Time: Nov 21 03:20:30 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 20 04:34:35 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/22/2024
Supervised By :mohammad ahmed 11/22/2024

