




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111924\
 Data File : BP023273.D
 Acq On : 21 Nov 2024 06:34
 Operator : RC/JU
 Sample : P4872-21
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E29Y8

Manual IntegrationsAPPROVED

Quant Time: Nov 21 07:02:16 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 20 04:34:35 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/22/2024
 Supervised By :mohammad ahmed 11/22/2024

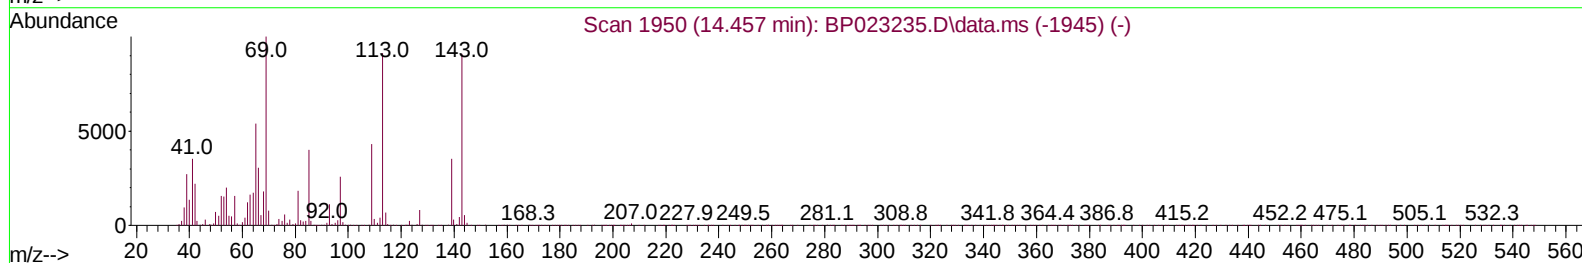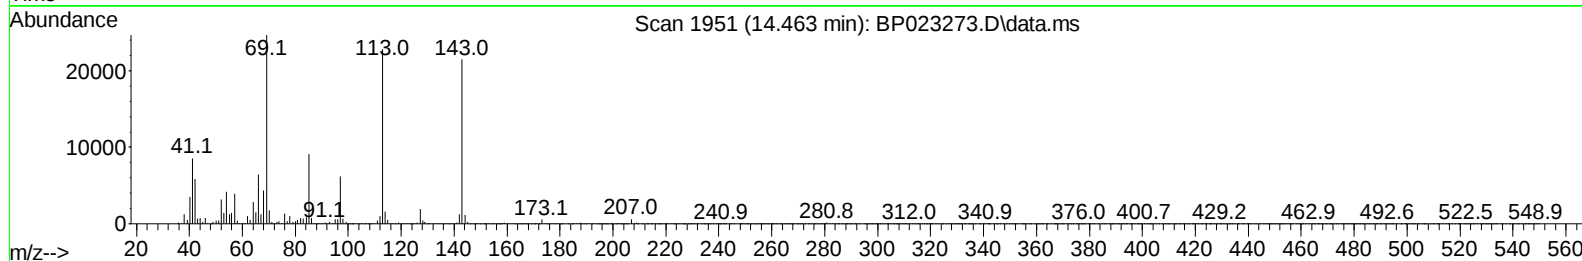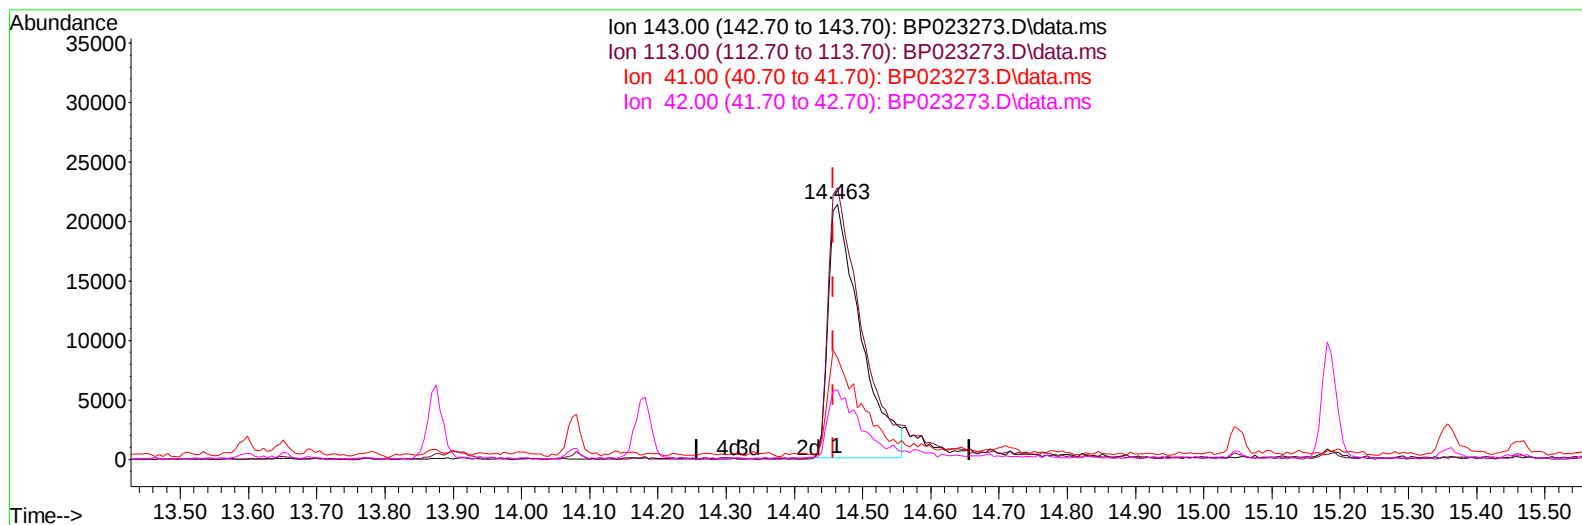

TIC: BP023273.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.463min (+ 0.006) 22.36 ng/u1

response 70595

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	107.90	106.41
41.00	39.20	39.81
42.00	25.90	27.35




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111924\
Data File : BP023273.D
Acq On : 21 Nov 2024 06:34
Operator : RC/JU
Sample : P4872-21
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E29Y8

Manual IntegrationsAPPROVED

Quant Time: Nov 21 07:02:16 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 20 04:34:35 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/22/2024
Supervised By :mohammad ahmed 11/22/2024

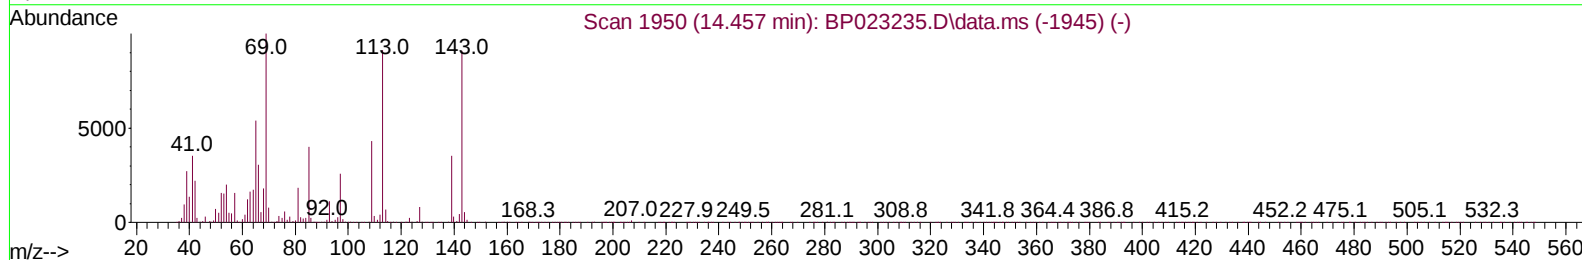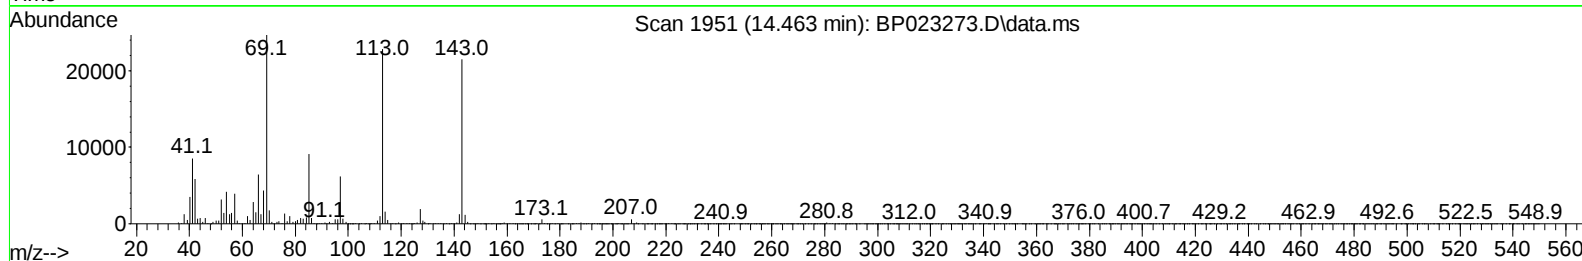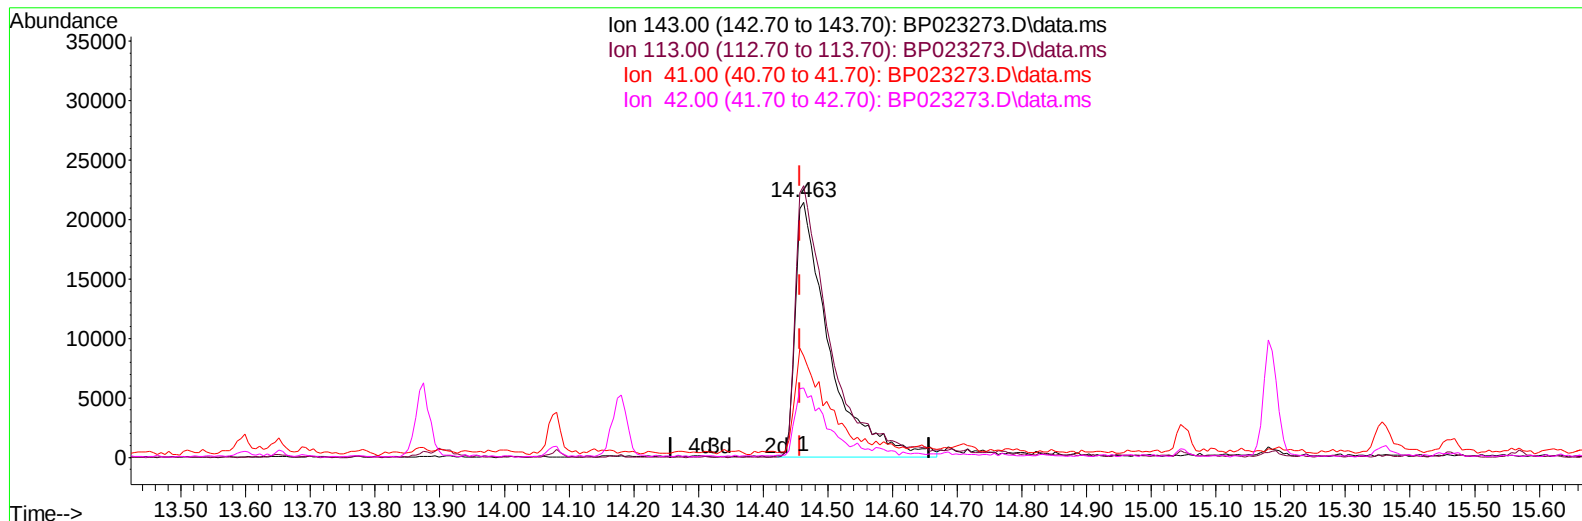

TIC: BP023273.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.463min (+ 0.006) 24.98 ng/ul m

response 78856

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	107.90	106.41
41.00	39.20	39.81
42.00	25.90	27.35

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111924\
 Data File : BP023273.D
 Acq On : 21 Nov 2024 06:34
 Operator : RC/JU
 Sample : P4872-21
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E29Y8

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/22/2024
 Supervised By :mohammad ahmed 11/22/2024

Quant Time: Nov 21 07:03:48 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 20 04:34:35 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.569	152	106062	20.000	ng/ul	0.00
20) Naphthalene-d8	10.316	136	389896	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.181	164	291498	20.000	ng/ul	0.00
64) Phenanthrene-d10	16.986	188	729230	20.000	ng/ul	-0.01
79) Chrysene-d12	21.433	240	843182	20.000	ng/ul	0.01
88) Perylene-d12	24.645	264	982184	20.000	ng/ul	0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.134	96	11128	5.043	ng/uL	0.00
4) Pyridine-d5	3.546	84	152268	23.227	ng/ul	0.00
7) Phenol-d5	6.775	99	223729	28.532	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.916	67	131998	28.652	ng/ul	0.00
11) 2-Chlorophenol-d4	7.116	132	163866	28.534	ng/ul	0.00
15) 4-Methylphenol-d8	8.281	113	189258	29.329	ng/ul	0.00
21) Nitrobenzene-d5	8.710	128	82338	30.334	ng/ul	0.00
24) 2-Nitrophenol-d4	9.416	143	99608	30.781	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.963	165	199905	29.499	ng/ul	0.00
31) 4-Chloroaniline-d4	10.469	131	231039	28.577	ng/ul	0.00
46) Dimethylphthalate-d6	13.598	166	714518	34.010	ng/ul	0.01
49) Acenaphthylene-d8	13.875	160	760140	34.676	ng/ul	0.00
54) 4-Nitrophenol-d4	14.463	143	78856m	24.976	ng/ul	0.00
60) Fluorene-d10	15.181	176	640129	34.752	ng/ul	-0.02
65) 4,6-Dinitro-2-methylph...	15.357	200	72675	16.636	ng/ul	0.00
73) Anthracene-d10	17.092	188	1086494	35.189	ng/ul	0.00
81) Pyrene-d10	19.480	212	1417025	36.486	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.421	264	1690704	36.138	ng/ul	0.00
Target Compounds						
					Qvalue	
8) Phenol	6.799	94	11033	1.347	ng/ul#	74

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111924\
Data File : BP023273.D
Acq On : 21 Nov 2024 06:34
Operator : RC/JU
Sample : P4872-21
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E29Y8

Manual IntegrationsAPPROVED

Quant Time: Nov 21 07:03:48 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 20 04:34:35 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/22/2024
Supervised By :mohammad ahmed 11/22/2024

