




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111924\
Data File : BP023274.D
Acq On : 21 Nov 2024 07:15
Operator : RC/JU
Sample : P4872-14
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E29Y1

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/22/2024
Supervised By :mohammad ahmed 11/22/2024

Quant Time: Nov 21 07:39:45 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 20 04:34:35 2024
Response via : Initial Calibration

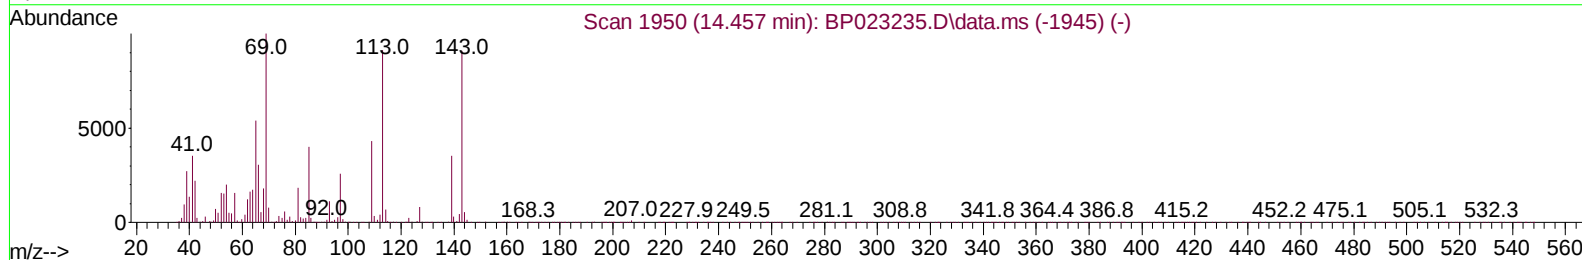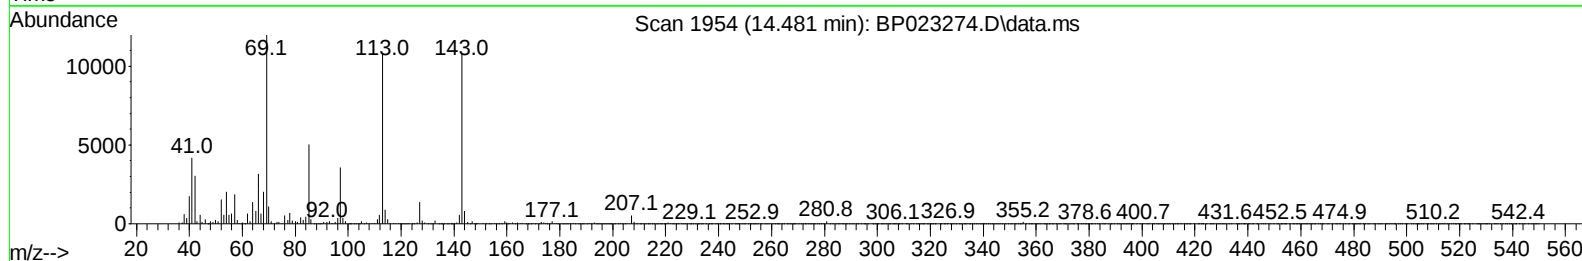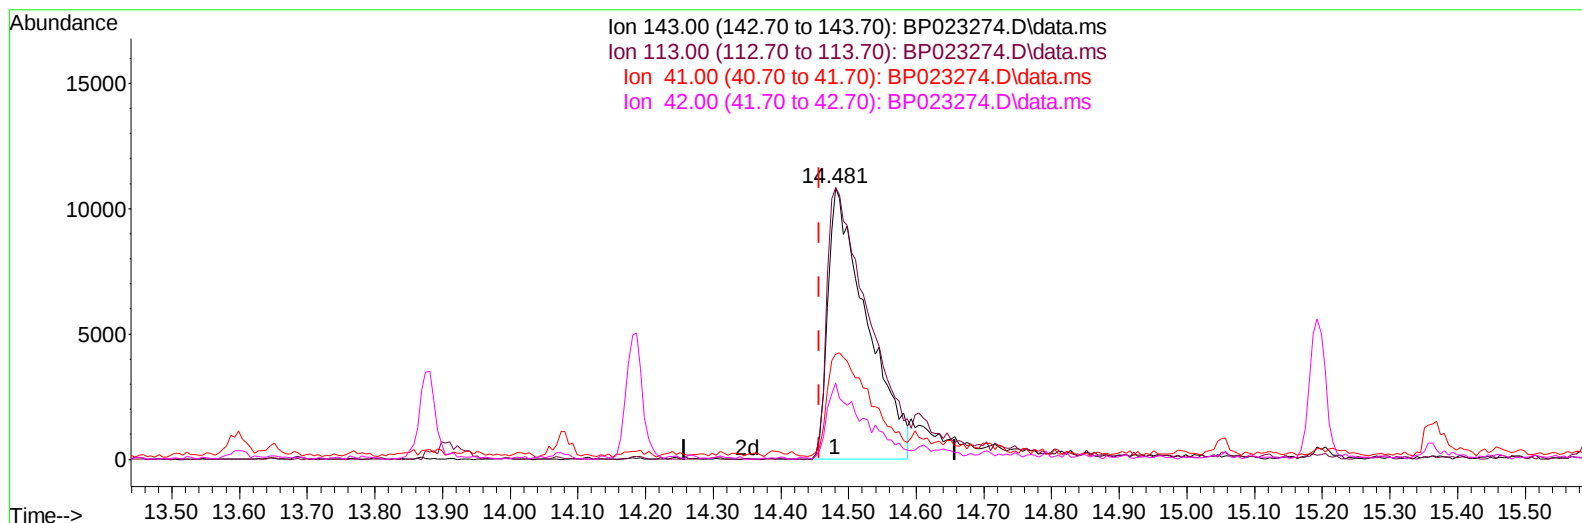

TIC: BP023274.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.481min (+ 0.024) 13.47 ng/u1

response 42696

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	107.90	100.03
41.00	39.20	38.75
42.00	25.90	28.14




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111924\
Data File : BP023274.D
Acq On : 21 Nov 2024 07:15
Operator : RC/JU
Sample : P4872-14
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E29Y1

Manual IntegrationsAPPROVED

Quant Time: Nov 21 07:39:45 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 20 04:34:35 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/22/2024
Supervised By :mohammad ahmed 11/22/2024

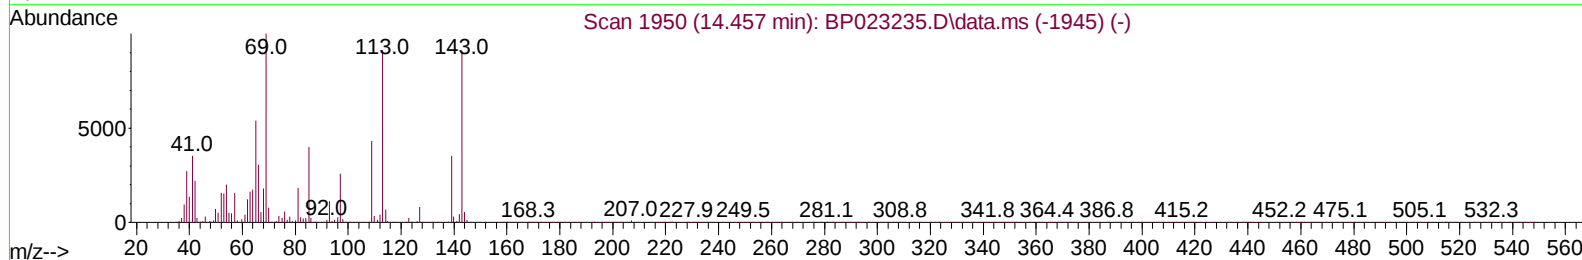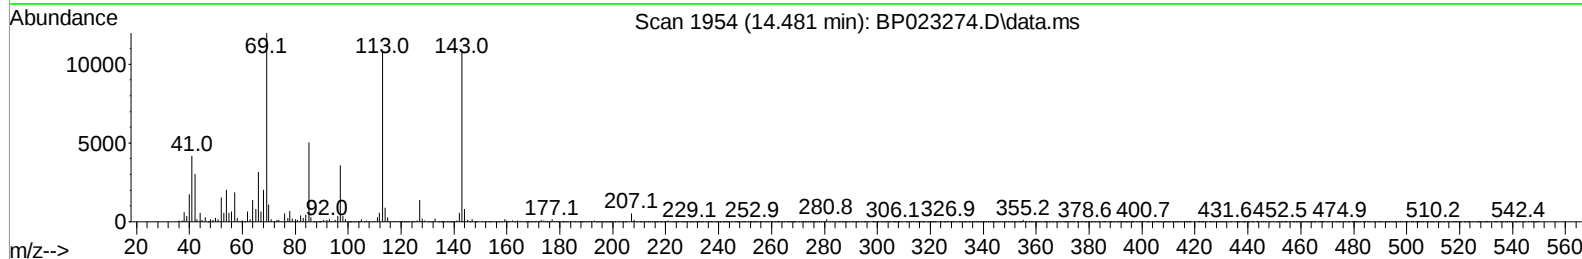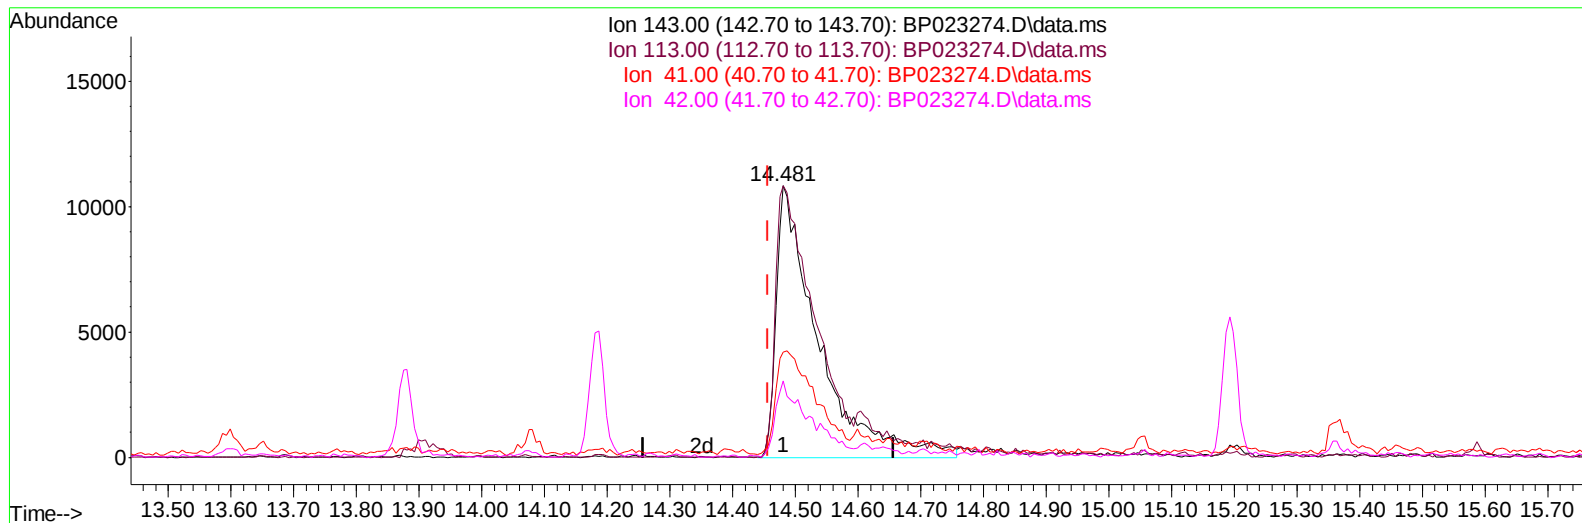

TIC: BP023274.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.481min (+ 0.024) 15.89 ng/ul m

response 50354

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	107.90	100.03
41.00	39.20	38.75
42.00	25.90	28.14

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111924\
 Data File : BP023274.D
 Acq On : 21 Nov 2024 07:15
 Operator : RC/JU
 Sample : P4872-14
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E29Y1

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/22/2024
 Supervised By :mohammad ahmed 11/22/2024

Quant Time: Nov 21 07:40:46 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 20 04:34:35 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.563	152	106890	20.000	ng/ul	0.00
20) Naphthalene-d8	10.310	136	386672	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.187	164	292625	20.000	ng/ul	0.00
64) Phenanthrene-d10	16.998	188	696839	20.000	ng/ul	0.00
79) Chrysene-d12	21.439	240	759151	20.000	ng/ul	0.02
88) Perylene-d12	24.668	264	882625	20.000	ng/ul	0.04
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.134	96	6329	2.846	ng/uL	0.00
4) Pyridine-d5	3.552	84	90226	13.656	ng/ul	0.00
7) Phenol-d5	6.769	99	131447	16.633	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.916	67	79527	17.128	ng/ul	0.00
11) 2-Chlorophenol-d4	7.111	132	101754	17.581	ng/ul	0.00
15) 4-Methylphenol-d8	8.281	113	110052	16.923	ng/ul	0.00
21) Nitrobenzene-d5	8.710	128	49796	18.498	ng/ul	0.00
24) 2-Nitrophenol-d4	9.422	143	59456	18.527	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.963	165	117778	17.525	ng/ul	0.00
31) 4-Chloroaniline-d4	10.469	131	137459	17.144	ng/ul	0.00
46) Dimethylphthalate-d6	13.598	166	462726	21.940	ng/ul	0.01
49) Acenaphthylene-d8	13.881	160	468334	21.282	ng/ul	0.00
54) 4-Nitrophenol-d4	14.481	143	50354m	15.887	ng/ul	0.02
60) Fluorene-d10	15.192	176	396782	21.458	ng/ul	-0.01
65) 4,6-Dinitro-2-methylph...	15.363	200	38808	9.297	ng/ul	0.01
73) Anthracene-d10	17.104	188	695894	23.586	ng/ul	0.00
81) Pyrene-d10	19.486	212	869080	24.854	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.445	264	1005140	23.908	ng/ul	0.02

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111924\
Data File : BP023274.D
Acq On : 21 Nov 2024 07:15
Operator : RC/JU
Sample : P4872-14
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E29Y1

Manual IntegrationsAPPROVED

Quant Time: Nov 21 07:40:46 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 20 04:34:35 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/22/2024
Supervised By :mohammad ahmed 11/22/2024

