

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111924\
 Data File : BP023214.D
 Acq On : 19 Nov 2024 11:53
 Operator : RC/JU
 Sample : PB165076BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK076

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP023214.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.140	22	26	32	rBV	23860	33728	1.20%	0.138%
2	3.552	92	96	115	rBV	228805	430097	15.25%	1.757%
3	3.852	144	147	155	rVB7	5793	10080	0.36%	0.041%
4	6.775	636	644	663	rBV	283496	576597	20.44%	2.356%
5	6.922	663	669	684	rVB	262240	418794	14.85%	1.711%
6	7.116	695	702	714	rBV	331764	584267	20.72%	2.387%
7	7.575	771	780	793	rBV	274673	514088	18.23%	2.100%
8	8.281	894	900	921	rBV	329878	706857	25.06%	2.888%
9	8.716	967	974	992	rBV	320525	583517	20.69%	2.384%
10	8.875	994	1001	1007	rBV5	9340	26225	0.93%	0.107%
11	9.428	1086	1095	1115	rBV	272933	519374	18.42%	2.122%
12	9.969	1178	1187	1213	rBV	321062	764720	27.12%	3.124%
13	10.163	1218	1220	1225	rVB6	2060	3496	0.12%	0.014%
14	10.316	1238	1246	1259	rBV	364692	649354	23.02%	2.653%
15	10.475	1265	1273	1293	rBV	297208	664122	23.55%	2.713%
16	11.940	1515	1522	1531	rBV6	5079	14183	0.50%	0.058%
17	13.604	1796	1805	1819	rBV	813608	1226175	43.48%	5.010%
18	13.875	1843	1851	1863	rBV	790189	1274570	45.19%	5.207%
19	14.181	1896	1903	1912	rBV	587890	920694	32.65%	3.761%
20	14.463	1945	1951	1955	rBV2	117484	262002	9.29%	1.070%
21	15.192	2069	2075	2087	rBV	1169514	1726935	61.23%	7.055%
22	15.363	2096	2104	2116	rBV	249842	524694	18.60%	2.144%
23	15.581	2135	2141	2144	rVB7	2467	3547	0.13%	0.014%
24	15.998	2208	2212	2216	rVV7	2003	3122	0.11%	0.013%
25	16.286	2257	2261	2265	rBV6	1983	3917	0.14%	0.016%
26	16.657	2321	2324	2328	rVB6	3071	4602	0.16%	0.019%
27	16.781	2342	2345	2350	rVB6	1915	3658	0.13%	0.015%
28	16.992	2375	2381	2391	rBV	949863	1234657	43.78%	5.044%
29	17.086	2391	2397	2416	rVV2	1101454	1999200	70.89%	8.168%
30	17.681	2495	2498	2504	rBV7	4363	7054	0.25%	0.029%
31	17.951	2538	2544	2552	rBV4	22957	55740	1.98%	0.228%
32	18.780	2683	2685	2687	rBV3	3150	2859	0.10%	0.012%
33	19.033	2724	2728	2733	rBV2	16305	25293	0.90%	0.103%
34	19.116	2738	2742	2746	rVB2	14297	21689	0.77%	0.089%
35	19.275	2766	2769	2775	rBV6	15633	21918	0.78%	0.090%
36	19.486	2799	2805	2820	rBV	1937894	2549872	90.41%	10.418%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111924\
Data File : BP023214.D
Acq On : 19 Nov 2024 11:53
Operator : RC/JU
Sample : PB165076BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK076

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Title : SVOA CALIBRATION

37	21.427	3130	3135	3147	rBV	913284	1560427	55.33%	6.375%
38	24.421	3634	3644	3658	rVB	1091560	2820268	100.00%	11.522%
39	24.645	3674	3682	3700	rVB	624646	1724402	61.14%	7.045%




Sum of corrected areas: 24476794

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111924\
Data File : BP023214.D
Acq On : 19 Nov 2024 11:53
Operator : RC/JU
Sample : PB165076BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK076

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

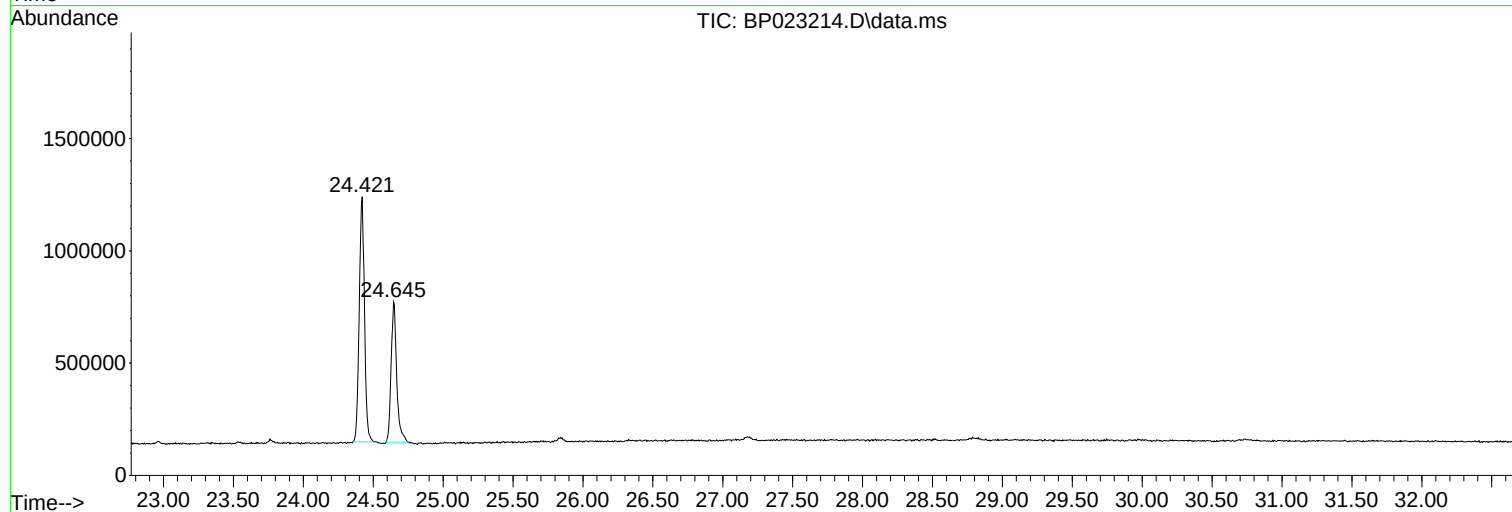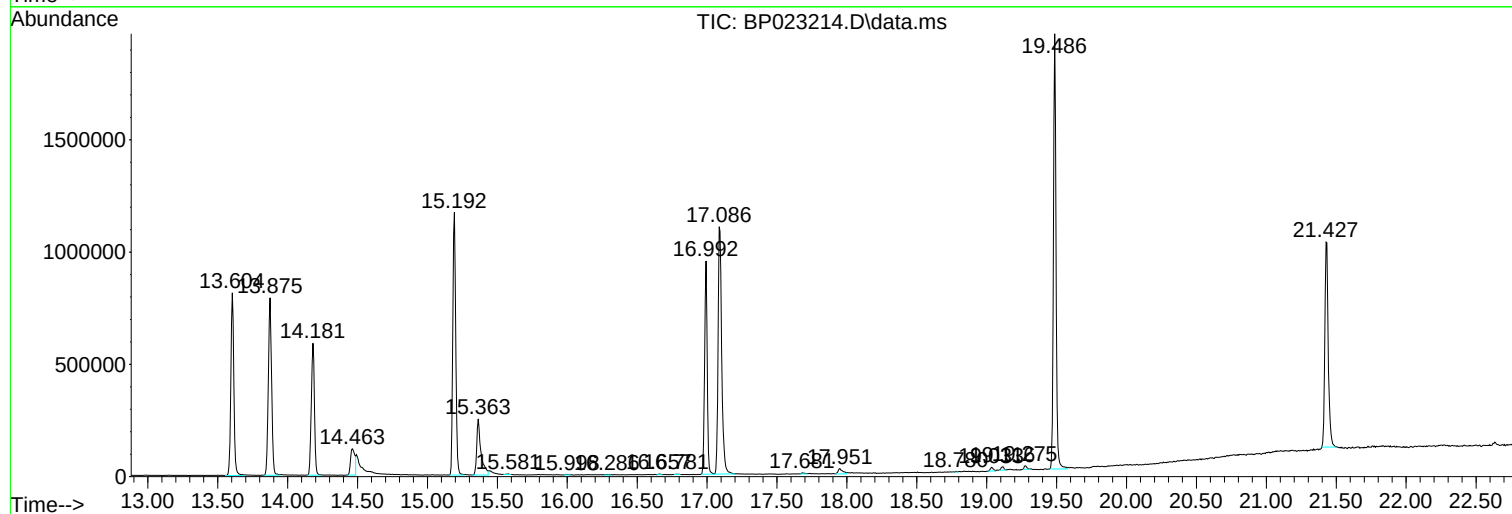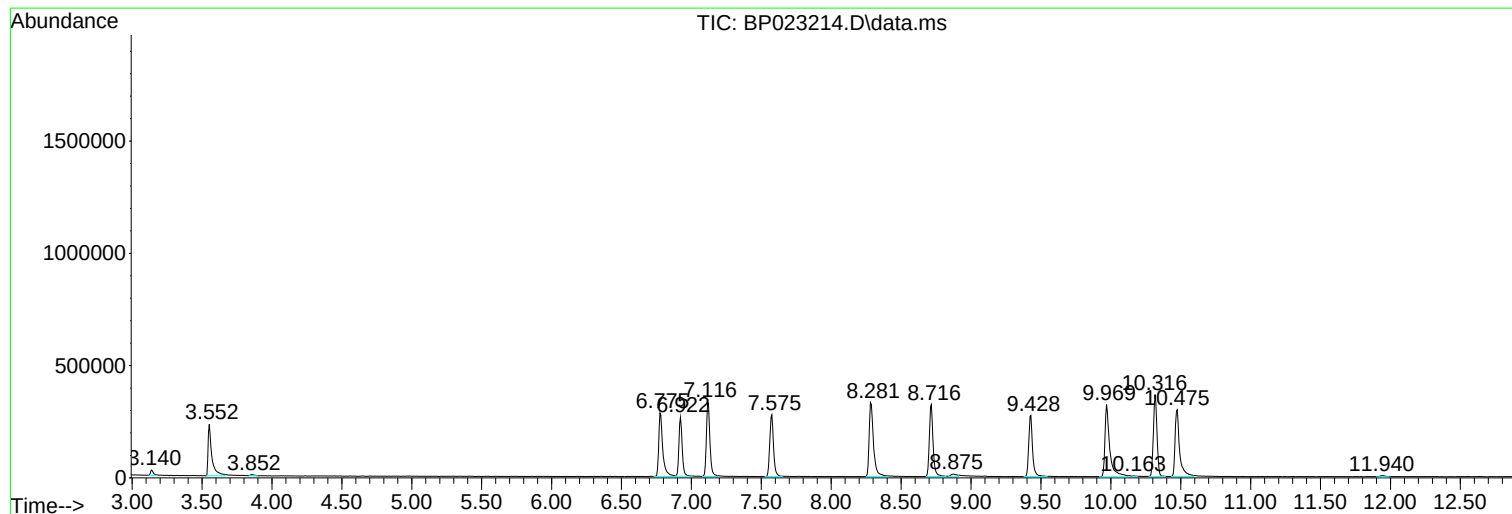

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111924\
Data File : BP023214.D
Acq On : 19 Nov 2024 11:53
Operator : RC/JU
Sample : PB165076BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK076

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111924\
Data File : BP023214.D
Acq On : 19 Nov 2024 11:53
Operator : RC/JU
Sample : PB165076BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK076

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc