

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111924\
 Data File : BP023218.D
 Acq On : 19 Nov 2024 15:17
 Operator : RC/JU
 Sample : P4875-11
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E29S9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP023218.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.140	21	26	30	rBV	15585	22369	0.70%	0.087%
2	3.564	95	98	116	rBV	57069	130591	4.06%	0.511%
3	3.858	144	148	156	rBV	15353	23916	0.74%	0.094%
4	4.281	215	220	225	rVB2	7704	11081	0.34%	0.043%
5	6.369	569	575	576	rBV6	3491	5002	0.16%	0.020%
6	6.399	578	580	586	rVB7	2680	4735	0.15%	0.019%
7	6.711	629	633	639	rBV2	5567	9004	0.28%	0.035%
8	6.787	639	646	663	rVV	62955	150089	4.67%	0.587%
9	6.922	663	669	684	rVB	248153	394996	12.28%	1.545%
10	7.122	696	703	717	rBV	286913	499816	15.54%	1.955%
11	7.563	772	778	787	rBV	285056	516511	16.06%	2.020%
12	7.646	787	792	799	rVB	15093	28583	0.89%	0.112%
13	8.287	894	901	918	rBV	216530	443161	13.78%	1.733%
14	8.399	918	920	926	rVB7	2524	4526	0.14%	0.018%
15	8.657	956	964	967	rBV6	3894	7897	0.25%	0.031%
16	8.710	967	973	994	rVB	314004	558311	17.36%	2.184%
17	9.099	1034	1039	1046	rVB7	4487	7584	0.24%	0.030%
18	9.422	1087	1094	1111	rBV	249496	514737	16.01%	2.013%
19	9.975	1179	1188	1208	rBV	329250	822731	25.59%	3.218%
20	10.169	1217	1221	1225	rVB7	3177	4166	0.13%	0.016%
21	10.316	1237	1246	1255	rBV	372480	675364	21.00%	2.641%
22	10.481	1265	1274	1291	rBV	210135	537018	16.70%	2.100%
23	11.569	1455	1459	1467	rVB9	2318	4706	0.15%	0.018%
24	11.946	1517	1523	1531	rVB3	4131	8778	0.27%	0.034%
25	12.781	1660	1665	1670	rBV9	2353	4716	0.15%	0.018%
26	13.034	1702	1708	1714	rBV6	3915	6896	0.21%	0.027%
27	13.157	1724	1729	1735	rBV7	6132	10389	0.32%	0.041%
28	13.604	1798	1805	1820	rBV	949283	1262179	39.25%	4.936%
29	13.798	1831	1838	1842	rBV3	6351	11221	0.35%	0.044%
30	13.881	1842	1852	1869	rVB	786512	1309954	40.74%	5.123%
31	14.145	1891	1897	1900	rBV2	118740	198106	6.16%	0.775%
32	14.193	1900	1905	1917	rVV	580924	1070173	33.28%	4.185%
33	14.281	1917	1920	1925	rVB4	13834	24476	0.76%	0.096%
34	14.516	1955	1960	1963	rBV5	20871	42398	1.32%	0.166%
35	14.681	1982	1988	1993	rBV6	15637	27916	0.87%	0.109%
36	15.004	2037	2043	2046	rBV5	3069	5333	0.17%	0.021%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111924\
 Data File : BP023218.D
 Acq On : 19 Nov 2024 15:17
 Operator : RC/JU
 Sample : P4875-11
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E29S9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
 Title : SVOA CALIBRATION

37	15.040	2047	2049	2055	rVB6	3540	5620	0.17%	0.022%
38	15.187	2068	2074	2096	rBV	1080994	1803700	56.09%	7.054%
39	15.369	2099	2105	2116	rBV2	268351	615850	19.15%	2.409%
40	15.592	2139	2143	2147	rVB7	3109	4873	0.15%	0.019%
41	15.734	2162	2167	2170	rVV6	4135	6123	0.19%	0.024%
42	15.781	2170	2175	2182	rVV9	8347	15309	0.48%	0.060%
43	15.992	2206	2211	2219	rBV	37252	56241	1.75%	0.220%
44	16.075	2219	2225	2229	rBV	14711	34724	1.08%	0.136%
45	16.569	2307	2309	2315	rVB6	3407	5126	0.16%	0.020%
46	16.992	2371	2381	2392	rBV	846524	1297714	40.36%	5.075%
47	17.104	2393	2400	2414	rBV2	1378080	2242007	69.72%	8.769%
48	17.581	2477	2481	2486	rBV	6313	10713	0.33%	0.042%
49	17.686	2494	2499	2504	rBV	131059	160957	5.01%	0.630%
50	17.939	2537	2542	2549	rBV4	41339	78763	2.45%	0.308%
51	18.386	2614	2618	2624	rBV9	4056	7054	0.22%	0.028%
52	19.033	2724	2728	2731	rBV	24947	34504	1.07%	0.135%
53	19.063	2731	2733	2737	rVB5	10789	11100	0.35%	0.043%
54	19.110	2737	2741	2745	rBV	16690	26067	0.81%	0.102%
55	19.280	2765	2770	2776	rBV7	29791	57139	1.78%	0.223%
56	19.486	2799	2805	2821	rVB	2163515	2920592	90.82%	11.423%
57	19.757	2847	2851	2857	rBV6	12479	21524	0.67%	0.084%
58	21.439	3131	3137	3149	rVB	899740	1665512	51.79%	6.514%
59	22.639	3338	3341	3350	rVB3	43703	65429	2.03%	0.256%
60	24.427	3637	3645	3658	rVB	1175992	3215640	100.00%	12.576%
61	24.657	3676	3684	3704	rVB	630065	1846943	57.44%	7.223%




Sum of corrected areas: 25568653

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111924\
Data File : BP023218.D
Acq On : 19 Nov 2024 15:17
Operator : RC/JU
Sample : P4875-11
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E29S9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

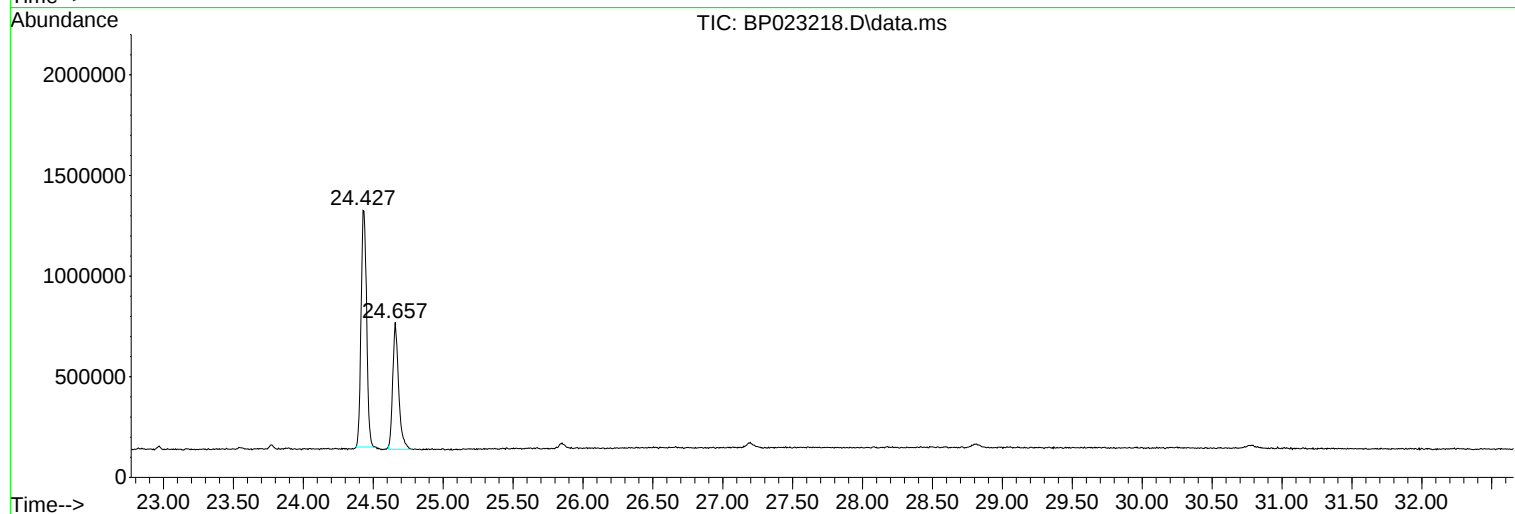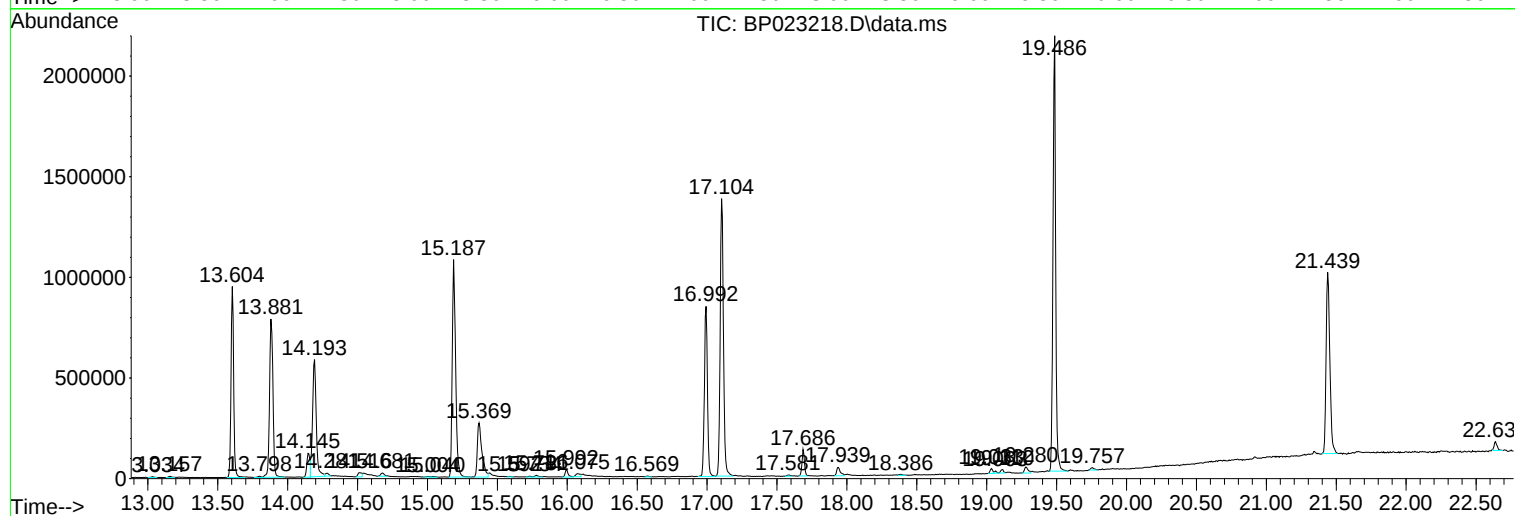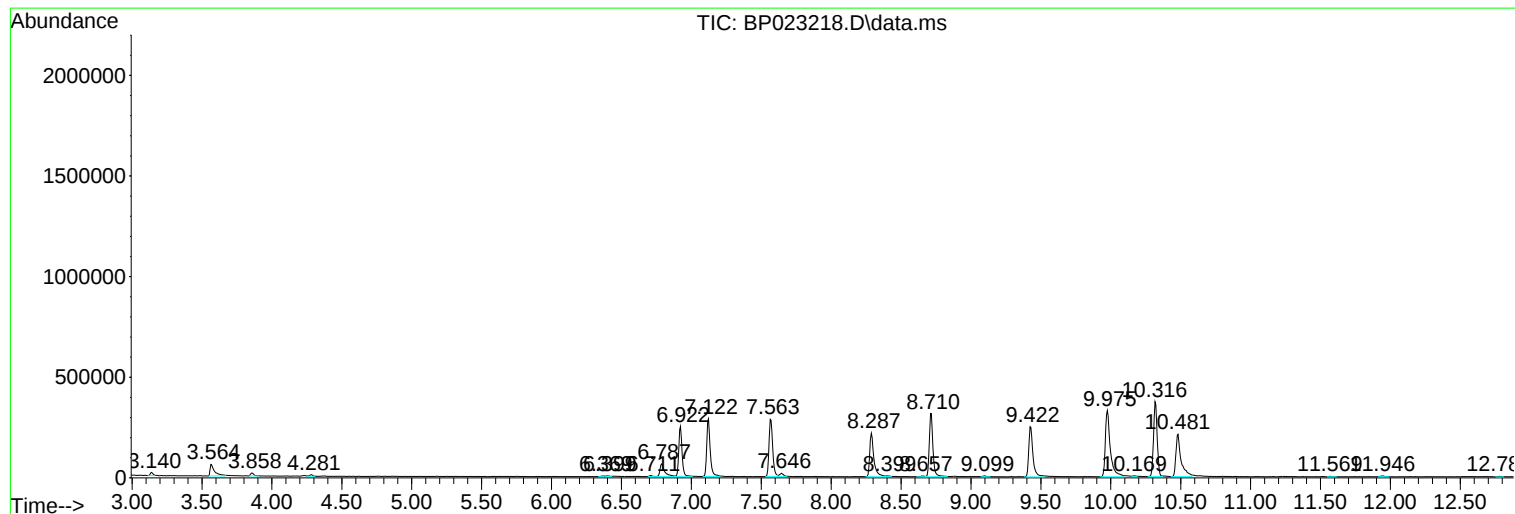

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111924\
Data File : BP023218.D
Acq On : 19 Nov 2024 15:17
Operator : RC/JU
Sample : P4875-11
Misc :
ALS Vial : 8 Sample Multiplier: 1










Instrument :
BNA_P
ClientSampleId :
E29S9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 7,9-Di-tert-butyl-1-oxaspiro... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.	
17.686	2.48 ng/ul	160957	Phenanthrene-d10	16.992	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	7,9-Di-tert-butyl-1-oxaspiro(4,5...	276	C17H24O3	082304-66-3	98
2	7,9-Di-tert-butyl-1-oxaspiro(4,5...	276	C17H24O3	082304-66-3	95
3	7,9-Di-tert-butyl-1-oxaspiro(4,5...	276	C17H24O3	082304-66-3	93
4	9-Ethyl-10-methylantracene	220	C17H16	019713-49-6	38
5	Butylated Hydroxytoluene	220	C15H24O	000128-37-0	38

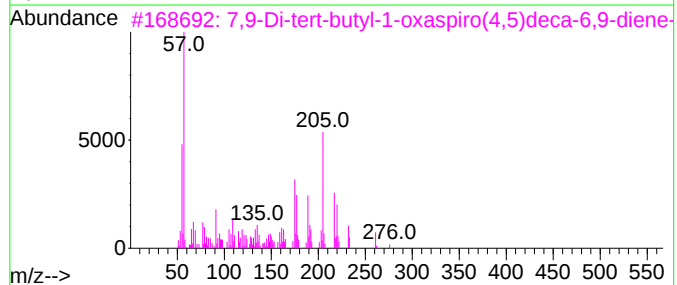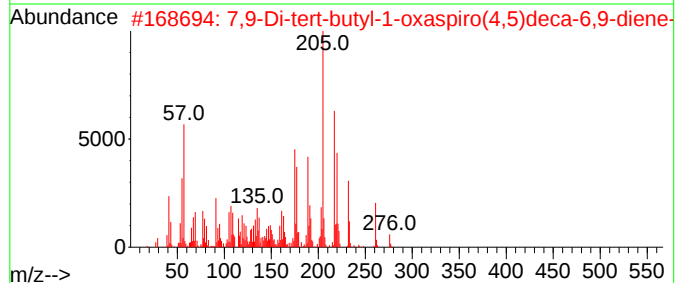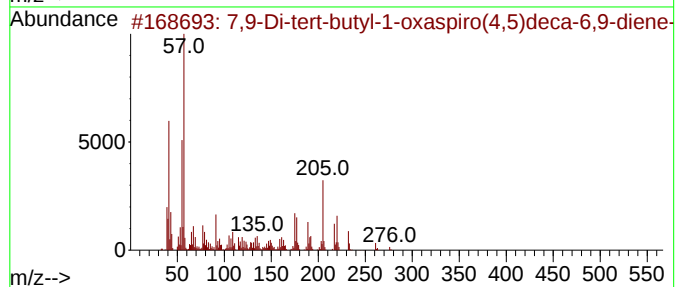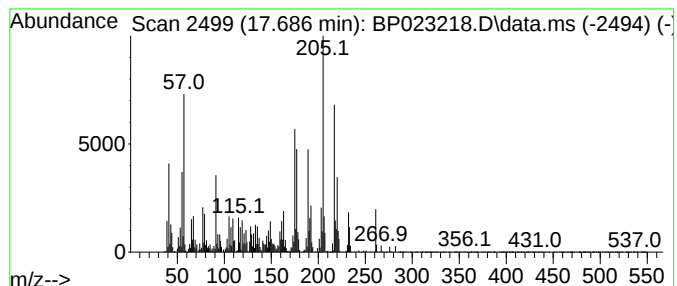

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111924\
Data File : BP023218.D
Acq On : 19 Nov 2024 15:17
Operator : RC/JU
Sample : P4875-11
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E29S9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
7,9-Di-tert-but...	17.686	2.5	ng/u1	160957	4	16.992	1297710	20.0