

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111924\
 Data File : BP023225.D
 Acq On : 19 Nov 2024 20:02
 Operator : RC/JU
 Sample : P4875-04
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E29Z7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP023225.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.140	22	26	33	rVB	15014	23174	0.81%	0.107%
2	3.475	78	83	91	rBV10	1157	3173	0.11%	0.015%
3	3.564	95	98	110	rBV	40053	90239	3.17%	0.418%
4	3.858	145	148	152	rVB	4371	5578	0.20%	0.026%
5	4.281	217	220	224	rVB	3395	4465	0.16%	0.021%
6	6.710	629	633	640	rVB5	2343	4634	0.16%	0.021%
7	6.787	640	646	663	rBV2	96990	224434	7.87%	1.039%
8	6.916	663	668	680	rVB	197594	310473	10.89%	1.438%
9	7.122	696	703	721	rBV	255417	440364	15.45%	2.039%
10	7.569	773	779	794	rBV	276349	476611	16.72%	2.207%
11	8.281	892	900	920	rBV	223904	485346	17.03%	2.248%
12	8.722	968	975	993	rBV	241883	447361	15.70%	2.072%
13	9.104	1037	1040	1046	rVB4	5108	7106	0.25%	0.033%
14	9.434	1088	1096	1112	rBV	205468	393310	13.80%	1.822%
15	9.975	1181	1188	1213	rBV	256152	592899	20.80%	2.746%
16	10.316	1240	1246	1257	rVB	362605	596984	20.94%	2.765%
17	10.481	1267	1274	1292	rBV	188480	461083	16.18%	2.135%
18	11.963	1515	1526	1529	rBV7	3265	6854	0.24%	0.032%
19	13.598	1796	1804	1817	rBV	560512	1025306	35.97%	4.749%
20	13.875	1842	1851	1866	rBV	651698	1022358	35.87%	4.735%
21	14.192	1898	1905	1915	rVV	606291	875860	30.73%	4.056%
22	14.263	1915	1917	1925	rVB8	2042	4148	0.15%	0.019%
23	14.510	1953	1959	1975	rBV4	35497	132352	4.64%	0.613%
24	14.686	1985	1989	1997	rVB10	3657	6442	0.23%	0.030%
25	15.210	2071	2078	2087	rBV	1157252	1453480	50.99%	6.732%
26	15.357	2097	2103	2119	rBV2	254186	531327	18.64%	2.461%
27	15.592	2138	2143	2147	rBV	31426	45243	1.59%	0.210%
28	16.010	2211	2214	2217	rVB5	2301	3456	0.12%	0.016%
29	16.169	2235	2241	2248	rVB7	3218	6080	0.21%	0.028%
30	16.416	2280	2283	2287	rBV6	1878	3158	0.11%	0.015%
31	16.675	2324	2327	2332	rVB6	2267	3437	0.12%	0.016%
32	16.780	2343	2345	2351	rVB5	2157	3129	0.11%	0.014%
33	16.880	2358	2362	2367	rVB7	2329	3929	0.14%	0.018%
34	17.004	2377	2383	2393	rBV	847245	1176465	41.28%	5.449%
35	17.098	2393	2399	2416	rVV	1249364	1855766	65.11%	8.595%
36	17.227	2420	2421	2425	rVB4	4127	3025	0.11%	0.014%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111924\
Data File : BP023225.D
Acq On : 19 Nov 2024 20:02
Operator : RC/JU
Sample : P4875-04
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E29Z7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M

Title : SVOA CALIBRATION

37	17.375	2443	2446	2450	rBV5	4604	6850	0.24%	0.032%
38	17.933	2536	2541	2557	rBV5	32087	66156	2.32%	0.306%
39	18.310	2601	2605	2606	rBV4	3455	4568	0.16%	0.021%
40	18.480	2631	2634	2635	rBV3	5203	5135	0.18%	0.024%
41	19.033	2723	2728	2734	rBV3	16747	28032	0.98%	0.130%
42	19.122	2739	2743	2746	rBV	14940	20467	0.72%	0.095%
43	19.280	2766	2770	2778	rBV8	16891	29275	1.03%	0.136%
44	19.492	2799	2806	2816	rBV2	1558720	2449056	85.92%	11.342%
45	21.439	3131	3137	3149	rBV2	1005919	1580684	55.46%	7.321%
46	24.427	3636	3645	3657	rBV	1159814	2850267	100.00%	13.200%
47	24.651	3675	3683	3704	rVB2	526733	1822645	63.95%	8.441%




Sum of corrected areas: 21592184

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111924\
Data File : BP023225.D
Acq On : 19 Nov 2024 20:02
Operator : RC/JU
Sample : P4875-04
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E29Z7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

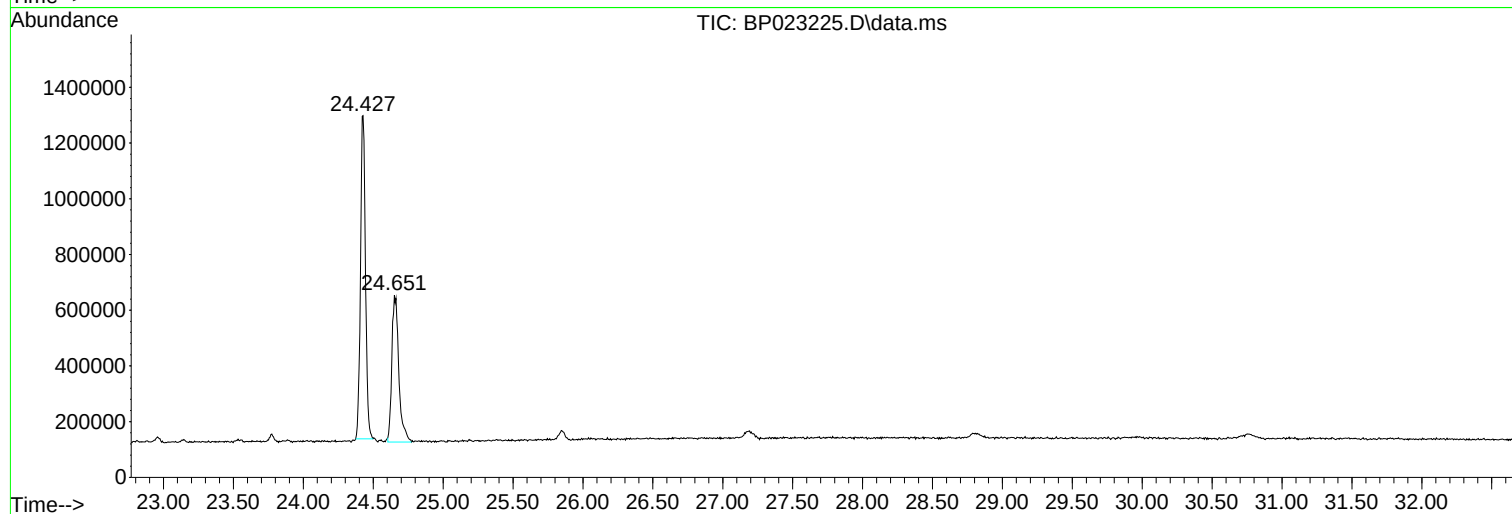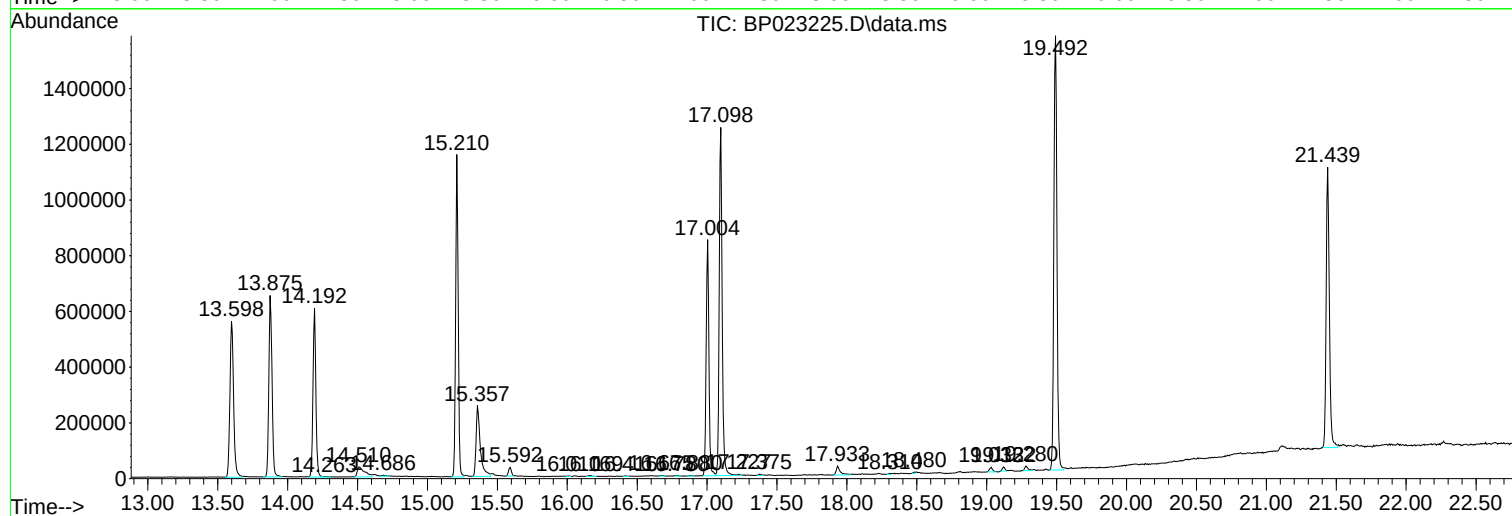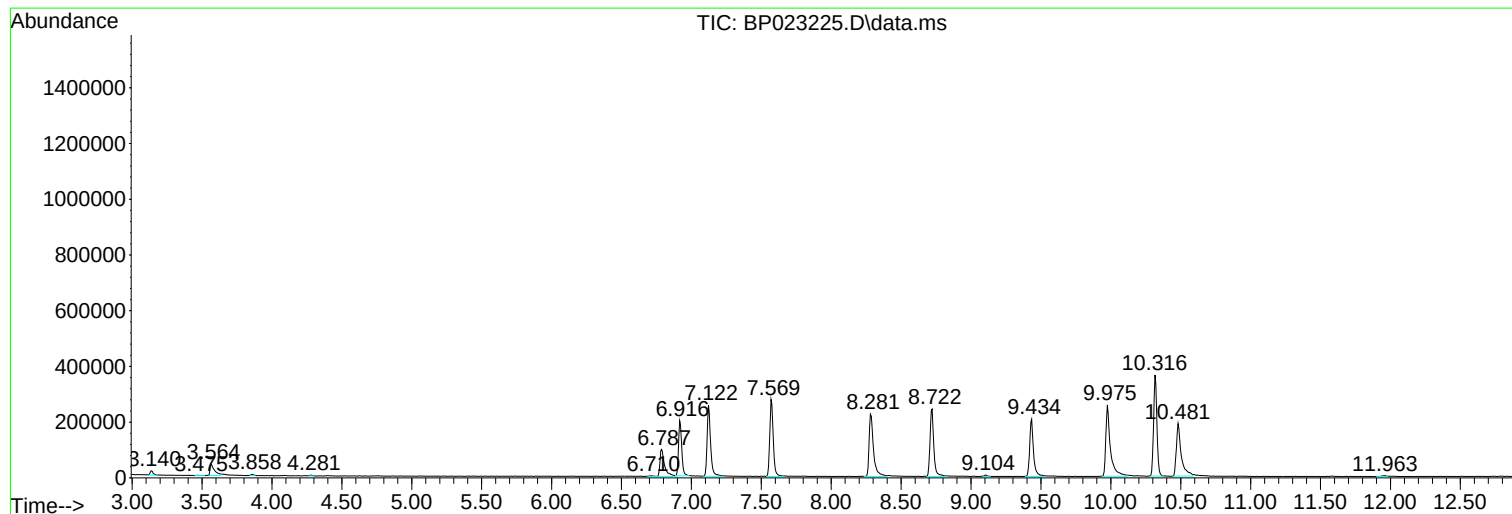

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111924\
Data File : BP023225.D
Acq On : 19 Nov 2024 20:02
Operator : RC/JU
Sample : P4875-04
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E29Z7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111924\
Data File : BP023225.D
Acq On : 19 Nov 2024 20:02
Operator : RC/JU
Sample : P4875-04
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E29Z7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc