

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111924\
 Data File : BP023228.D
 Acq On : 19 Nov 2024 22:04
 Operator : RC/JU
 Sample : P4875-09
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E2A23

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP023228.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.140	22	26	34	rVB	15924	23084	0.69%	0.095%
2	3.858	144	148	155	rVB	18177	27038	0.81%	0.111%
3	4.217	207	209	215	rVV6	4553	7184	0.21%	0.030%
4	4.281	215	220	224	rVB3	3955	6007	0.18%	0.025%
5	4.369	231	235	240	rVB8	2986	4388	0.13%	0.018%
6	6.781	639	645	658	rBV	103155	220828	6.60%	0.910%
7	6.922	663	669	678	rBV	238805	392551	11.74%	1.618%
8	7.116	696	702	725	rVV	339877	559325	16.72%	2.306%
9	7.569	770	779	788	rBV	248994	463759	13.86%	1.912%
10	7.646	788	792	802	rVB2	13259	29842	0.89%	0.123%
11	8.281	893	900	920	rBV2	239575	548891	16.41%	2.263%
12	8.652	958	963	967	rBV6	4284	7997	0.24%	0.033%
13	8.716	967	974	989	rVV	291008	570935	17.07%	2.354%
14	8.875	998	1001	1008	rVB8	3711	6199	0.19%	0.026%
15	9.105	1036	1040	1045	rVB8	2614	4562	0.14%	0.019%
16	9.428	1087	1095	1118	rBV	265224	535407	16.01%	2.207%
17	9.975	1180	1188	1213	rBV	286768	757673	22.65%	3.124%
18	10.322	1239	1247	1255	rBV	340689	580687	17.36%	2.394%
19	10.510	1272	1279	1299	rBV3	29604	101050	3.02%	0.417%
20	11.946	1516	1523	1529	rBV8	4122	9993	0.30%	0.041%
21	12.781	1657	1665	1674	rVB8	2079	4346	0.13%	0.018%
22	13.040	1706	1709	1715	rVB5	3251	5339	0.16%	0.022%
23	13.210	1733	1738	1743	rBV8	1786	4041	0.12%	0.017%
24	13.604	1797	1805	1818	rBV	713930	1321019	39.49%	5.446%
25	13.869	1839	1850	1864	rBV	855805	1336189	39.95%	5.509%
26	14.181	1896	1903	1913	rBV	601595	879200	26.28%	3.625%
27	14.269	1915	1918	1925	rVB7	5283	8448	0.25%	0.035%
28	14.498	1950	1957	1972	rBV3	43971	168336	5.03%	0.694%
29	14.675	1985	1987	1991	rVB4	3783	3892	0.12%	0.016%
30	14.875	2017	2021	2027	rBV6	2308	3642	0.11%	0.015%
31	15.198	2070	2076	2088	rBV	1622216	1893842	56.62%	7.807%
32	15.357	2096	2103	2118	rBV	270812	604490	18.07%	2.492%
33	15.457	2118	2120	2136	rVV8	16909	45346	1.36%	0.187%
34	16.581	2307	2311	2316	rVB6	3178	4745	0.14%	0.020%
35	16.663	2321	2325	2330	rVB8	2138	3385	0.10%	0.014%
36	16.786	2341	2346	2349	rBV6	2340	4222	0.13%	0.017%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111924\
Data File : BP023228.D
Acq On : 19 Nov 2024 22:04
Operator : RC/JU
Sample : P4875-09
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E2A23

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Title : SVOA CALIBRATION

37	16.986	2375	2380	2391	rVB	829073	1122342	33.55%	4.627%
38	17.098	2391	2399	2419	rVV2	1184592	2250426	67.28%	9.278%
39	17.239	2419	2423	2429	rVB9	5156	8188	0.24%	0.034%
40	17.686	2493	2499	2505	rBV	99841	146573	4.38%	0.604%
41	17.957	2541	2545	2549	rBV5	7893	13476	0.40%	0.056%
42	18.192	2575	2585	2587	rBV5	4413	7412	0.22%	0.031%
43	19.033	2723	2728	2733	rVB3	19490	32357	0.97%	0.133%
44	19.110	2737	2741	2747	rVB	18391	26715	0.80%	0.110%
45	19.286	2768	2771	2776	rBV6	6287	7412	0.22%	0.031%
46	19.486	2798	2805	2817	rBV	1963266	2930396	87.60%	12.081%
47	21.433	3131	3136	3149	rVB2	963284	1529427	45.72%	6.305%
48	24.410	3633	3642	3659	rVB	1250237	3345027	100.00%	13.790%
49	24.645	3673	3682	3703	rVB	561112	1689122	50.50%	6.964%




Sum of corrected areas: 24256755

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111924\
Data File : BP023228.D
Acq On : 19 Nov 2024 22:04
Operator : RC/JU
Sample : P4875-09
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E2A23

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

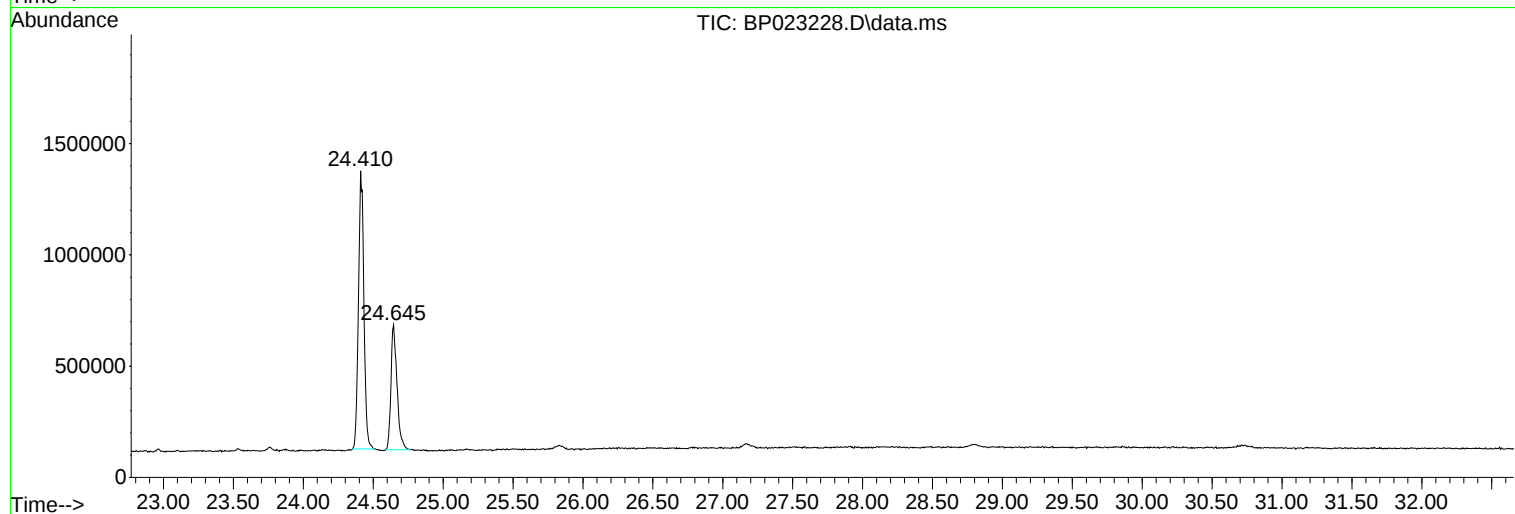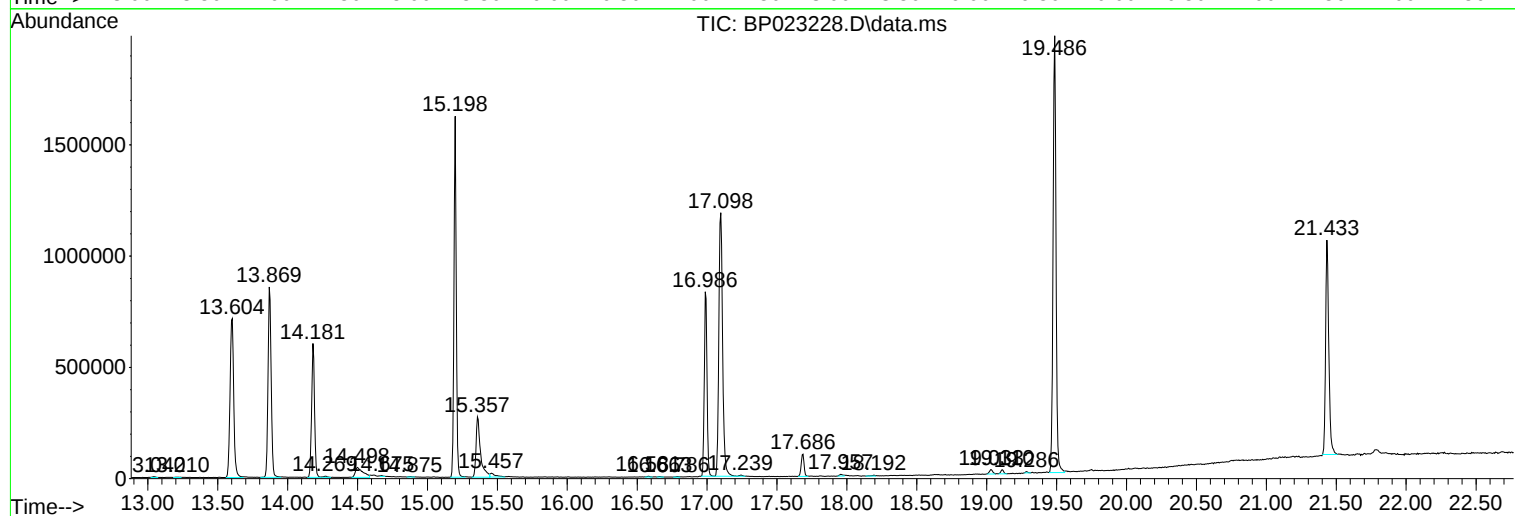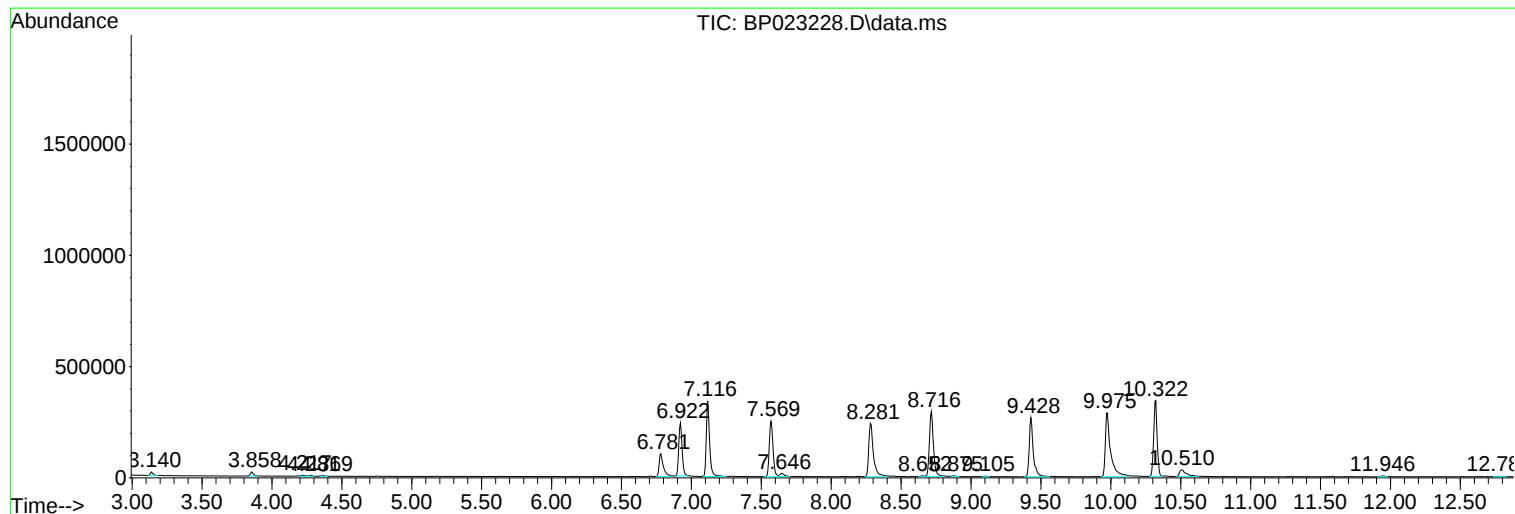

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111924\
Data File : BP023228.D
Acq On : 19 Nov 2024 22:04
Operator : RC/JU
Sample : P4875-09
Misc :
ALS Vial : 17 Sample Multiplier: 1










Instrument :
BNA_P
ClientSampleId :
E2A23

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 7,9-Di-tert-butyl-1-oxaspiro... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.	
17.686	2.61 ng/ul	146573	Phenanthrene-d10	16.986	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	7,9-Di-tert-butyl-1-oxaspiro(4,5...	276	C17H24O3	082304-66-3	99
2	7,9-Di-tert-butyl-1-oxaspiro(4,5...	276	C17H24O3	082304-66-3	98
3	7,9-Di-tert-butyl-1-oxaspiro(4,5...	276	C17H24O3	082304-66-3	92
4	(1R,3aR,5aR,9aS)-1,4,4,7-Tetrame...	220	C15H24O	104188-25-2	64
5	2,5-Cyclohexadien-1-one, 2,6-bis...	232	C16H24O	006738-27-8	47

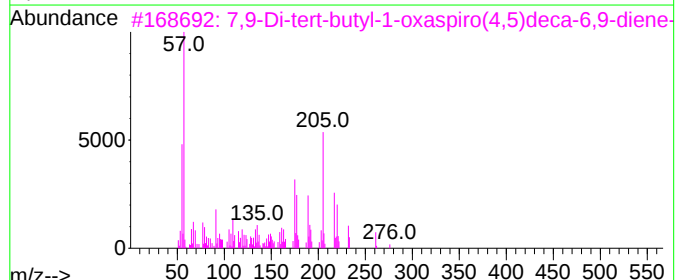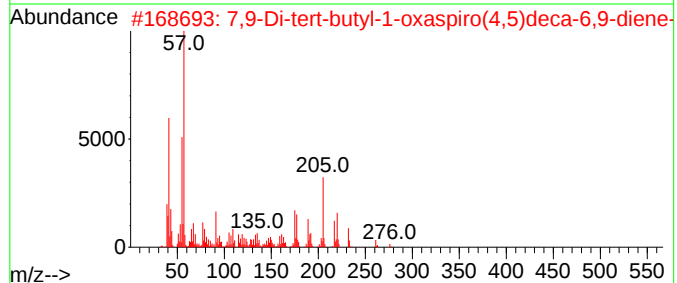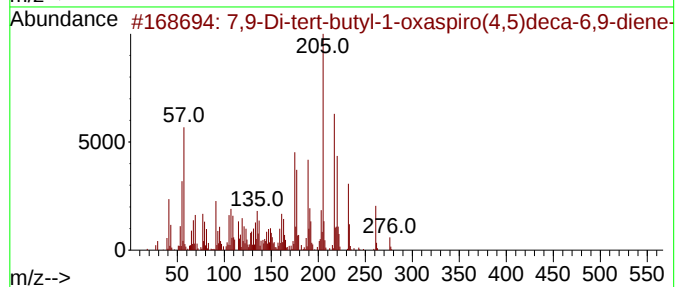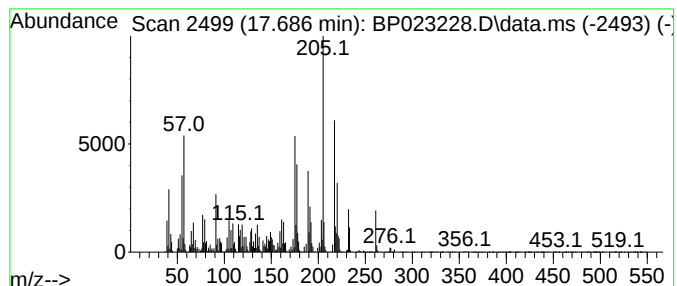

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111924\
Data File : BP023228.D
Acq On : 19 Nov 2024 22:04
Operator : RC/JU
Sample : P4875-09
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E2A23

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
7,9-Di-tert-but...	17.686	2.6	ng/ul	146573	4	16.986	1122340	20.0