

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111924\
 Data File : BP023236.D
 Acq On : 20 Nov 2024 04:08
 Operator : RC/JU
 Sample : PB165061BL
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK061

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP023236.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.134	22	25	35	rVB	25567	38966	1.25%	0.144%
2	3.546	92	95	121	rBV	250518	478266	15.34%	1.769%
3	3.852	143	147	155	rVB3	8263	13616	0.44%	0.050%
4	6.710	628	633	637	rBV3	4854	7577	0.24%	0.028%
5	6.769	637	643	663	rVV	306422	621648	19.93%	2.300%
6	6.916	663	668	689	rVB	259403	452597	14.51%	1.675%
7	7.116	695	702	725	rBV	357000	616811	19.78%	2.282%
8	7.569	772	779	794	rBV	319170	563563	18.07%	2.085%
9	8.281	894	900	921	rBV	380619	767372	24.61%	2.839%
10	8.716	966	974	997	rBV	338488	626220	20.08%	2.317%
11	9.422	1085	1094	1116	rBV	285305	557956	17.89%	2.064%
12	9.969	1179	1187	1221	rBV	359851	836801	26.83%	3.096%
13	10.322	1239	1247	1256	rBV	432578	727301	23.32%	2.691%
14	10.469	1265	1272	1290	rBV	290960	710873	22.80%	2.630%
15	11.957	1516	1525	1534	rBV9	4332	13389	0.43%	0.050%
16	13.592	1797	1803	1815	rBV	925856	1323300	42.44%	4.896%
17	13.881	1844	1852	1873	rBV	1061126	1452704	46.58%	5.375%
18	14.192	1898	1905	1922	rBV	747901	1065202	34.16%	3.941%
19	14.481	1946	1954	1955	rBV2	128020	206198	6.61%	0.763%
20	15.210	2070	2078	2091	rBV	1098189	1931794	61.95%	7.147%
21	15.363	2098	2104	2116	rBV	292208	542676	17.40%	2.008%
22	16.004	2209	2213	2218	rBV8	2561	4707	0.15%	0.017%
23	16.680	2322	2328	2331	rBV7	2434	4471	0.14%	0.017%
24	16.786	2343	2346	2351	rBV4	3129	4392	0.14%	0.016%
25	17.004	2375	2383	2392	rBV	949566	1418221	45.48%	5.247%
26	17.098	2394	2399	2415	rVV	1562035	2208012	70.81%	8.169%
27	17.698	2499	2501	2506	rVB5	2346	3498	0.11%	0.013%
28	17.945	2540	2543	2549	rBV8	5822	10053	0.32%	0.037%
29	19.027	2722	2727	2731	rBV3	18299	29803	0.96%	0.110%
30	19.116	2738	2742	2746	rBV	16720	22780	0.73%	0.084%
31	19.480	2797	2804	2820	rBV	1645225	2790512	89.49%	10.324%
32	21.439	3131	3137	3148	rBV	1159302	1836260	58.88%	6.794%
33	24.439	3637	3647	3662	rVB	1272252	3118404	100.00%	11.537%
34	24.662	3675	3685	3704	rVB	590056	2022722	64.86%	7.484%

Sum of corrected areas: 27028665




Instrument :
BNA_P
ClientSampleId :
SBLK061

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111924\
Data File : BP023236.D
Acq On : 20 Nov 2024 04:08
Operator : RC/JU
Sample : PB165061BL
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK061

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

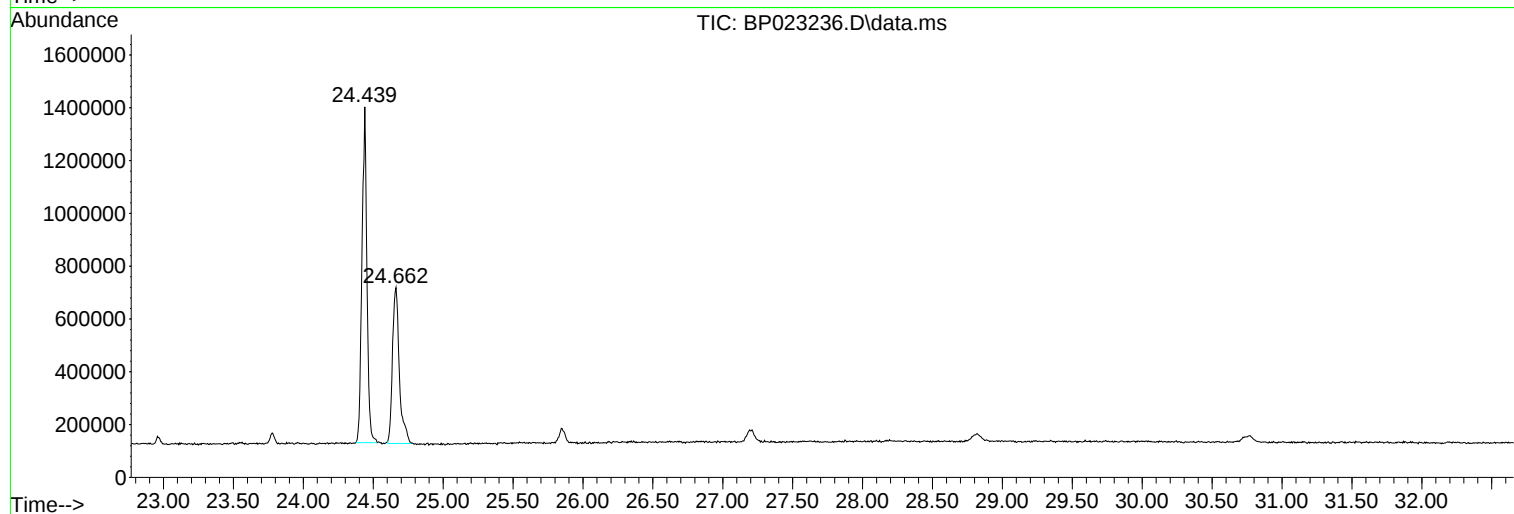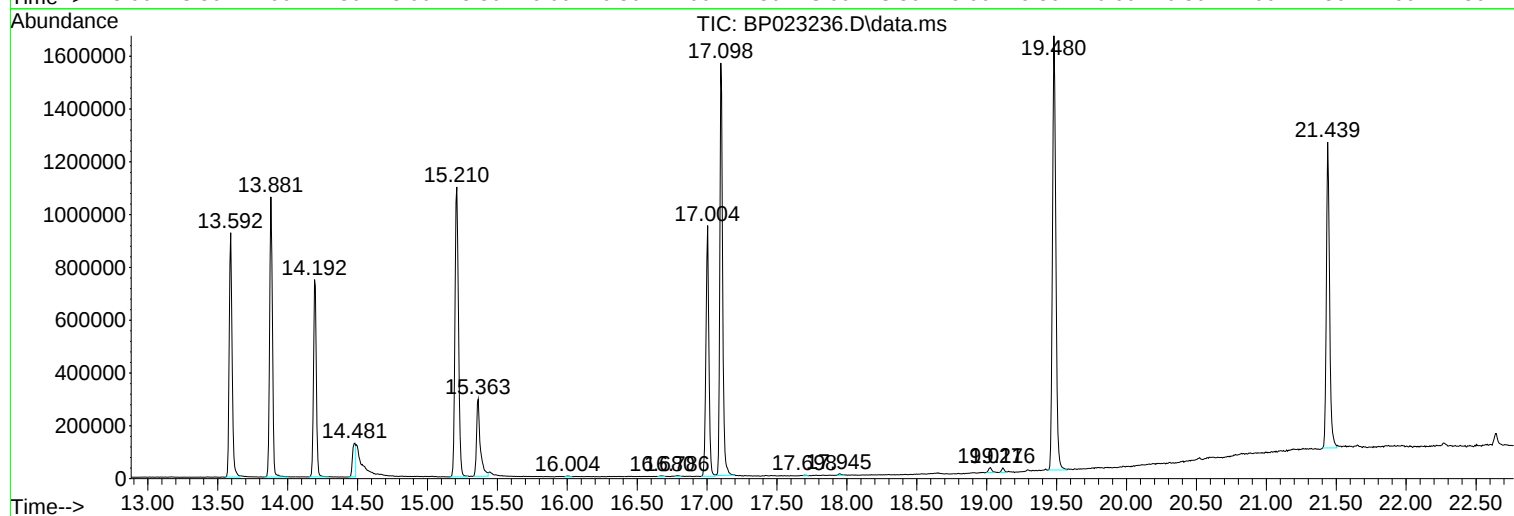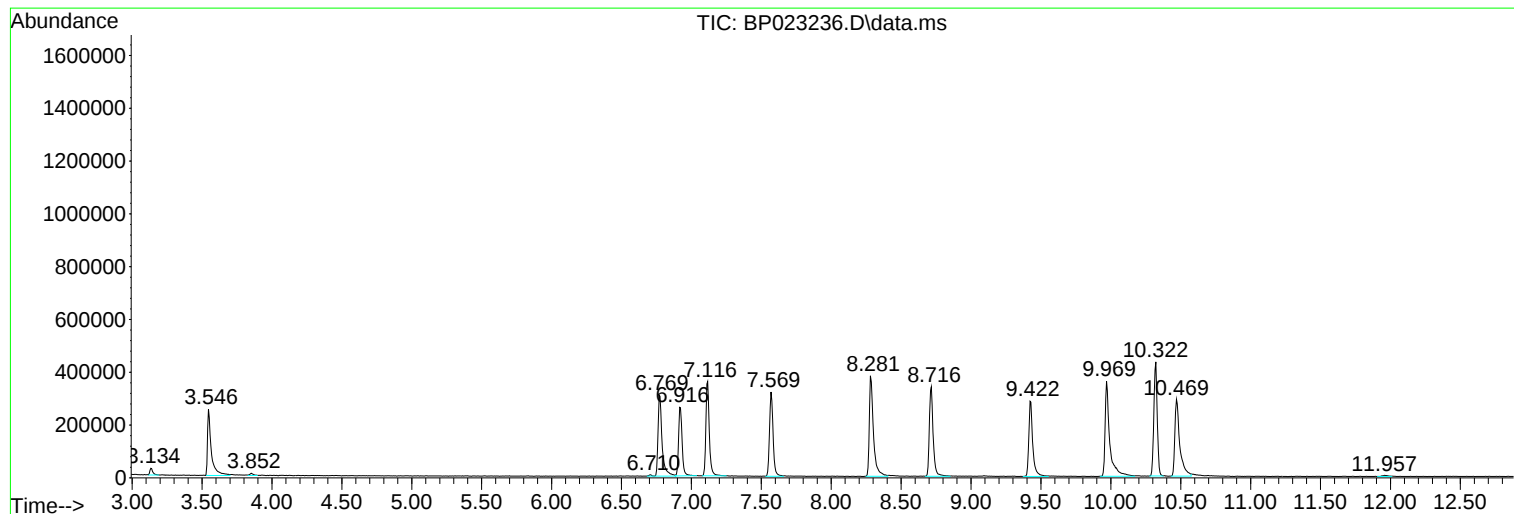

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111924\
Data File : BP023236.D
Acq On : 20 Nov 2024 04:08
Operator : RC/JU
Sample : PB165061BL
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK061

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111924\
Data File : BP023236.D
Acq On : 20 Nov 2024 04:08
Operator : RC/JU
Sample : PB165061BL
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK061

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc