

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111924\
 Data File : BP023247.D
 Acq On : 20 Nov 2024 12:17
 Operator : RC/JU
 Sample : PB165090BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK090

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP023247.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.134	21	25	32	rBV	16826	23551	1.07%	0.126%
2	3.546	91	95	119	rBV	165877	322994	14.68%	1.725%
3	3.852	143	147	155	rVB3	7019	12021	0.55%	0.064%
4	6.769	636	643	662	rBV	198454	410438	18.66%	2.193%
5	6.916	662	668	683	rVB	175346	289745	13.17%	1.548%
6	7.111	696	701	716	rBV	247201	412691	18.76%	2.205%
7	7.563	771	778	793	rBV	218961	400909	18.22%	2.142%
8	8.281	893	900	927	rBV	237073	506175	23.01%	2.704%
9	8.710	964	973	991	rBV	222529	424878	19.31%	2.270%
10	8.863	993	999	1000	rBV5	5679	6753	0.31%	0.036%
11	9.422	1087	1094	1118	rBV	181187	367032	16.68%	1.961%
12	9.975	1180	1188	1208	rBV	211854	536021	24.37%	2.863%
13	10.316	1239	1246	1262	rBV	297088	512908	23.31%	2.740%
14	10.469	1265	1272	1288	rBV	193979	465176	21.14%	2.485%
15	11.957	1519	1525	1539	rVB7	3102	8822	0.40%	0.047%
16	13.598	1797	1804	1815	rBV	708416	890887	40.50%	4.759%
17	13.875	1844	1851	1867	rBV	601163	949788	43.17%	5.074%
18	14.187	1896	1904	1916	rBV	450184	743134	33.78%	3.970%
19	14.481	1945	1954	1964	rBV2	86192	280291	12.74%	1.497%
20	15.187	2065	2074	2085	rBV	620387	1261495	57.34%	6.739%
21	15.357	2098	2103	2115	rBV	188306	378939	17.22%	2.024%
22	15.439	2115	2117	2130	rVB7	13413	27762	1.26%	0.148%
23	16.981	2373	2379	2391	rBV	694422	1003795	45.63%	5.362%
24	17.098	2391	2399	2412	rBV	906555	1471972	66.91%	7.863%
25	17.963	2544	2546	2550	rVB5	3368	3830	0.17%	0.020%
26	18.086	2563	2567	2571	rVV6	1983	2514	0.11%	0.013%
27	19.028	2722	2727	2733	rBV3	11927	21016	0.96%	0.112%
28	19.110	2737	2741	2745	rVV2	9807	15988	0.73%	0.085%
29	19.480	2797	2804	2820	rBV	1186068	1900790	86.40%	10.154%
30	21.439	3130	3137	3148	rBV2	738590	1361627	61.89%	7.274%
31	24.427	3636	3645	3663	rVB	819402	2199949	100.00%	11.752%
32	24.645	3674	3682	3705	rVB	512889	1505733	68.44%	8.044%




Sum of corrected areas: 18719624

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111924\
Data File : BP023247.D
Acq On : 20 Nov 2024 12:17
Operator : RC/JU
Sample : PB165090BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK090

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

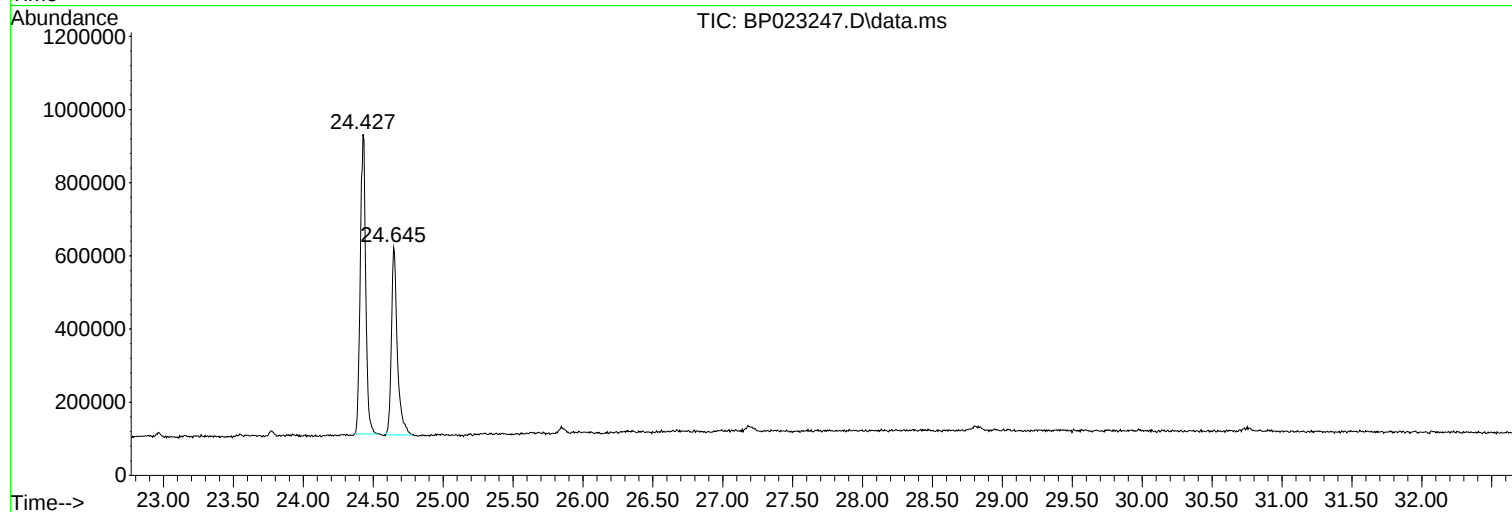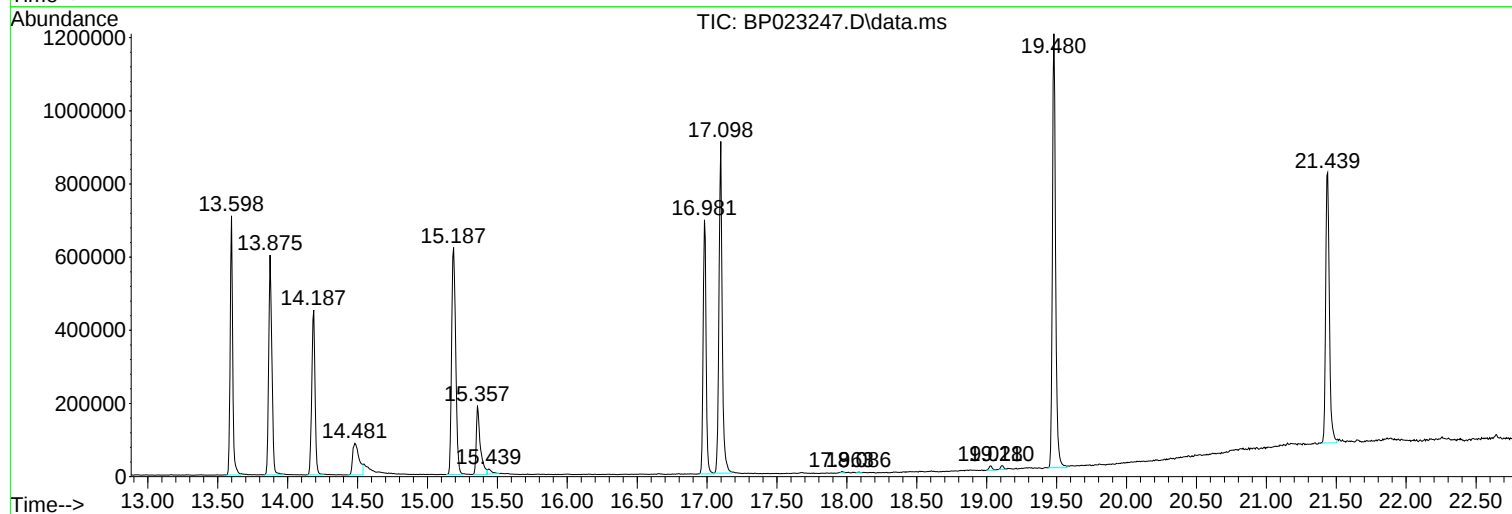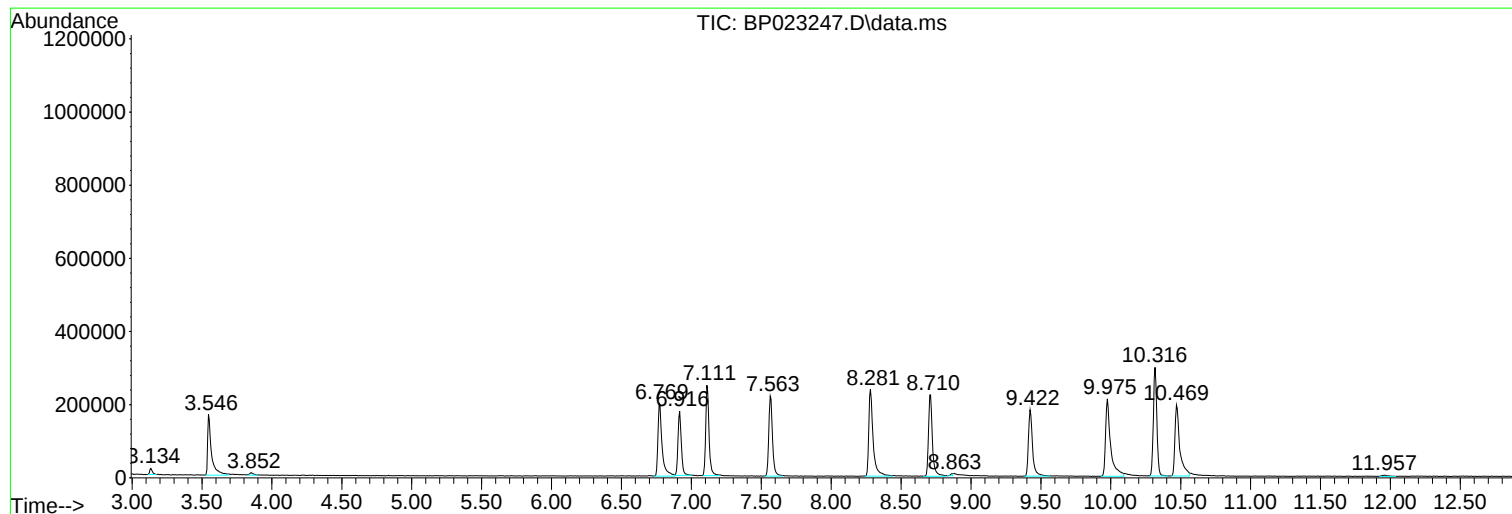

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111924\
Data File : BP023247.D
Acq On : 20 Nov 2024 12:17
Operator : RC/JU
Sample : PB165090BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK090

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111924\
Data File : BP023247.D
Acq On : 20 Nov 2024 12:17
Operator : RC/JU
Sample : PB165090BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK090

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------