

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111924\
 Data File : BP023255.D
 Acq On : 20 Nov 2024 17:43
 Operator : RC/JU
 Sample : P4875-21
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E2A20

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP023255.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.134	21	25	31	rBV	12876	18404	0.60%	0.079%
2	3.564	95	98	111	rBV	44479	100066	3.29%	0.431%
3	3.852	143	147	153	rBV	13998	22021	0.72%	0.095%
4	4.217	207	209	214	rVB6	2993	4215	0.14%	0.018%
5	4.275	214	219	225	rVB	6521	10564	0.35%	0.045%
6	6.705	626	632	638	rBV3	4683	6771	0.22%	0.029%
7	6.787	639	646	662	rBV2	46326	121087	3.98%	0.521%
8	6.916	662	668	680	rVB	221305	343031	11.28%	1.476%
9	7.116	695	702	725	rBV	237933	435001	14.30%	1.872%
10	7.563	772	778	787	rBV	254900	449917	14.79%	1.936%
11	7.634	787	790	799	rVB2	16963	30911	1.02%	0.133%
12	8.287	895	901	918	rBV	176362	364530	11.98%	1.569%
13	8.652	957	963	966	rBV5	3758	6728	0.22%	0.029%
14	8.710	966	973	996	rVV	265735	505593	16.62%	2.176%
15	8.869	996	1000	1012	rVV	4675	10902	0.36%	0.047%
16	9.093	1034	1038	1042	rBV5	2633	4011	0.13%	0.017%
17	9.422	1086	1094	1112	rBV2	216459	472345	15.53%	2.033%
18	9.963	1177	1186	1205	rBV	257345	645974	21.23%	2.780%
19	10.310	1237	1245	1256	rBV	338866	593187	19.50%	2.553%
20	10.469	1265	1272	1294	rBV	212589	529725	17.41%	2.280%
21	11.210	1394	1398	1401	rBV6	1848	3474	0.11%	0.015%
22	11.940	1515	1522	1527	rBV6	4640	9274	0.30%	0.040%
23	12.775	1659	1664	1669	rBV7	2376	3265	0.11%	0.014%
24	13.040	1705	1709	1714	rBV5	2478	5275	0.17%	0.023%
25	13.581	1794	1801	1819	rBV	760363	1191066	39.15%	5.126%
26	13.869	1839	1850	1869	rBV	887887	1227990	40.37%	5.285%
27	14.181	1896	1903	1913	rBV	647794	907627	29.83%	3.906%
28	14.263	1913	1917	1923	rVB8	6320	9487	0.31%	0.041%
29	14.522	1954	1961	1974	rBV4	22063	80125	2.63%	0.345%
30	14.687	1985	1989	1995	rVB9	4185	8747	0.29%	0.038%
31	14.875	2017	2021	2027	rBV8	3822	6029	0.20%	0.026%
32	14.992	2037	2041	2045	rVV3	3767	4839	0.16%	0.021%
33	15.040	2045	2049	2055	rVB7	2961	5595	0.18%	0.024%
34	15.204	2069	2077	2090	rBV	1326509	1725031	56.70%	7.424%
35	15.351	2096	2102	2113	rBV	288394	586615	19.28%	2.525%
36	15.587	2138	2142	2146	rVB7	3744	6013	0.20%	0.026%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111924\
 Data File : BP023255.D
 Acq On : 20 Nov 2024 17:43
 Operator : RC/JU
 Sample : P4875-21
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E2A20

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
 Title : SVOA CALIBRATION

37	15.998	2207	2212	2216	rBV8	2176	4105	0.13%	0.018%
38	16.587	2306	2312	2316	rBV5	3093	5541	0.18%	0.024%
39	16.957	2371	2375	2376	rVV4	2463	3058	0.10%	0.013%
40	16.998	2376	2382	2391	rVV	869208	1220336	40.11%	5.252%
41	17.092	2392	2398	2414	rVB	1569696	2227629	73.22%	9.588%
42	17.245	2420	2424	2430	rVB8	3831	6208	0.20%	0.027%
43	17.298	2430	2433	2438	rVB4	3139	4409	0.14%	0.019%
44	17.686	2494	2499	2509	rVB	104121	141523	4.65%	0.609%
45	17.804	2517	2519	2524	rVB5	2348	3121	0.10%	0.013%
46	17.939	2537	2542	2548	rBV6	13713	23175	0.76%	0.100%
47	18.004	2550	2553	2560	rVB	8429	11283	0.37%	0.049%
48	18.498	2633	2637	2638	rBV4	3508	3585	0.12%	0.015%
49	19.028	2722	2727	2732	rBV3	20148	33362	1.10%	0.144%
50	19.116	2739	2742	2746	rBV2	13883	19076	0.63%	0.082%
51	19.286	2767	2771	2776	rBV6	8422	16114	0.53%	0.069%
52	19.416	2791	2793	2798	rVB5	3984	4923	0.16%	0.021%
53	19.486	2798	2805	2821	rBV	1683396	2889588	94.98%	12.437%
54	21.433	3130	3136	3146	rBV	948139	1508982	49.60%	6.495%
55	24.427	3635	3645	3659	rBV	1150382	3042209	100.00%	13.094%
56	24.645	3674	3682	3701	rVB	514775	1610741	52.95%	6.933%




Sum of corrected areas: 23234403

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111924\
Data File : BP023255.D
Acq On : 20 Nov 2024 17:43
Operator : RC/JU
Sample : P4875-21
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E2A20

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

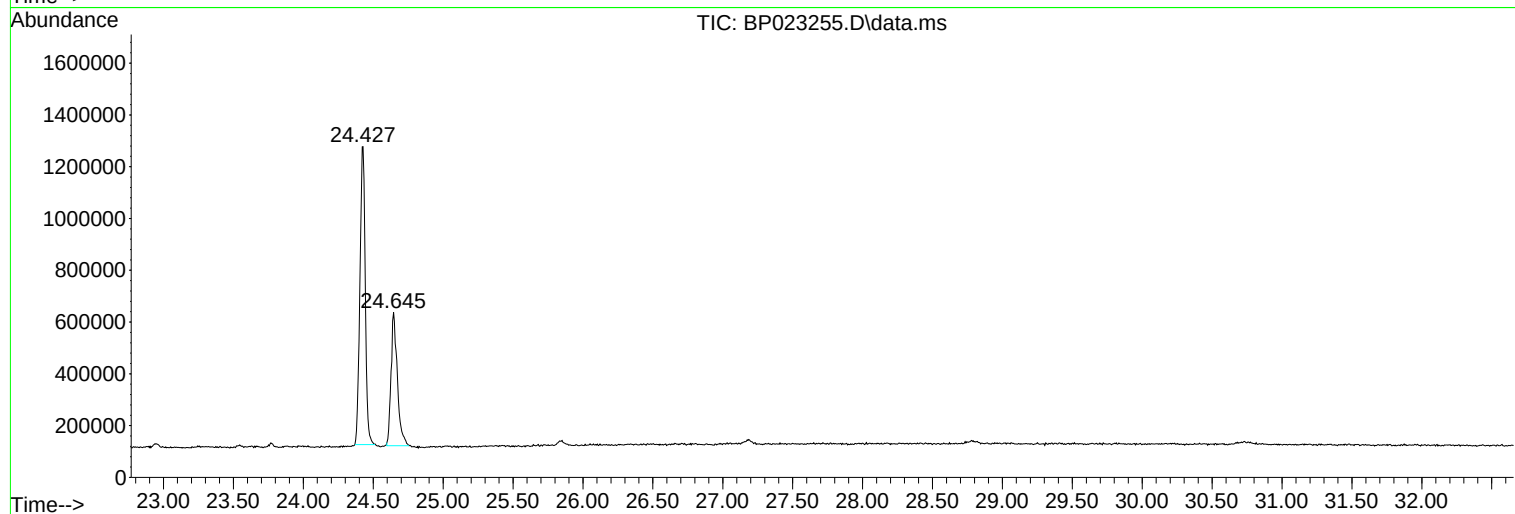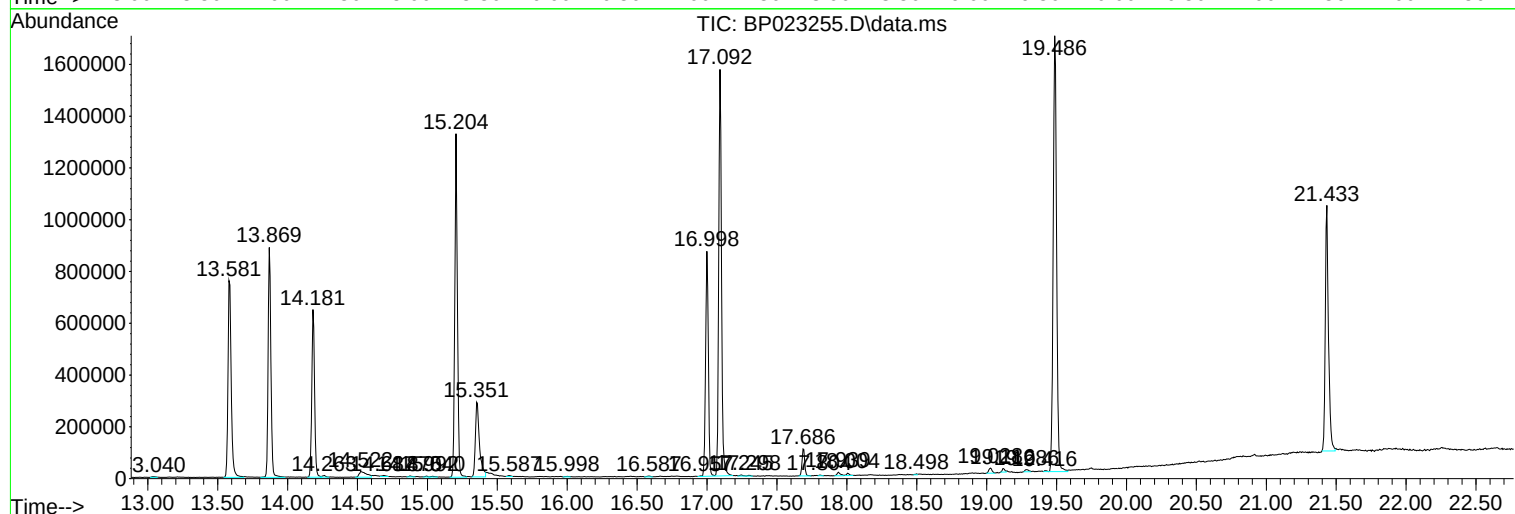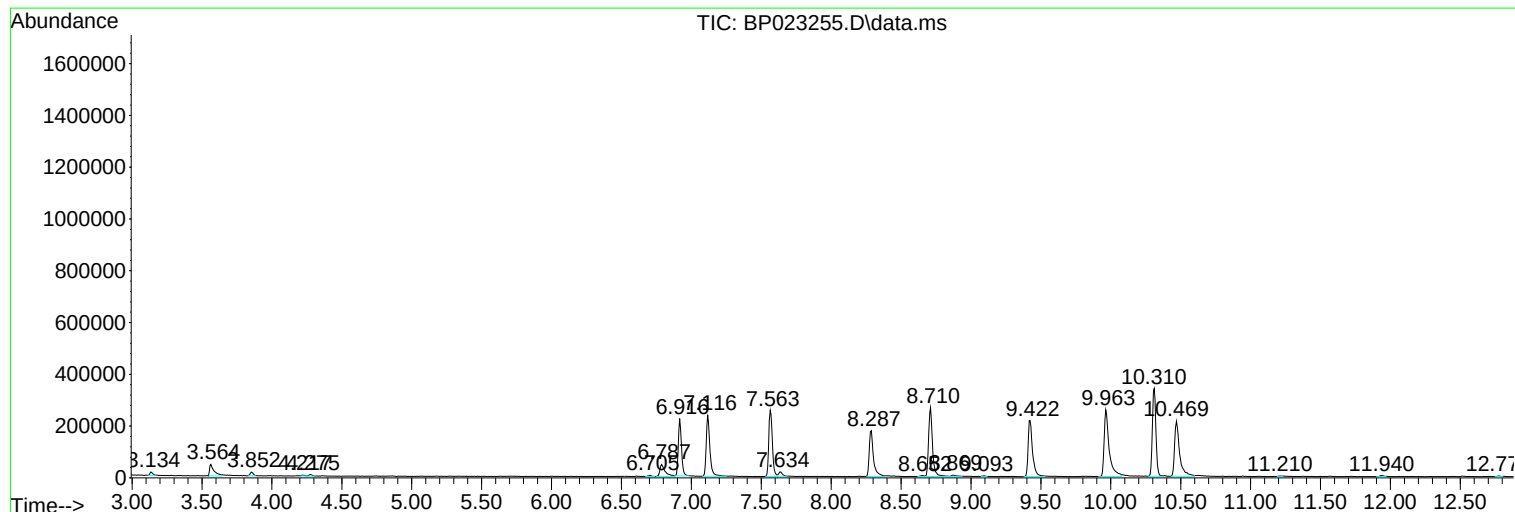

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111924\
Data File : BP023255.D
Acq On : 20 Nov 2024 17:43
Operator : RC/JU
Sample : P4875-21
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E2A20










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 7,9-Di-tert-butyl-1-oxaspiro... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
17.686	2.32 ng/ul	141523	Phenanthrene-d10	16.998

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	7,9-Di-tert-butyl-1-oxaspiro(4,5...	276	C17H24O3	082304-66-3	94		
2	7,9-Di-tert-butyl-1-oxaspiro(4,5...	276	C17H24O3	082304-66-3	90		
3	7,9-Di-tert-butyl-1-oxaspiro(4,5...	276	C17H24O3	082304-66-3	46		
4	Ethanone, 1-(5,6,7,8-tetrahydro-...	220	C14H20O2	071596-88-8	43		
5	1-(3-Amino-4,6-dimethylthieno[2,...	220	C11H12N2OS	052505-42-7	43		

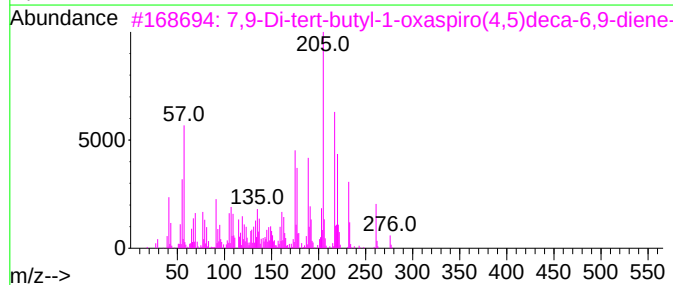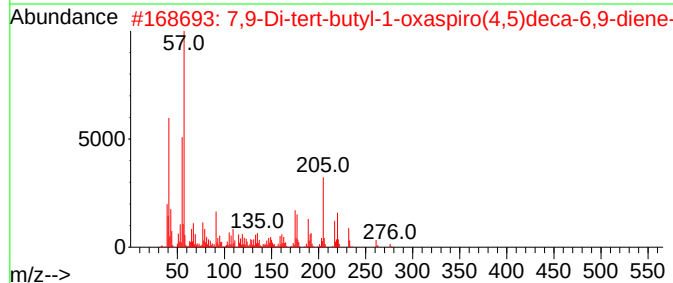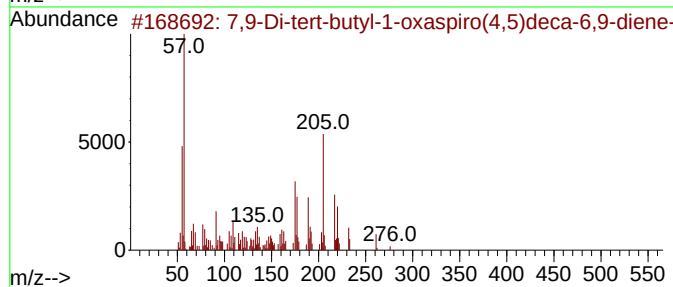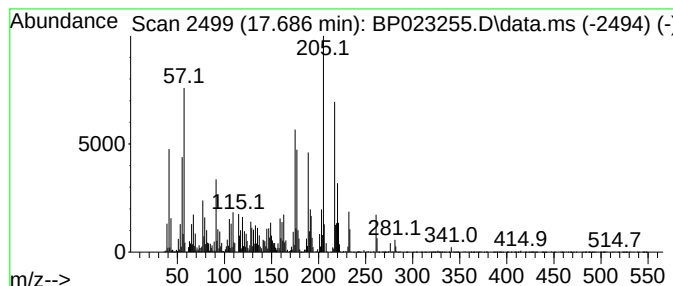

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111924\
Data File : BP023255.D
Acq On : 20 Nov 2024 17:43
Operator : RC/JU
Sample : P4875-21
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E2A20

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
7,9-Di-tert-but...	17.686	2.3	ng/u1	141523	4	16.998	1220340	20.0