

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111924\
 Data File : BP023288.D
 Acq On : 21 Nov 2024 17:25
 Operator : RC/JU
 Sample : PB165168BL
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK168

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP023288.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.134	21	25	31	rBV	18490	25614	1.17%	0.135%
2	3.546	91	95	114	rBV	181986	342660	15.71%	1.809%
3	3.852	143	147	154	rVB4	4091	6419	0.29%	0.034%
4	6.775	637	644	663	rBV	215335	443477	20.34%	2.341%
5	6.916	663	668	680	rVB	203849	309117	14.17%	1.632%
6	7.110	695	701	720	rBV	257721	445041	20.41%	2.350%
7	7.563	771	778	797	rBV	241817	399299	18.31%	2.108%
8	8.281	893	900	919	rBV2	273569	540185	24.77%	2.852%
9	8.710	965	973	988	rBV	249729	440666	20.21%	2.326%
10	9.422	1085	1094	1113	rBV	194298	382421	17.54%	2.019%
11	9.969	1177	1187	1218	rBV	221031	588985	27.01%	3.110%
12	10.316	1236	1246	1258	rBV	305385	512925	23.52%	2.708%
13	10.469	1265	1272	1296	rBV	221506	522391	23.95%	2.758%
14	11.945	1516	1523	1528	rBV4	3118	6308	0.29%	0.033%
15	13.587	1797	1802	1826	rBV	647301	881825	40.44%	4.656%
16	13.875	1842	1851	1864	rBV	667587	977293	44.81%	5.160%
17	14.181	1894	1903	1924	rBV	462604	755471	34.64%	3.988%
18	14.486	1947	1955	1968	rBV	106692	324167	14.86%	1.711%
19	15.198	2069	2076	2088	rBV	646137	1265892	58.05%	6.683%
20	15.357	2097	2103	2113	rBV	197292	349547	16.03%	1.845%
21	16.998	2375	2382	2393	rBV	677810	1008107	46.23%	5.322%
22	17.098	2393	2399	2413	rVV	1047158	1498386	68.71%	7.911%
23	17.945	2539	2543	2546	rBV5	4164	5359	0.25%	0.028%
24	18.063	2560	2563	2566	rBV4	1544	2268	0.10%	0.012%
25	18.092	2566	2568	2573	rBV6	1992	3347	0.15%	0.018%
26	18.633	2658	2660	2662	rBV2	2508	2412	0.11%	0.013%
27	19.027	2723	2727	2733	rBV3	16337	24400	1.12%	0.129%
28	19.110	2737	2741	2747	rBV3	11361	19701	0.90%	0.104%
29	19.480	2798	2804	2819	rBV	1178035	1932106	88.60%	10.200%
30	21.445	3132	3138	3152	rBV	779774	1327525	60.87%	7.009%
31	24.451	3639	3649	3665	rVB	818266	2180781	100.00%	11.513%
32	24.668	3677	3686	3703	rVB	460390	1417327	64.99%	7.483%




Sum of corrected areas: 18941422

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111924\
Data File : BP023288.D
Acq On : 21 Nov 2024 17:25
Operator : RC/JU
Sample : PB165168BL
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK168

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

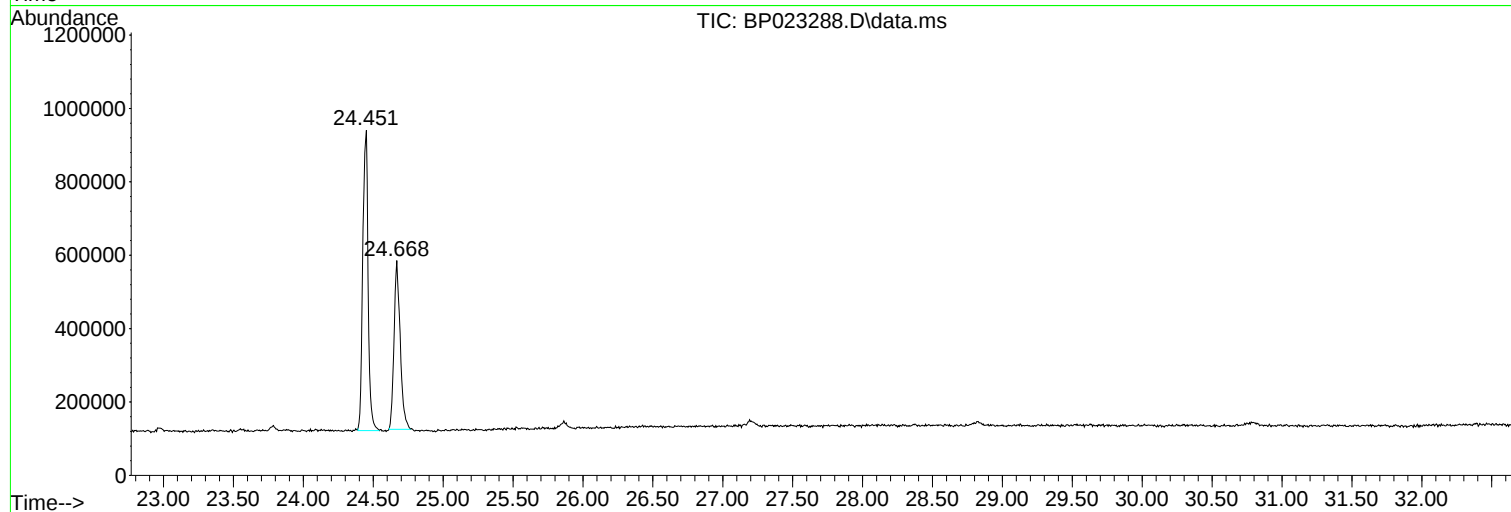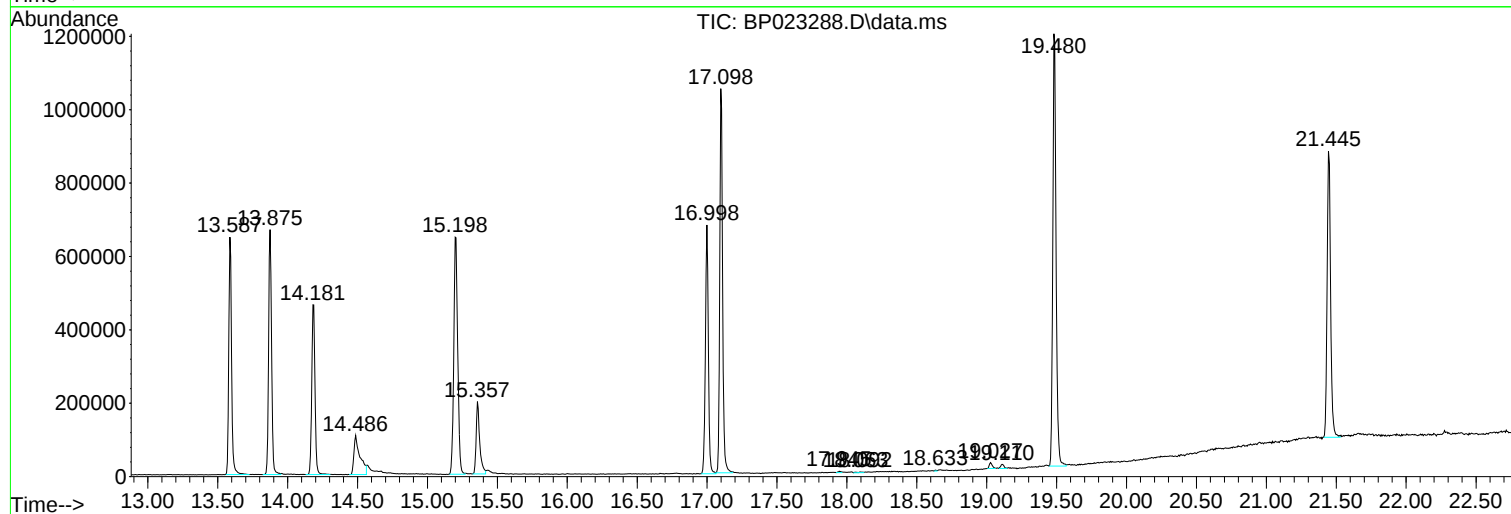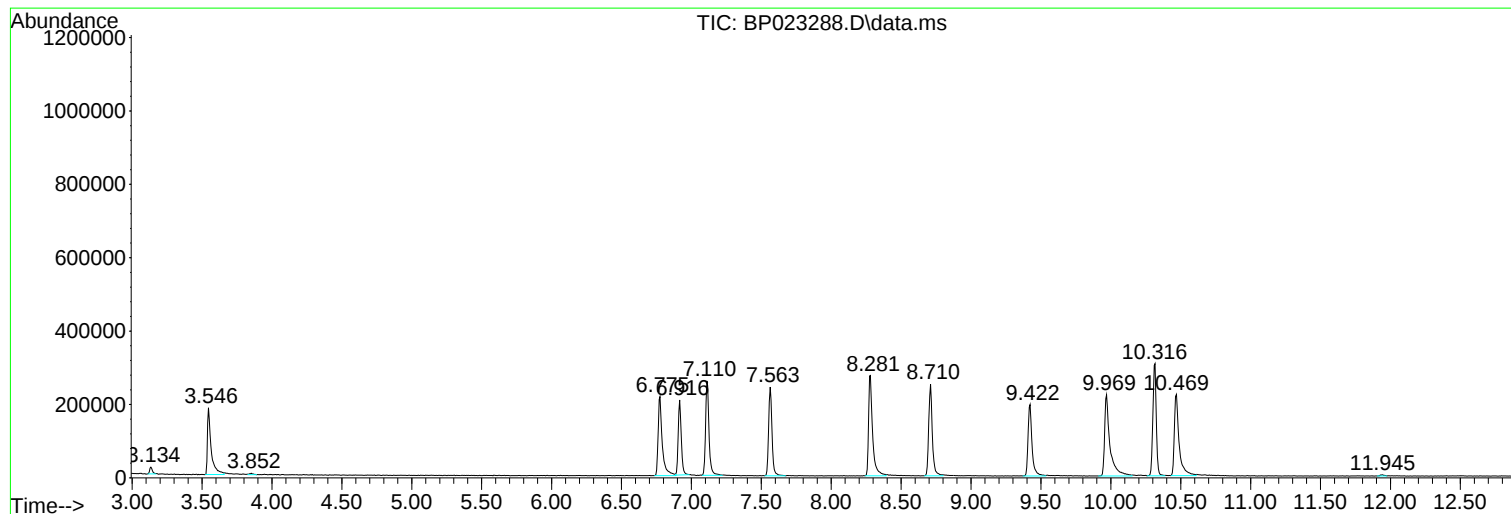

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111924\
Data File : BP023288.D
Acq On : 21 Nov 2024 17:25
Operator : RC/JU
Sample : PB165168BL
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK168

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111924\
Data File : BP023288.D
Acq On : 21 Nov 2024 17:25
Operator : RC/JU
Sample : PB165168BL
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK168

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc