

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112020\
 Data File : BP004025.D
 Acq On : 20 Nov 2020 15:15
 Operator : CG/JU
 Sample : L4716-02
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 STOCKPILE-2

Manual Integrations
 APPROVED

mohammad
 11/24/2020 8:55:16 AM

Quant Time: Nov 20 16:22:49 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 20 12:19:10 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.269	152	131828	20.00	ng	0.00
21) Naphthalene-d8	11.099	136	510463	20.00	ng	# 0.00
39) Acenaphthene-d10	14.887	164	305931	20.00	ng	0.00
64) Phenanthrene-d10	17.622	188	632902	20.00	ng	0.00
76) Chrysene-d12	21.657	240	593654	20.00	ng	0.00
86) Perylene-d12	24.127	264	588822	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.805	112	759888	96.20	ng	0.00
7) Phenol-d6	7.452	99	999496	88.15	ng	0.00
23) Nitrobenzene-d5	9.428	82	656977	63.03	ng	-0.01
42) 2,4,6-Tribromophenol	16.375	330	389483	101.79	ng	0.00
45) 2-Fluorobiphenyl	13.510	172	1451973	66.35	ng	0.00
79) Terphenyl-d14	20.122	244	1860430	60.55	ng	0.00
Target Compounds						Qvalue
10) Phenol	7.475	94	84914	7.76	ng	77
50) Dimethylphthalate	14.316	163	88239	3.69	ng	98
71) Phenanthrene	17.663	178	164818	4.64	ng	98
75) Fluoranthene	19.598	202	541655	13.22	ng	100
78) Pyrene	19.945	202	509498	12.65	ng	98
81) Benzo(a)anthracene	21.639	228	276033	7.05	ng	97
83) Chrysene	21.692	228	278605	7.41	ng	97
87) Indeno(1,2,3-cd)pyrene	26.674	276	173986	4.10	ng	# 93
88) Benzo(b)fluoranthene	23.375	252	361278m	9.38	ng	
89) Benzo(k)fluoranthene	23.416	252	136404m	3.59	ng	
90) Benzo(a)pyrene	24.016	252	246959	6.92	ng	98
92) Benzo(g,h,i)perylene	27.457	276	179388	5.23	ng	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112020\
Data File : BP004025.D
Acq On : 20 Nov 2020 15:15
Operator : CG/JU
Sample : L4716-02
Misc :
ALS Vial : 9 Sample Multiplier: 1


Instrument :
BNA_P
ClientSampleId :
STOCKPILE-2

Manual Integrations
APPROVED

mohammad
11/24/2020 8:55:16 AM


Quant Time: Nov 20 16:22:49 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 20 12:19:10 2020
Response via : Initial Calibration

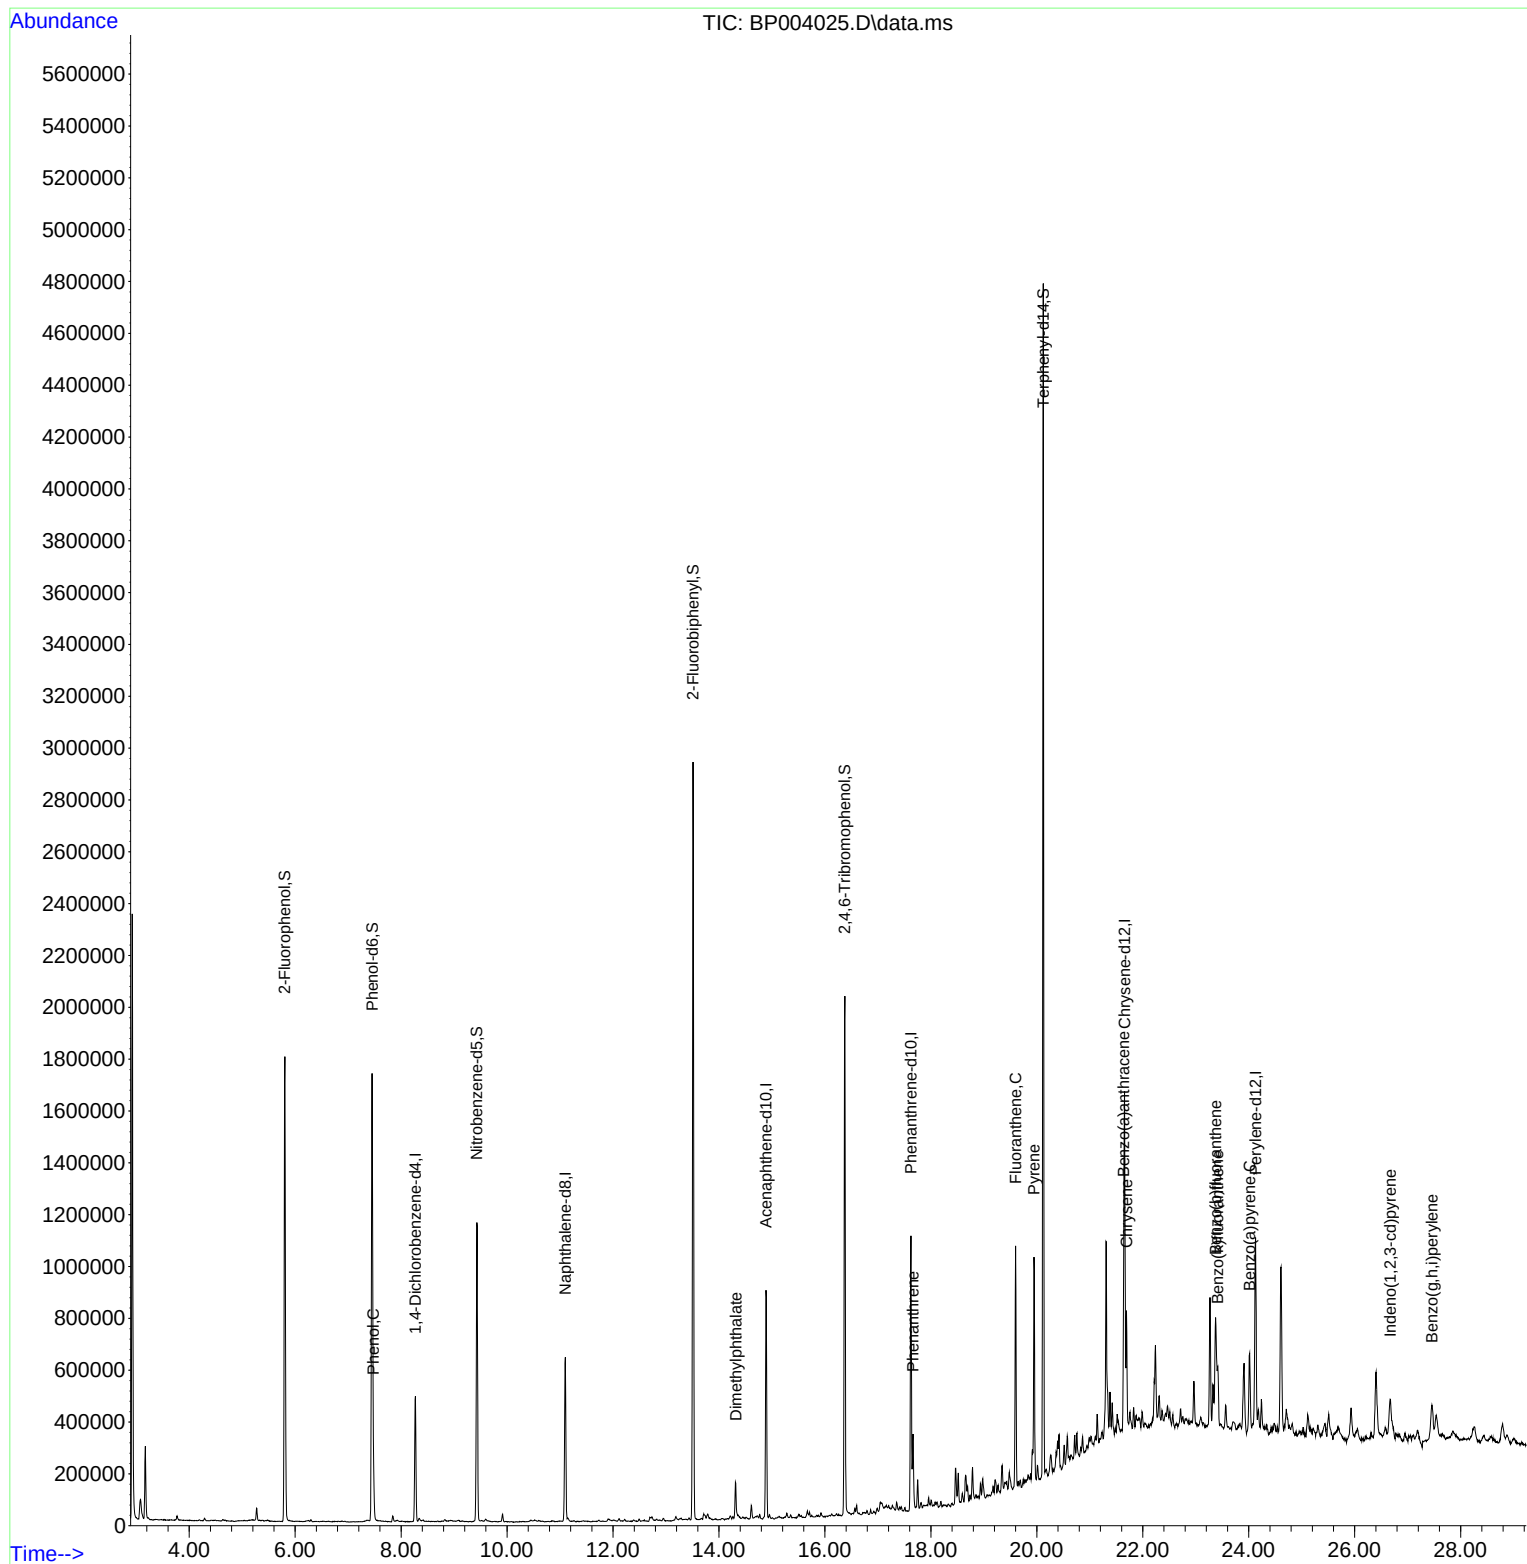



#1
1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 8.269 min Scan# 915
Delta R.T. 0.000 min
Lab File: BP004025.D
Acq: 20 Nov 2020 15:15




Instrument :
BNA_P
ClientSampleId :
STOCKPILE-2



Tgt Ion:152 Resp: 131828
Ion Ratio Lower Upper
152 100
150 151.4 123.8 185.6
115 58.2 43.8 65.6




Manual Integrations
APPROVED


mohammad
11/24/2020 8:55:16 AM

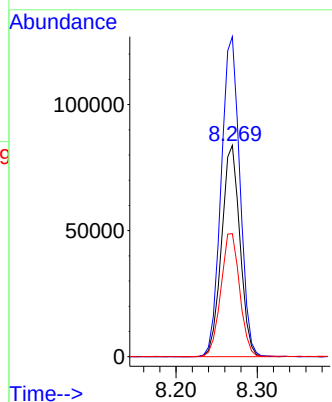

#5
2-Fluorophenol
Concen: 96.20 ng
RT: 5.805 min Scan# 496
Delta R.T. 0.006 min
Lab File: BP004025.D
Acq: 20 Nov 2020 15:15


Tgt Ion:112 Resp: 759888
Ion Ratio Lower Upper
112 100
64 62.7 32.8 49.2#
63 32.4 17.0 25.4#

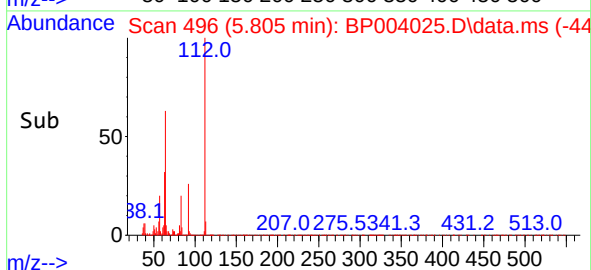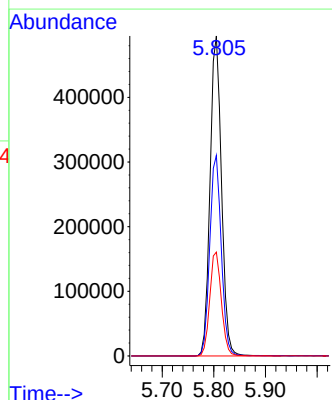



#7
Phenol-d6
Concen: 88.15 ng
RT: 7.452 min Scan# 776
Delta R.T. -0.006 min
Lab File: BP004025.D
Acq: 20 Nov 2020 15:15




Instrument :
BNA_P
ClientSampleId :
STOCKPILE-2




Tgt Ion: 99 Resp: 999496
Ion Ratio Lower Upper
99 100
42 18.2 8.6 13.0#
71 35.1 23.4 35.2

Manual Integrations
APPROVED



mohammad
11/24/2020 8:55:16 AM

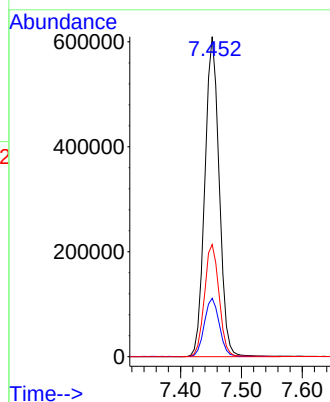


#10
Phenol
Concen: 7.76 ng
RT: 7.475 min Scan# 780
Delta R.T. -0.006 min
Lab File: BP004025.D
Acq: 20 Nov 2020 15:15



Tgt Ion: 94 Resp: 84914
Ion Ratio Lower Upper
94 100
65 29.7 2.3 42.3
66 46.5 10.9 50.9

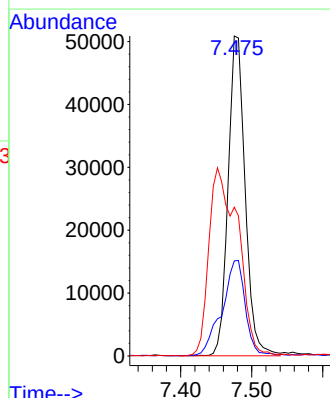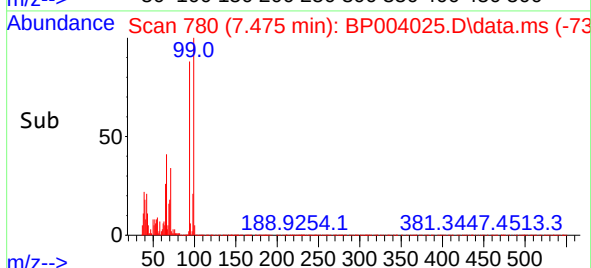







#21
Naphthalene-d8
Concen: 20.00 ng
RT: 11.099 min Scan# 1396
Delta R.T. 0.000 min
Lab File: BP004025.D
Acq: 20 Nov 2020 15:15

Tgt Ion:	136	Resp:	510463
Ion Ratio	Lower	Upper	
136	100		
137	10.9	8.6	13.0
54	9.2	3.6	5.4#
68	5.7	3.3	4.9#

Instrument :
BNA_P
ClientSampleId :
STOCKPILE-2




Manual Integrations
APPROVED


mohammad
11/24/2020 8:55:16 AM

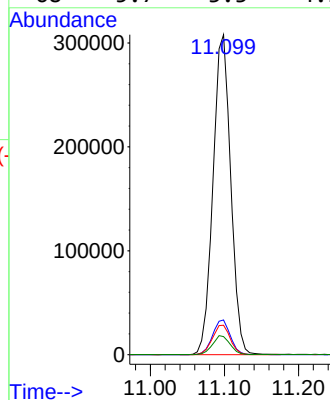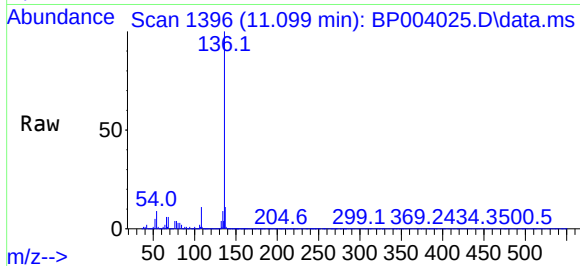

#23
Nitrobenzene-d5
Concen: 63.03 ng
RT: 9.428 min Scan# 1112
Delta R.T. -0.011 min
Lab File: BP004025.D
Acq: 20 Nov 2020 15:15


Tgt Ion:	82	Resp:	656977
Ion Ratio	Lower	Upper	
82	100		
128	41.2	45.6	68.4#
54	54.5	30.1	45.1#

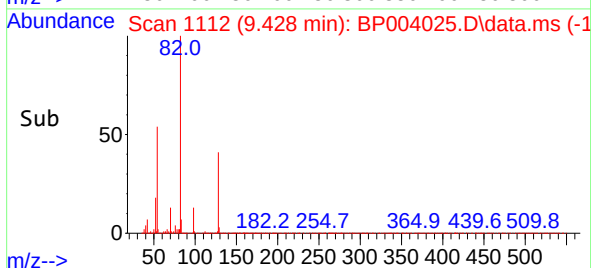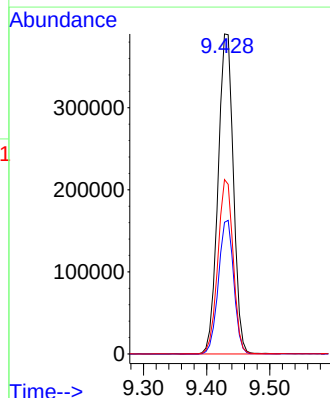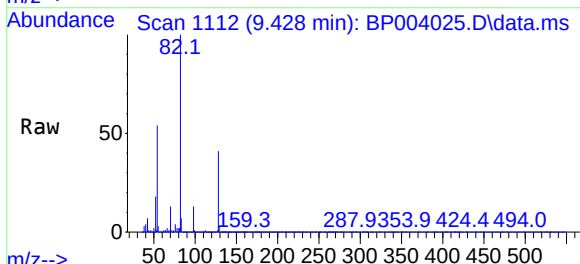



#39
Acenaphthene-d10
Concen: 20.00 ng
RT: 14.887 min Scan# 2040
Delta R.T. -0.006 min
Lab File: BP004025.D
Acq: 20 Nov 2020 15:15




Instrument :
BNA_P
ClientSampleId :
STOCKPILE-2




Tgt Ion:164 Resp: 305931
Ion Ratio Lower Upper
164 100
162 99.4 79.4 119.2
160 43.0 36.1 54.1

Manual Integrations
APPROVED



mohammad
11/24/2020 8:55:16 AM

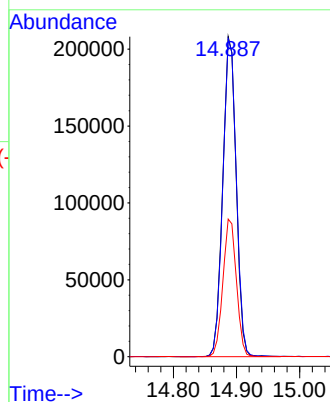


#42
2,4,6-Tribromophenol
Concen: 101.79 ng
RT: 16.375 min Scan# 2293
Delta R.T. 0.000 min
Lab File: BP004025.D
Acq: 20 Nov 2020 15:15




Tgt Ion:330 Resp: 389483
Ion Ratio Lower Upper
330 100
332 96.7 77.1 115.7
141 31.0 23.4 35.2

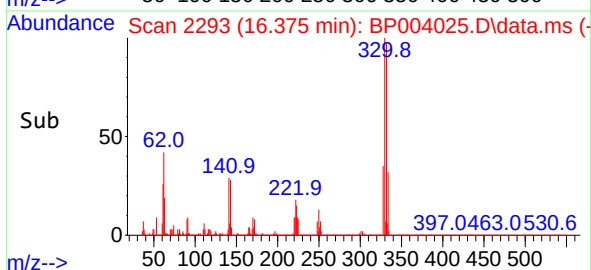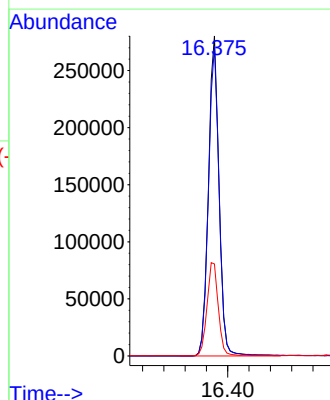



#45
2-Fluorobiphenyl
Concen: 66.35 ng
RT: 13.510 min Scan# 1806
Delta R.T. -0.006 min
Lab File: BP004025.D
Acq: 20 Nov 2020 15:15




Instrument :
BNA_P
ClientSampleId :
STOCKPILE-2

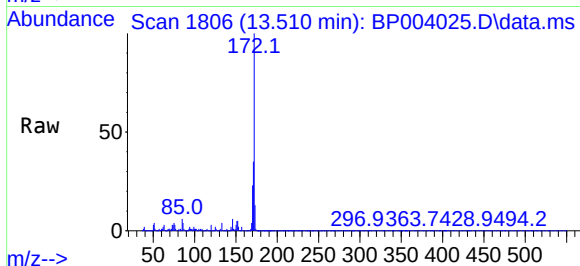

Tgt Ion:172 Resp: 1451973
Ion Ratio Lower Upper
172 100
171 34.6 28.5 42.7
170 22.7 19.2 28.8




Manual Integrations
APPROVED


mohammad
11/24/2020 8:55:16 AM

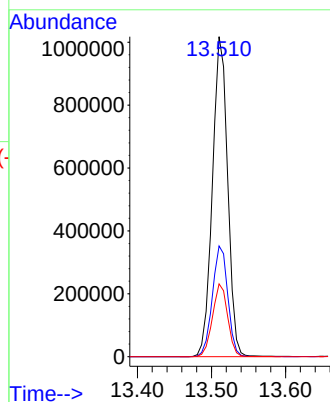

#50
Dimethylphthalate
Concen: 3.69 ng
RT: 14.316 min Scan# 1943
Delta R.T. -0.006 min
Lab File: BP004025.D
Acq: 20 Nov 2020 15:15


Tgt Ion:163 Resp: 88239
Ion Ratio Lower Upper
163 100
194 3.9 3.3 4.9
164 9.0 8.2 12.2

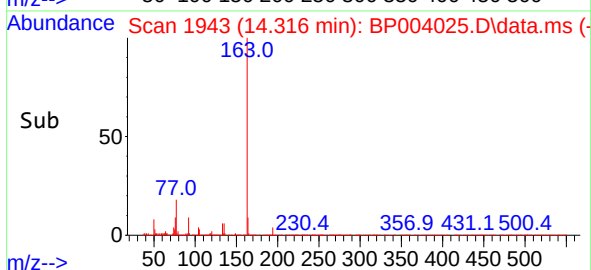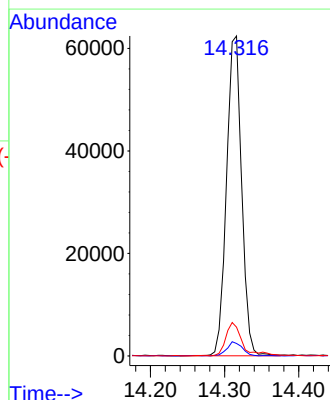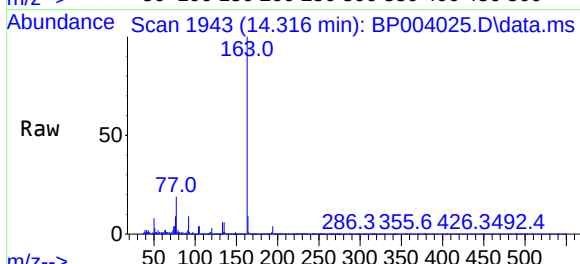



#64
Phenanthrene-d10
Concen: 20.00 ng
RT: 17.622 min Scan# 2505
Delta R.T. 0.000 min
Lab File: BP004025.D
Acq: 20 Nov 2020 15:15




Instrument :
BNA_P
ClientSampleId :
STOCKPILE-2




Tgt Ion:188 Resp: 632902
Ion Ratio Lower Upper
188 100
94 7.9 6.2 9.2
80 9.2 6.2 9.2

Manual Integrations
APPROVED



mohammad
11/24/2020 8:55:16 AM

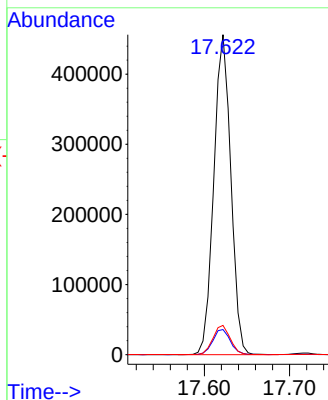


#71
Phenanthrene
Concen: 4.64 ng
RT: 17.663 min Scan# 2512
Delta R.T. -0.006 min
Lab File: BP004025.D
Acq: 20 Nov 2020 15:15



Tgt Ion:178 Resp: 164818
Ion Ratio Lower Upper
178 100
176 17.9 15.3 22.9
179 16.3 12.5 18.7

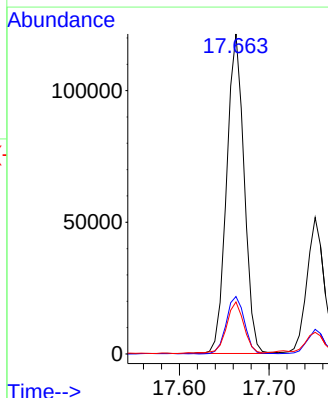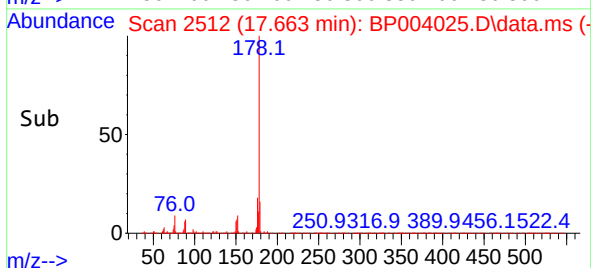







#75
Fluoranthene
Concen: 13.22 ng
RT: 19.598 min Scan# 2841
Delta R.T. -0.006 min
Lab File: BP004025.D
Acq: 20 Nov 2020 15:15

Tgt Ion:	202	Resp:	541655
Ion Ratio	Lower	Upper	
202	100		
101	9.8	0.0	29.4
203	17.8	0.0	37.8

Instrument :
BNA_P
ClientSampleId :
STOCKPILE-2




Manual Integrations
APPROVED


mohammad
11/24/2020 8:55:16 AM

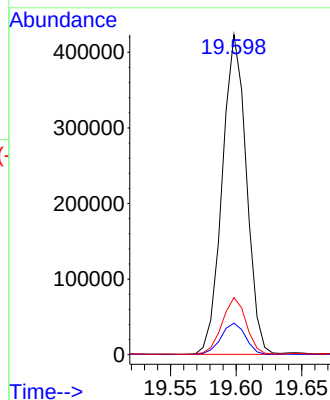

#76
Chrysene-d12
Concen: 20.00 ng
RT: 21.657 min Scan# 3191
Delta R.T. 0.000 min
Lab File: BP004025.D
Acq: 20 Nov 2020 15:15


Tgt Ion:	240	Resp:	593654
Ion Ratio	Lower	Upper	
240	100		
120	8.7	7.8	11.6
236	25.0	20.8	31.2

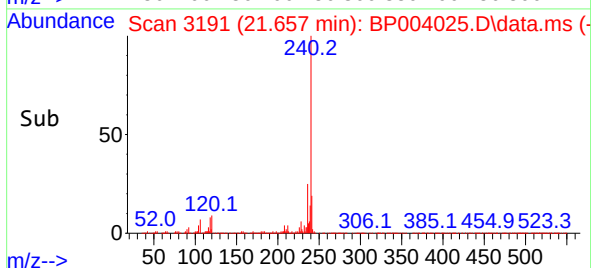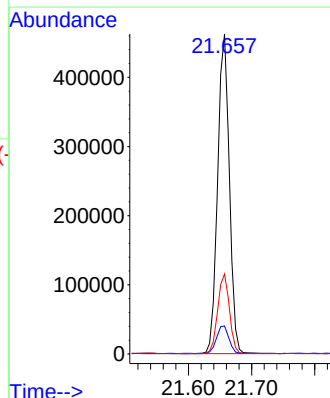



#78
Pyrene
Concen: 12.65 ng
RT: 19.945 min Scan# 2900
Delta R.T. -0.006 min
Lab File: BP004025.D
Acq: 20 Nov 2020 15:15




Instrument :
BNA_P
ClientSampleId :
STOCKPILE-2

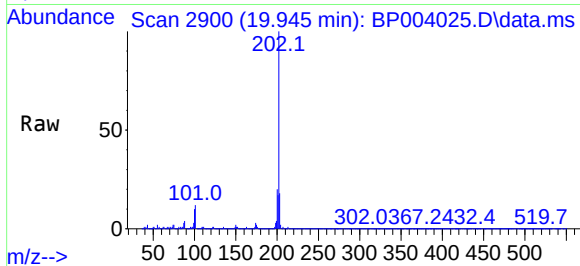


Tgt Ion:202 Resp: 509498
Ion Ratio Lower Upper
202 100
200 20.1 17.1 25.7
203 17.8 14.2 21.2

Manual Integrations
APPROVED



mohammad
11/24/2020 8:55:16 AM

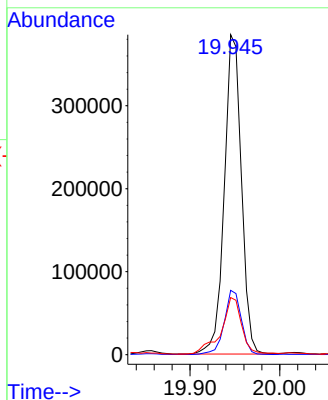


#79
Terphenyl-d14
Concen: 60.55 ng
RT: 20.122 min Scan# 2930
Delta R.T. 0.000 min
Lab File: BP004025.D
Acq: 20 Nov 2020 15:15

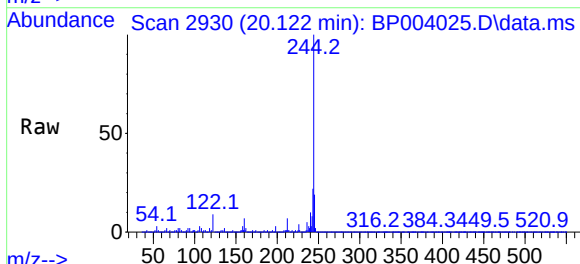


Tgt Ion:244 Resp: 1860430
Ion Ratio Lower Upper
244 100
212 7.1 5.8 8.6
122 8.8 7.8 11.8

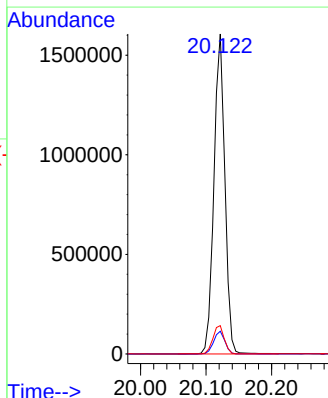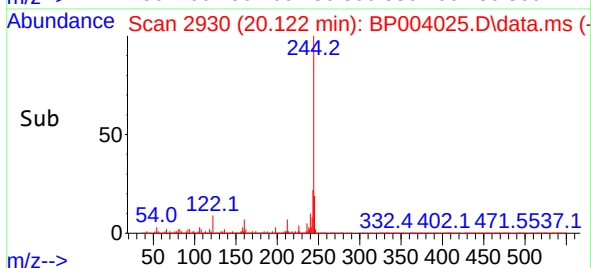



#81
Benzo(a)anthracene
Concen: 7.05 ng
RT: 21.639 min Scan# 3188
Delta R.T. 0.000 min
Lab File: BP004025.D
Acq: 20 Nov 2020 15:15




Instrument :
BNA_P
ClientSampleId :
STOCKPILE-2




Tgt Ion:228 Resp: 276033
Ion Ratio Lower Upper
228 100
226 26.0 22.1 33.1
229 21.0 15.9 23.9

Manual Integrations
APPROVED



mohammad
11/24/2020 8:55:16 AM

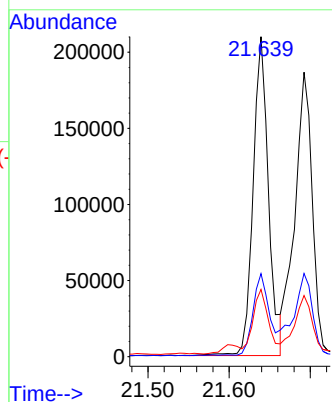


#83
Chrysene
Concen: 7.41 ng
RT: 21.692 min Scan# 3197
Delta R.T. -0.006 min
Lab File: BP004025.D
Acq: 20 Nov 2020 15:15




Tgt Ion:228 Resp: 278605
Ion Ratio Lower Upper
228 100
226 29.2 24.4 36.6
229 21.5 15.8 23.6

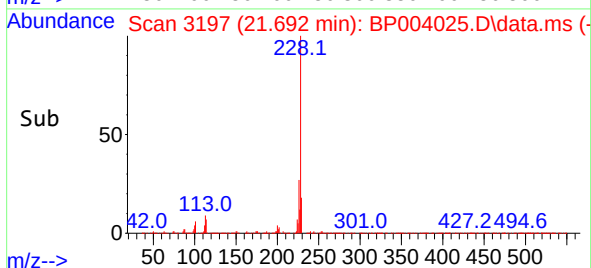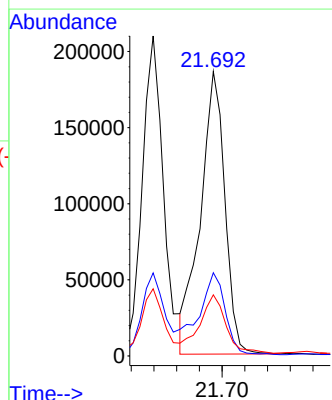



#86
Perylene-d12
Concen: 20.00 ng
RT: 24.127 min Scan# 3611
Delta R.T. 0.000 min
Lab File: BP004025.D
Acq: 20 Nov 2020 15:15




Instrument :
BNA_P
ClientSampleId :
STOCKPILE-2



Tgt Ion:264 Resp: 588822
Ion Ratio Lower Upper
264 100
260 23.3 18.8 28.2
265 22.5 17.4 26.2




Manual Integrations
APPROVED


mohammad
11/24/2020 8:55:16 AM

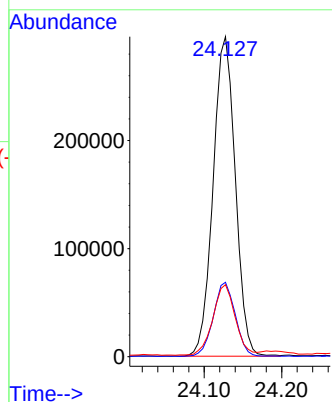

#87
Indeno(1,2,3-cd)pyrene
Concen: 4.10 ng
RT: 26.674 min Scan# 4044
Delta R.T. -0.011 min
Lab File: BP004025.D
Acq: 20 Nov 2020 15:15


Tgt Ion:276 Resp: 173986
Ion Ratio Lower Upper
276 100
138 17.4 18.7 28.1#
277 24.8 20.4 30.6

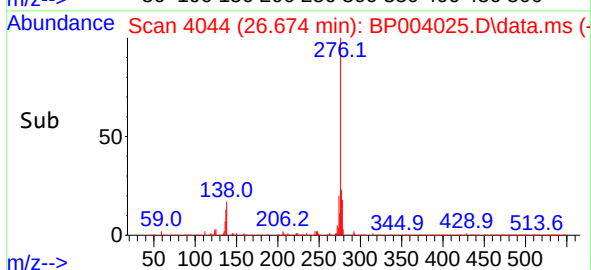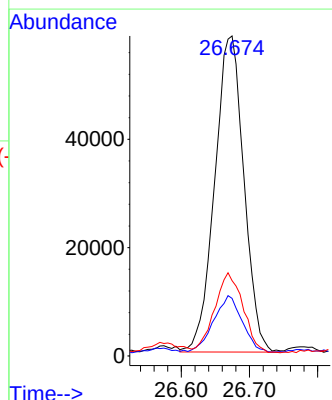



#88
Benzo(b)fluoranthene
Concen: 9.38 ng m
RT: 23.375 min Scan# 3483
Delta R.T. 0.000 min
Lab File: BP004025.D
Acq: 20 Nov 2020 15:15




Instrument :
BNA_P
ClientSampleId :
STOCKPILE-2




Tgt Ion:252 Resp: 361278
Ion Ratio Lower Upper
252 100
253 22.9 17.6 26.4
125 9.9 7.3 10.9

Manual Integrations
APPROVED



mohammad
11/24/2020 8:55:16 AM

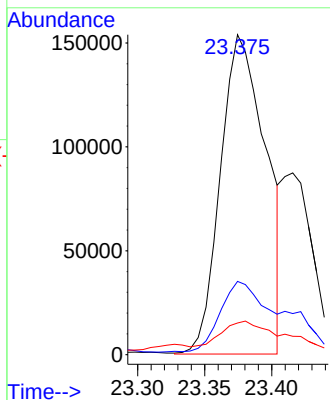


#89
Benzo(k)fluoranthene
Concen: 3.59 ng m
RT: 23.416 min Scan# 3490
Delta R.T. -0.006 min
Lab File: BP004025.D
Acq: 20 Nov 2020 15:15



Tgt Ion:252 Resp: 136404
Ion Ratio Lower Upper
252 100
253 22.6 17.8 26.8
125 10.1 7.4 11.2

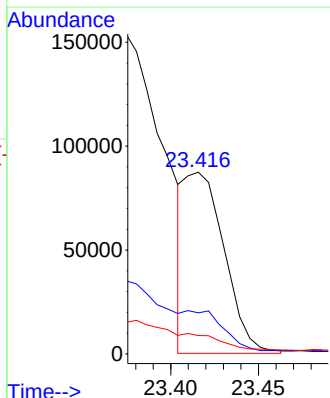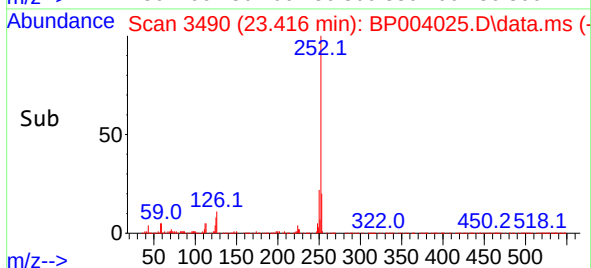







#90
Benzo(a)pyrene
Concen: 6.92 ng
RT: 24.016 min Scan# 3592
Delta R.T. 0.000 min
Lab File: BP004025.D
Acq: 20 Nov 2020 15:15

Tgt Ion:	252	Resp:	246959
Ion Ratio	Lower	Upper	
252	100		
253	23.2	17.4	26.0
125	10.3	8.2	12.4

Instrument :
BNA_P
ClientSampleId :
STOCKPILE-2

Manual Integrations
APPROVED

mohammad
11/24/2020 8:55:16 AM

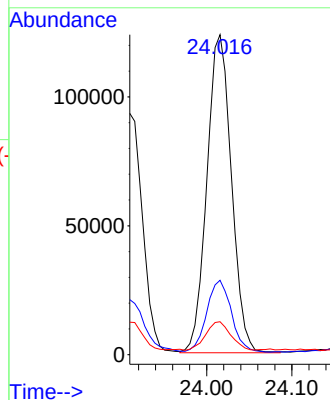

#92
Benzo(g,h,i)perylene
Concen: 5.23 ng
RT: 27.457 min Scan# 4177
Delta R.T. -0.011 min
Lab File: BP004025.D
Acq: 20 Nov 2020 15:15

Tgt Ion:	276	Resp:	179388
Ion Ratio	Lower	Upper	
276	100		
277	25.3	19.0	28.6
138	17.9	16.6	24.8

