

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112020\
 Data File : BP004026.D
 Acq On : 20 Nov 2020 16:18
 Operator : CG/JU
 Sample : L4829-15
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 MW-1A

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270E-BP110320.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP004026.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.923	3	6	18	rVB	1008742	1267824	15.95%	3.274%
2	3.075	23	32	42	rBV3	131301	339815	4.28%	0.878%
3	3.164	42	47	54	rBV	687228	974333	12.26%	2.516%
4	5.799	488	495	504	rBV	1347701	2067754	26.02%	5.340%
5	7.452	770	776	791	rVB	886511	1514202	19.05%	3.911%
6	7.916	849	855	862	rVB	60513	100295	1.26%	0.259%
7	8.263	899	914	921	rBV	506843	828513	10.43%	2.140%
8	8.828	1006	1010	1016	rVV	53632	81963	1.03%	0.212%
9	8.922	1020	1026	1032	rBV	125448	189532	2.38%	0.490%
10	9.299	1085	1090	1097	rVB2	53713	87259	1.10%	0.225%
11	9.434	1097	1113	1119	rBV	1799858	3109044	39.12%	8.030%
12	9.987	1202	1207	1213	rVB	73901	114392	1.44%	0.295%
13	10.299	1254	1260	1264	rBV2	57068	102029	1.28%	0.264%
14	10.504	1288	1295	1301	rVB3	55563	112360	1.41%	0.290%
15	10.681	1314	1325	1330	rVB3	36357	98710	1.24%	0.255%
16	11.099	1385	1396	1401	rBV	650053	1163003	14.63%	3.004%
17	11.146	1401	1404	1413	rVB	135253	266936	3.36%	0.689%
18	12.734	1665	1674	1680	rBV5	40240	112781	1.42%	0.291%
19	13.516	1800	1807	1820	rBV	4399094	6411551	80.68%	16.559%
20	14.316	1938	1943	1953	rBV	162567	230935	2.91%	0.596%
21	14.892	2035	2041	2048	rVB2	955398	1392029	17.52%	3.595%
22	16.381	2287	2294	2308	rBV	3262495	4656167	58.59%	12.026%
23	17.628	2500	2506	2514	rBV	1133152	1570643	19.76%	4.057%
24	20.127	2926	2931	2936	rBV	6604236	7946979	100.00%	20.525%
25	20.839	3048	3052	3055	rBV	212698	246943	3.11%	0.638%
26	21.310	3129	3132	3141	rVV3	211230	337315	4.24%	0.871%
27	21.386	3142	3145	3153	rVB	121744	149747	1.88%	0.387%
28	21.663	3187	3192	3197	rBV	1235607	1568120	19.73%	4.050%
29	24.139	3606	3613	3623	rVB	802954	1677814	21.11%	4.333%




Sum of corrected areas: 38718988

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112020\
Data File : BP004026.D
Acq On : 20 Nov 2020 16:18
Operator : CG/JU
Sample : L4829-15
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
MW-1A

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

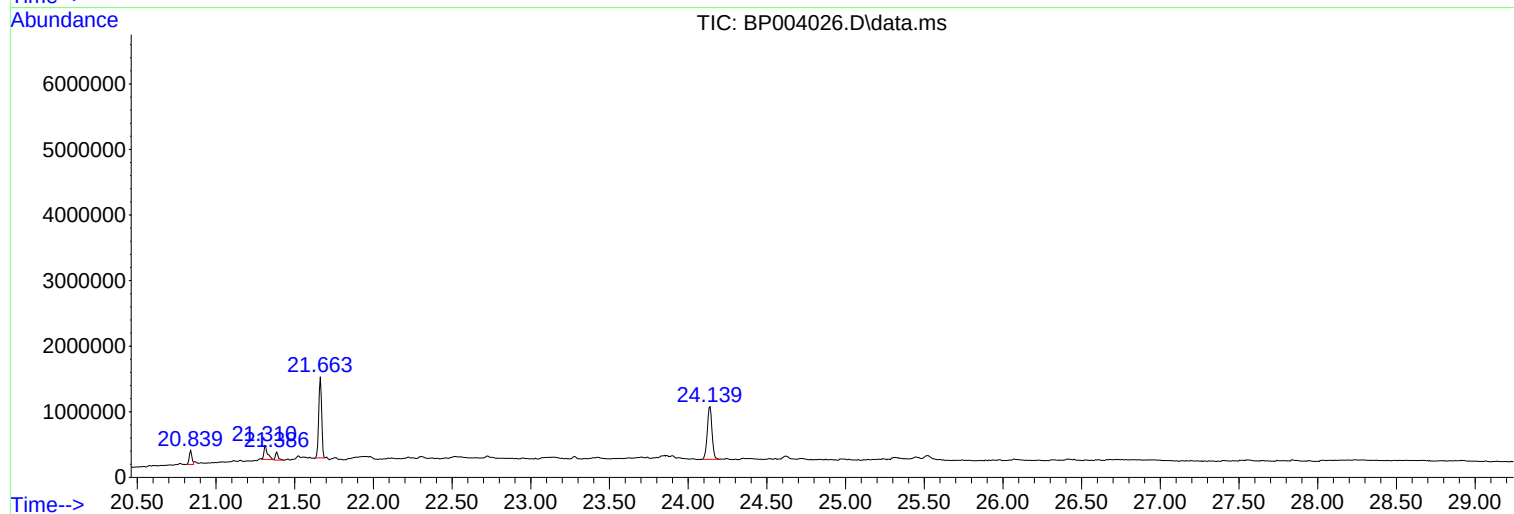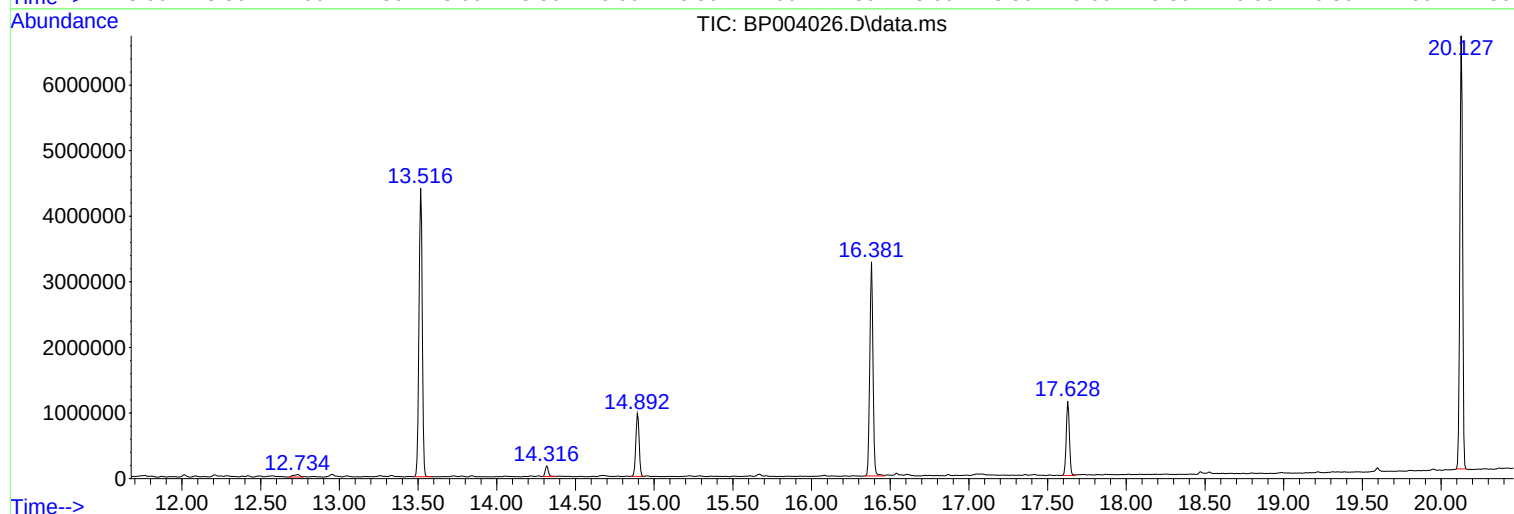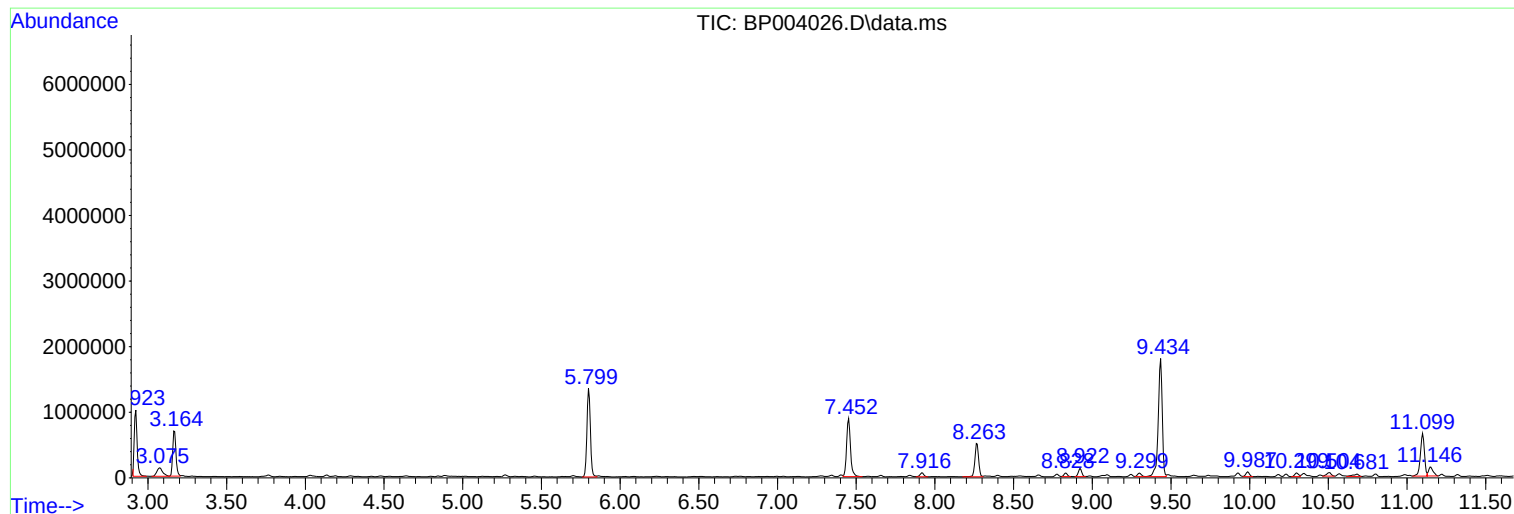

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112020\
Data File : BP004026.D
Acq On : 20 Nov 2020 16:18
Operator : CG/JU
Sample : L4829-15
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
MW-1A

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112020\
Data File : BP004026.D
Acq On : 20 Nov 2020 16:18
Operator : CG/JU
Sample : L4829-15
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
MW-1A

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc