
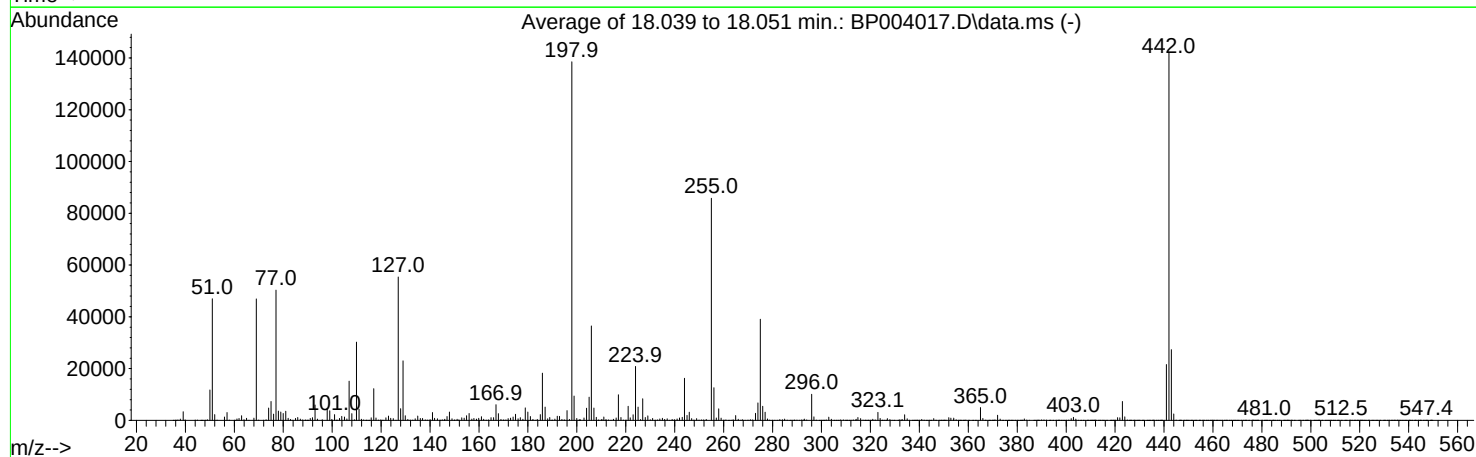


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112020\
Data File : BP004017.D
Acq On : 20 Nov 2020 10:27
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110320.M
Title : D
Last Update : Fri Nov 20 12:19:10 2020

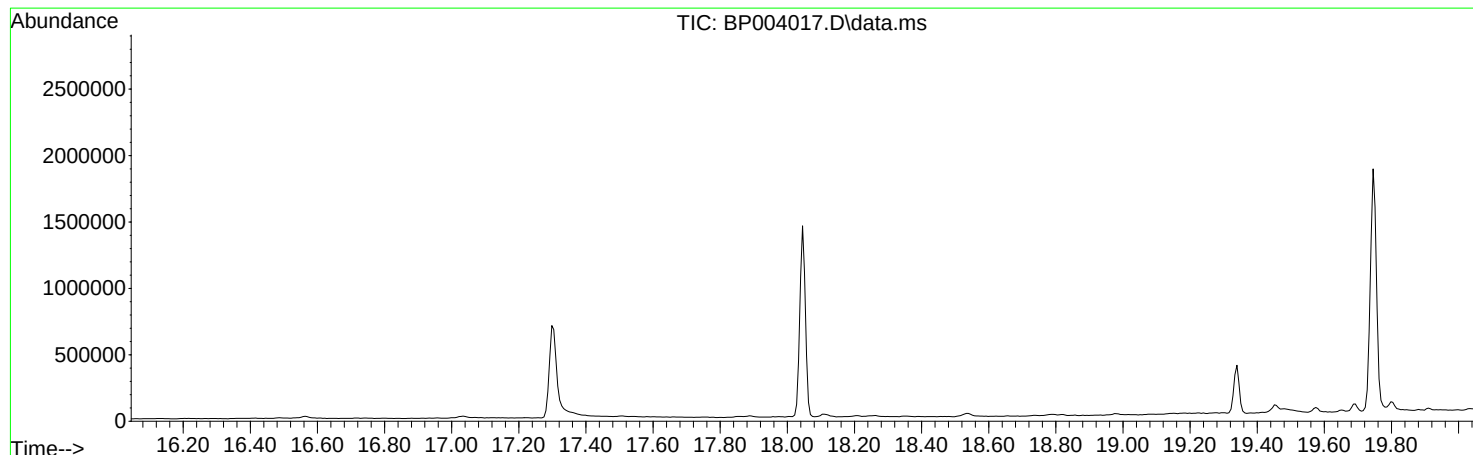

AutoFind: Scans 2576, 2577, 2578; Background Corrected with Scan 2565

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.9	46958	PASS
68	69	0.00	2	1.8	860	PASS
69	198	0.00	100	33.9	46950	PASS
70	69	0.00	2	0.2	99	PASS
127	198	10	80	40.0	55394	PASS
197	198	0.00	2	0.3	400	PASS
198	198	100	100	100.0	138515	PASS
199	198	5	9	6.8	9386	PASS
275	198	10	60	28.2	39073	PASS
365	198	1	100	3.6	4953	PASS
441	198	0.01	100	15.6	21585	PASS
442	442	100	100	100.0	142107	PASS
443	442	15	24	19.2	27309	PASS