
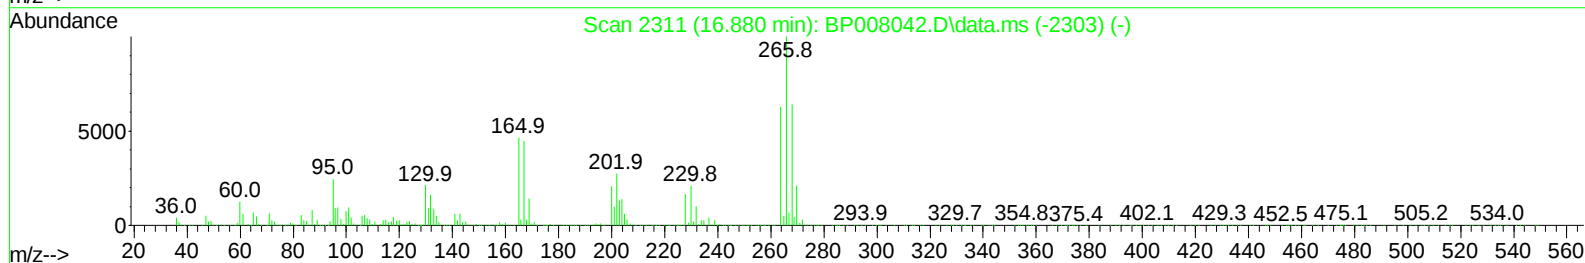
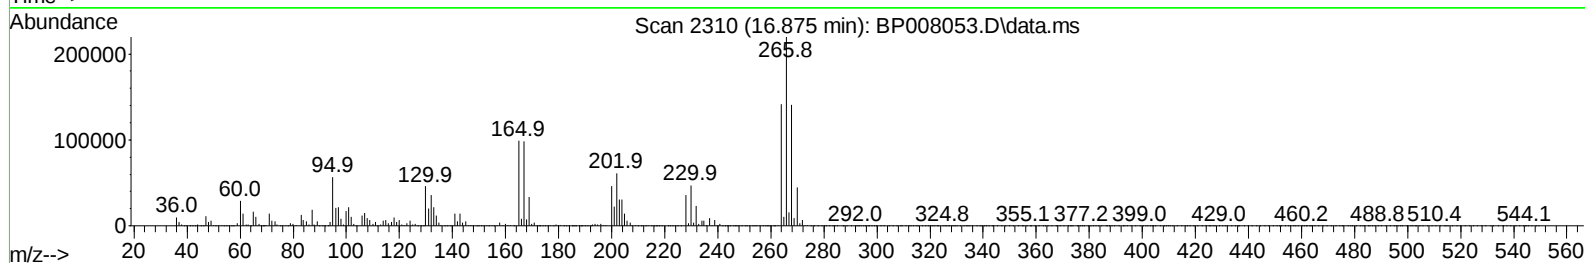


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112021\
Data File : BP008053.D
Acq On : 20 Nov 2021 12:34
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 22 07:15:06 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 20 00:21:11 2021
Response via : Initial Calibration

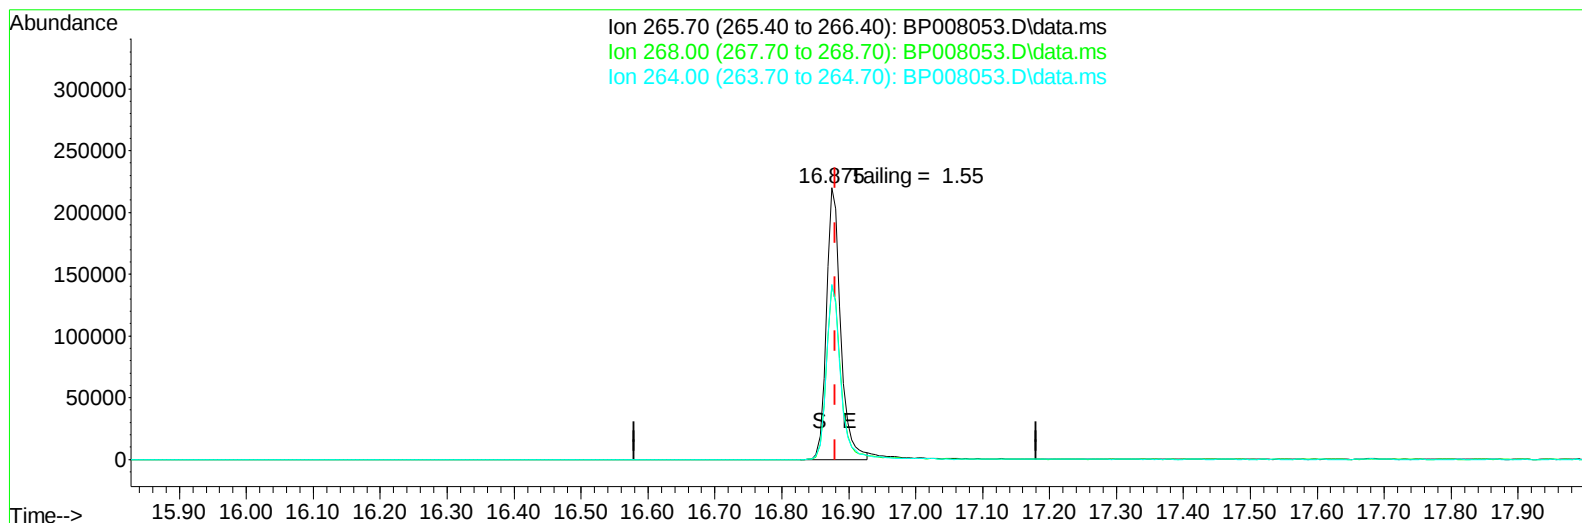

TIC: BP008053.D\data.ms

(70) Pentachlorophenol (C)




16.875min (-0.005) 1542508.19 ng

response 337232

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.10	64.13
264.00	62.80	64.54
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112021\
Data File : BP008053.D
Acq On : 20 Nov 2021 12:34
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 22 07:15:06 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 20 00:21:11 2021
Response via : Initial Calibration

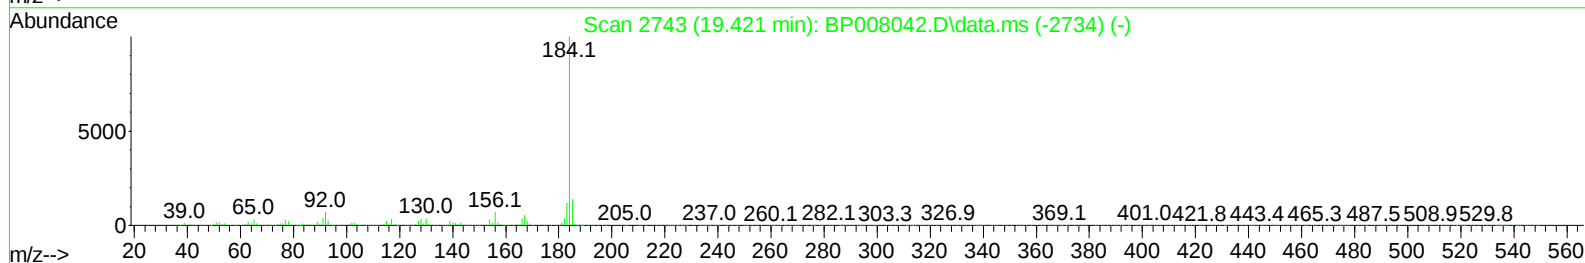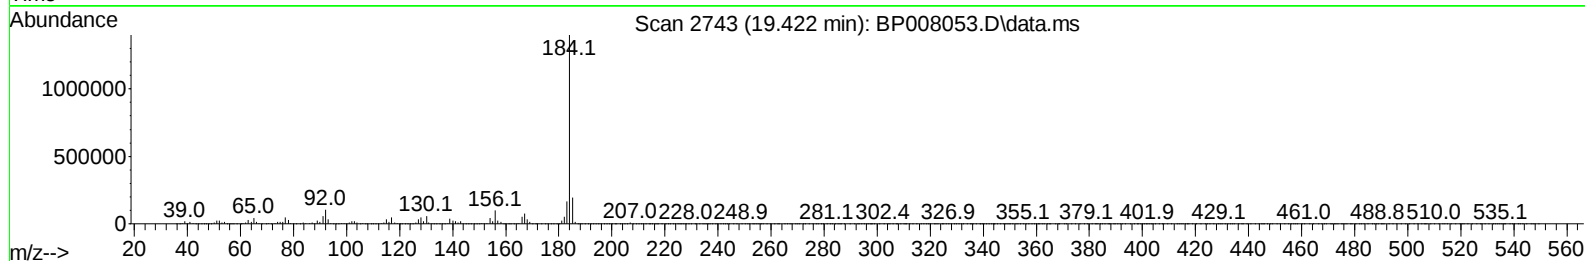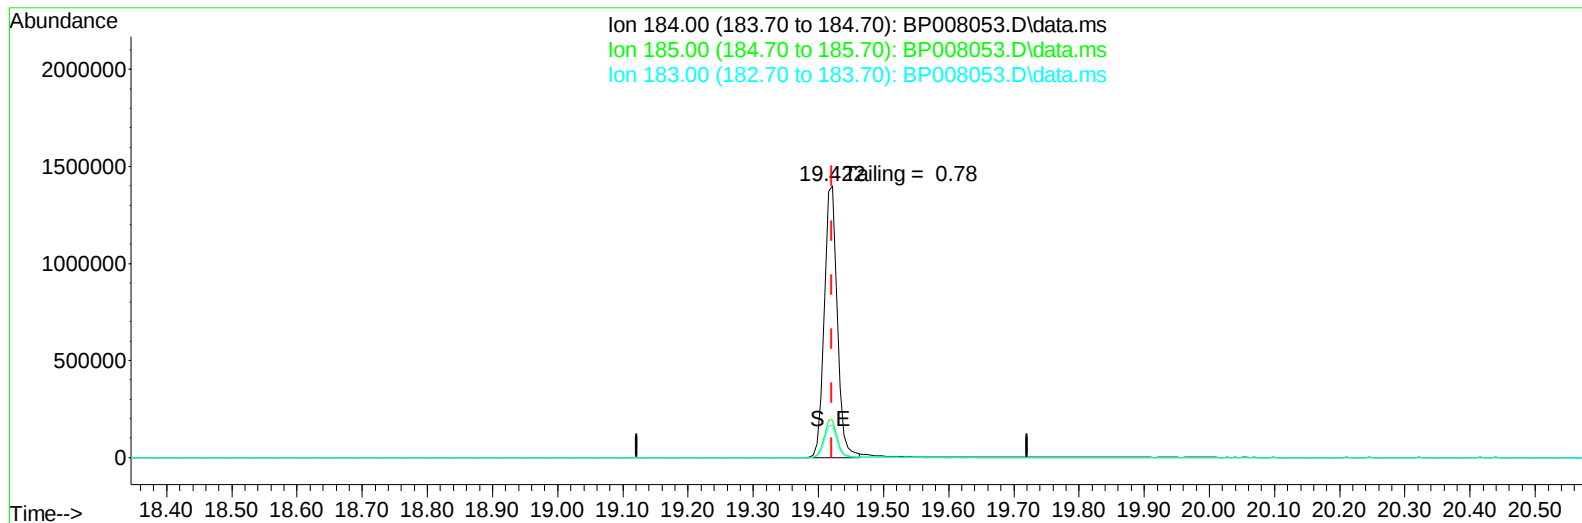

TIC: BP008053.D\data.ms

(77) Benzidine

19.422min (+ 0.001) 1416338.99 ng

response 1973130

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	13.84
183.00	11.80	11.88
0.00	0.00	0.00