


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112021\
 Data File : BP008053.D
 Acq On : 20 Nov 2021 12:34
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111921.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Nov 20 00:21:11 2021

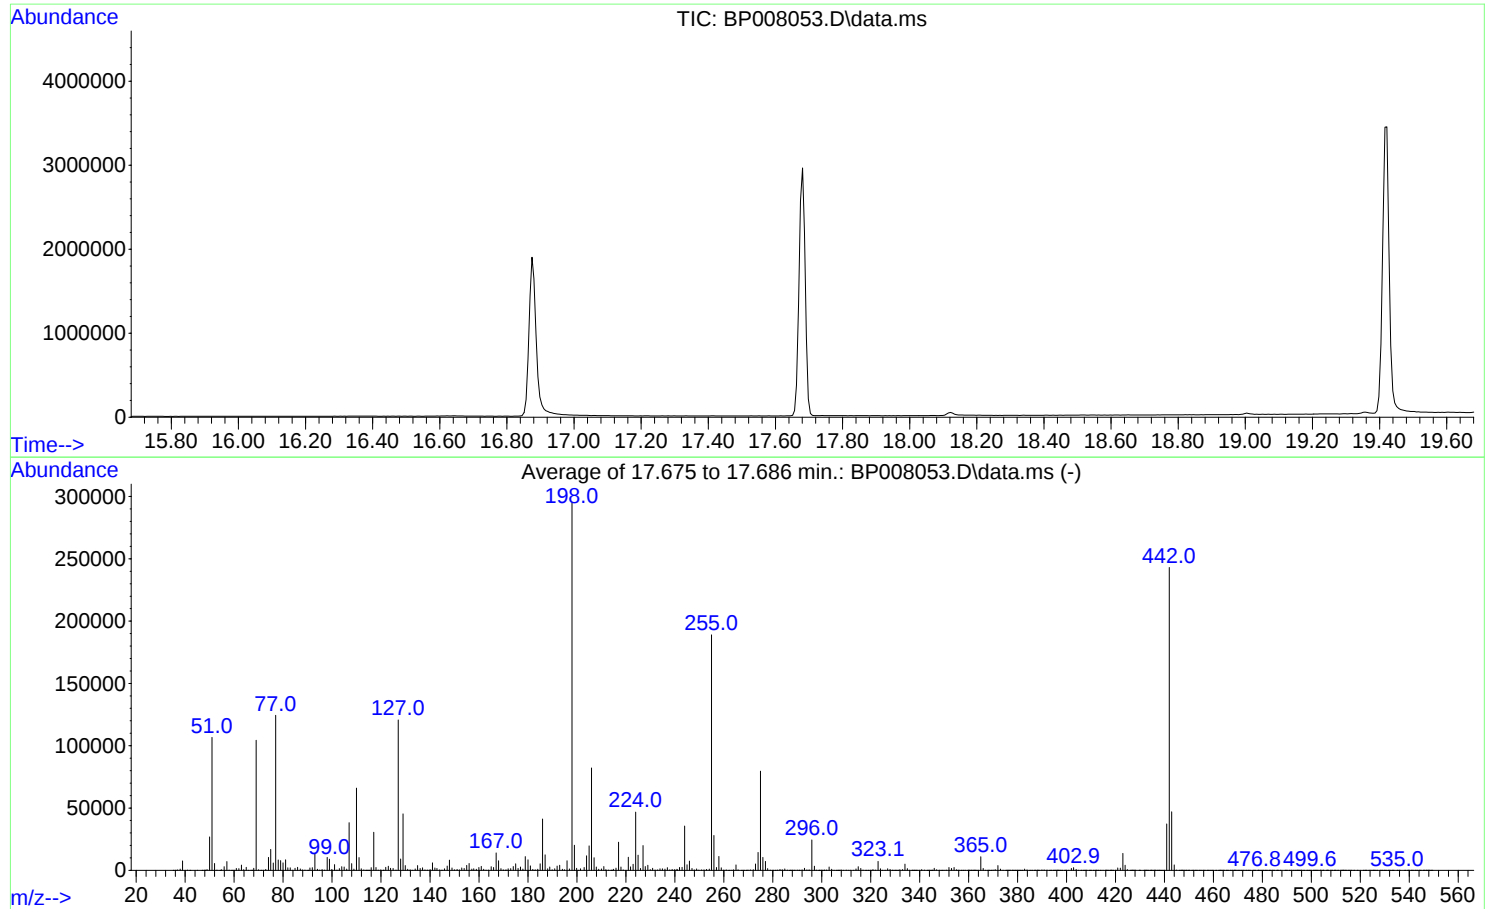

AutoFind: Scans 2446, 2447, 2448; Background Corrected with Scan 2438

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.1	106702	PASS
68	69	0.00	2	1.7	1727	PASS
69	198	0.00	100	35.4	104411	PASS
70	69	0.00	2	0.5	487	PASS
127	198	10	80	40.9	120757	PASS
197	198	0.00	2	0.4	1142	PASS
198	198	100	100	100.0	295189	PASS
199	198	5	9	6.8	20142	PASS
275	198	10	60	27.0	79664	PASS
365	198	1	100	3.7	10873	PASS
441	198	0.01	100	12.6	37215	PASS
442	442	100	100	100.0	243059	PASS
443	442	15	24	19.4	47066	PASS