
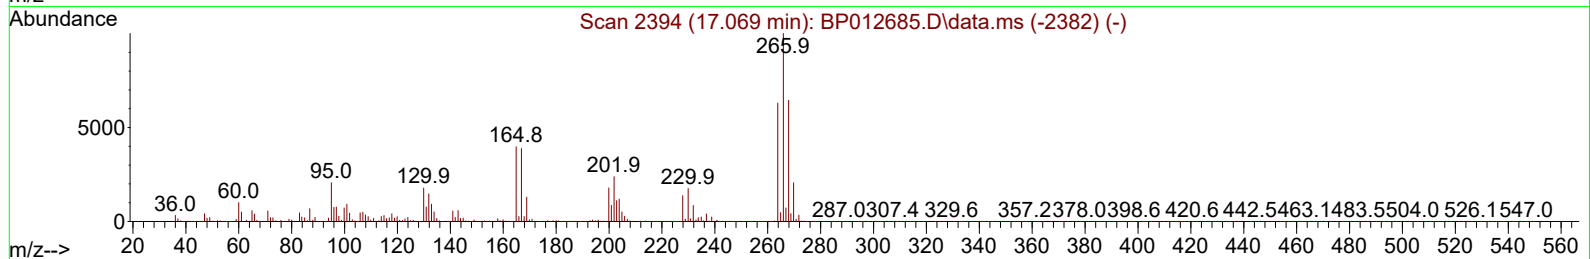
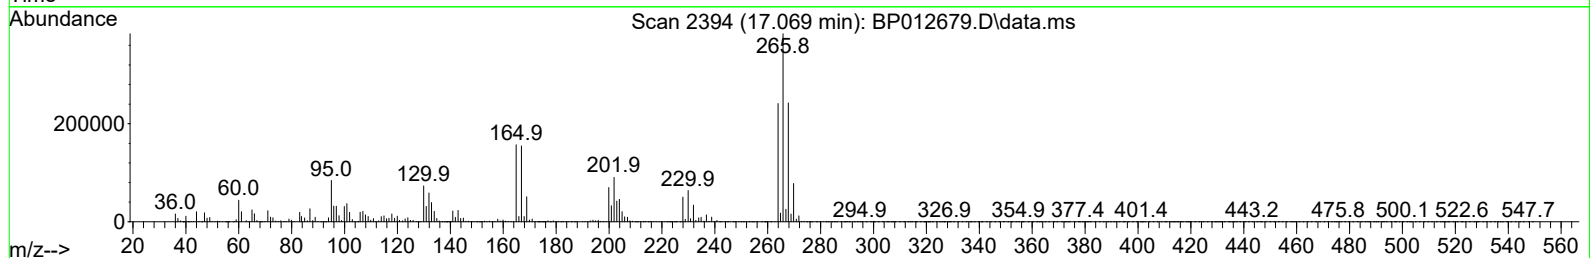


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112122\
Data File : BP012679.D
Acq On : 21 Nov 2022 09:41
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 22 05:57:14 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 21 23:51:17 2022
Response via : Initial Calibration

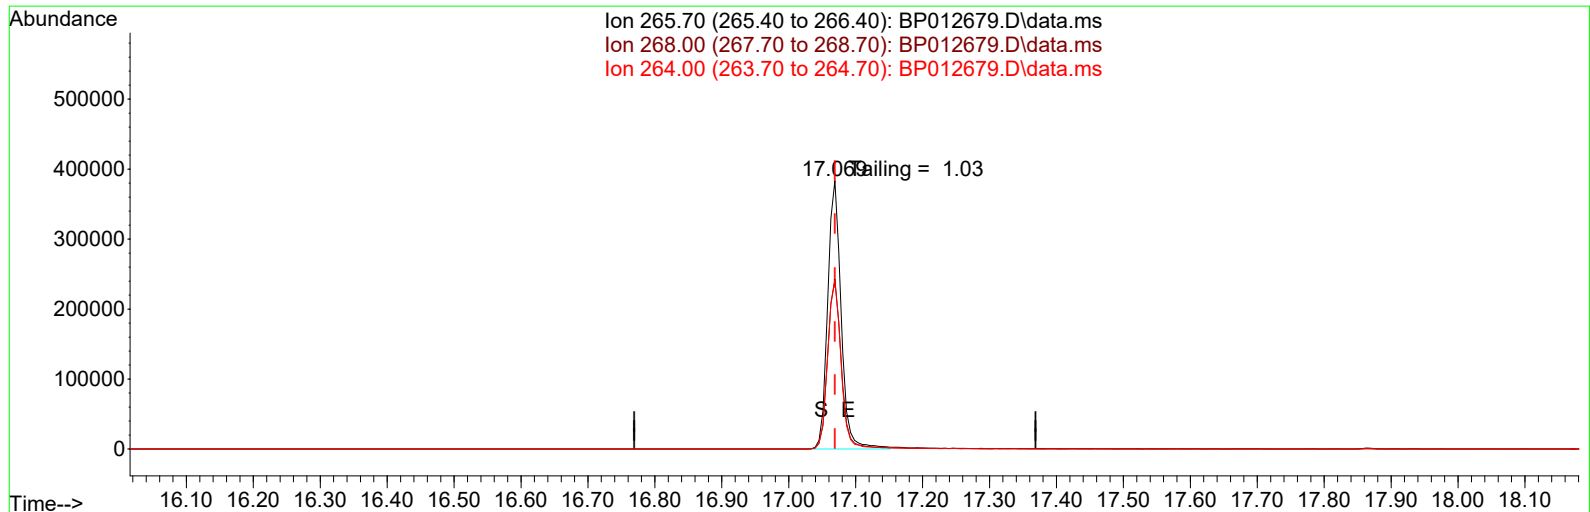

TIC: BP012679.D\data.ms

(70) Pentachlorophenol (C)




17.069min (-0.000) 911759.91 ng

response 540282

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	63.22
264.00	63.00	62.86
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112122\
 Data File : BP012679.D
 Acq On : 21 Nov 2022 09:41
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 22 05:57:14 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 21 23:51:17 2022
 Response via : Initial Calibration

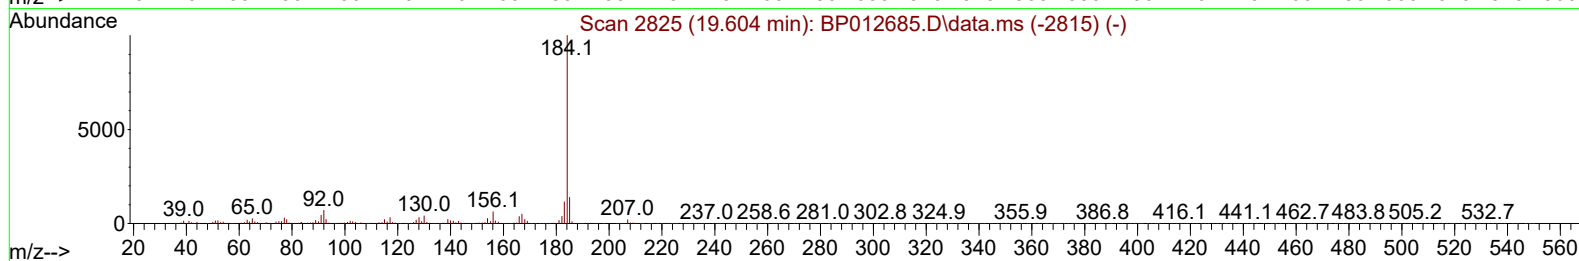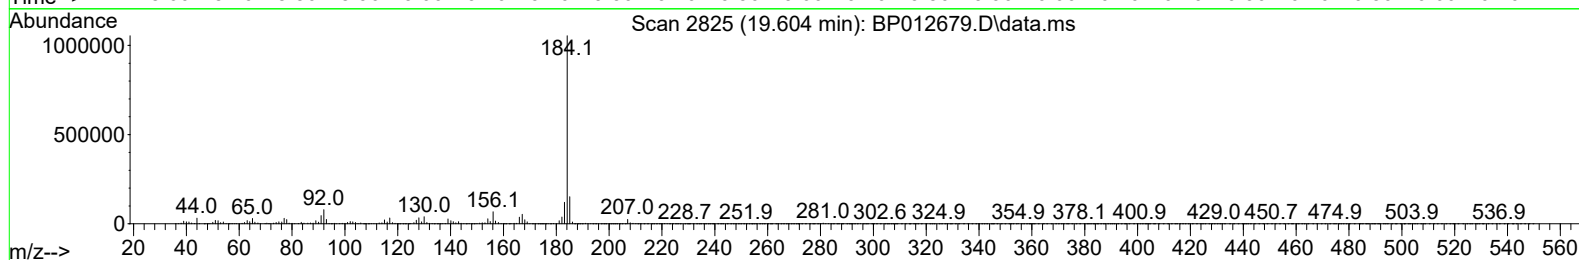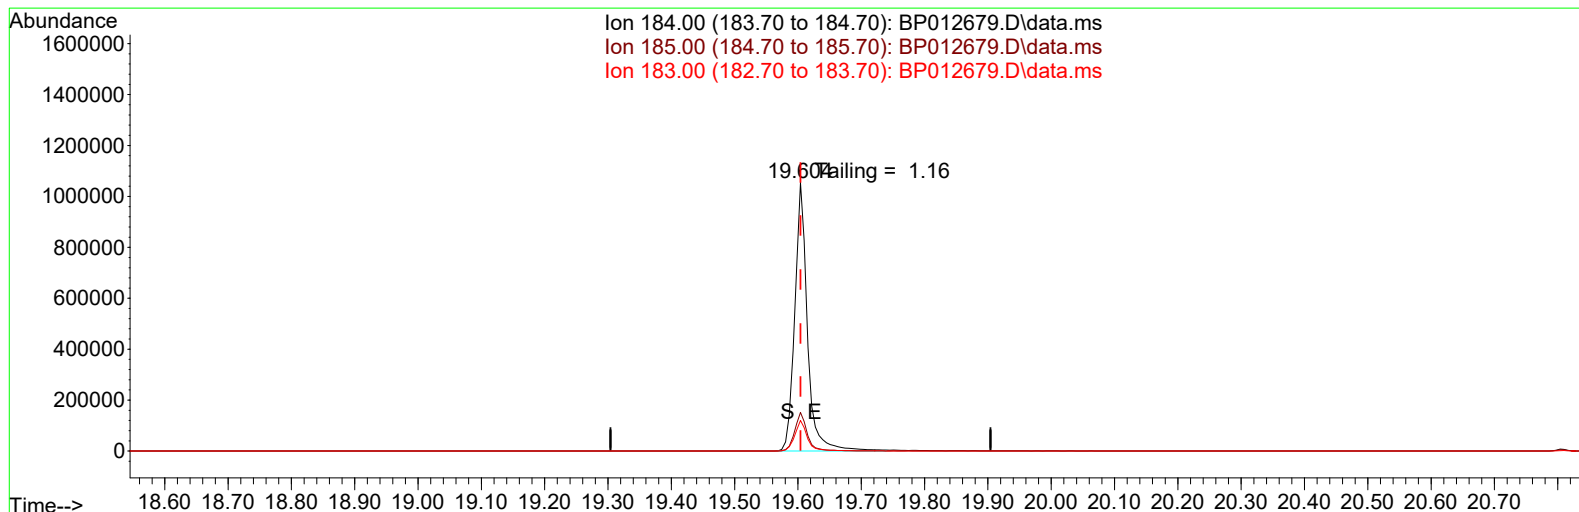

TIC: BP012679.D\data.ms

(77) Benzidine**19.604min (-0.000) 1440216.72 ng****response 1484394**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	14.41
183.00	11.50	11.42
0.00	0.00	0.00