


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112122\
 Data File : BP012679.D
 Acq On : 21 Nov 2022 09:41
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112122.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Nov 21 23:51:17 2022

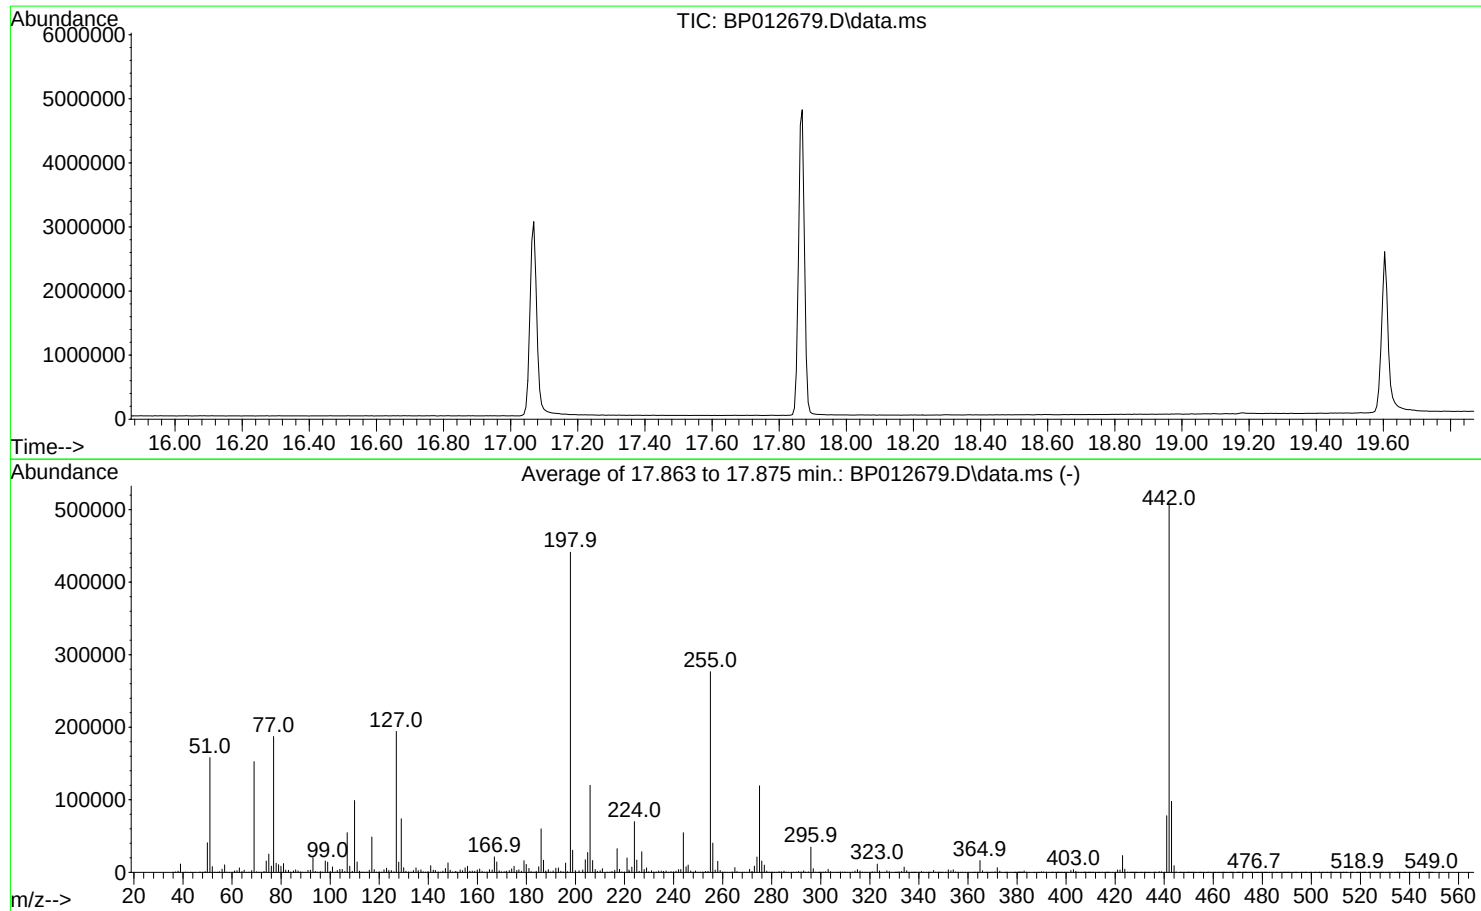




AutoFind: Scans 2529, 2530, 2531; Background Corrected with Scan 2518

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.8	158029	PASS
68	69	0.00	2	1.5	2314	PASS
69	198	0.00	100	34.6	152511	PASS
70	69	0.00	2	0.5	727	PASS
127	198	10	80	44.0	194164	PASS
197	198	0.00	2	0.2	751	PASS
198	198	100	100	100.0	441365	PASS
199	198	5	9	6.9	30284	PASS
275	198	10	60	27.0	119200	PASS
365	198	1	100	3.7	16311	PASS
441	198	0.01	100	17.7	77916	PASS
442	442	100	100	100.0	507179	PASS
443	442	15	24	19.3	97768	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112122\
Data File : BP012679.D
Acq On : 21 Nov 2022 09:41
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Nov 22 05:57:14 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 21 23:51:17 2022
Response via : Initial Calibration

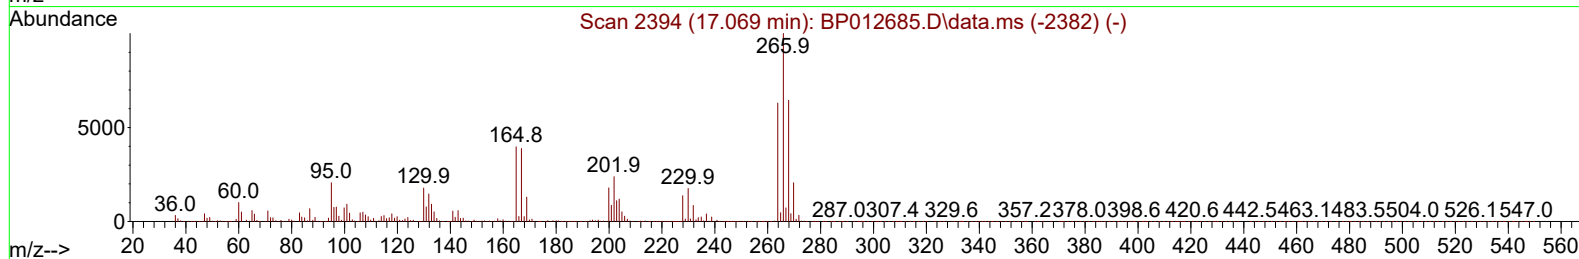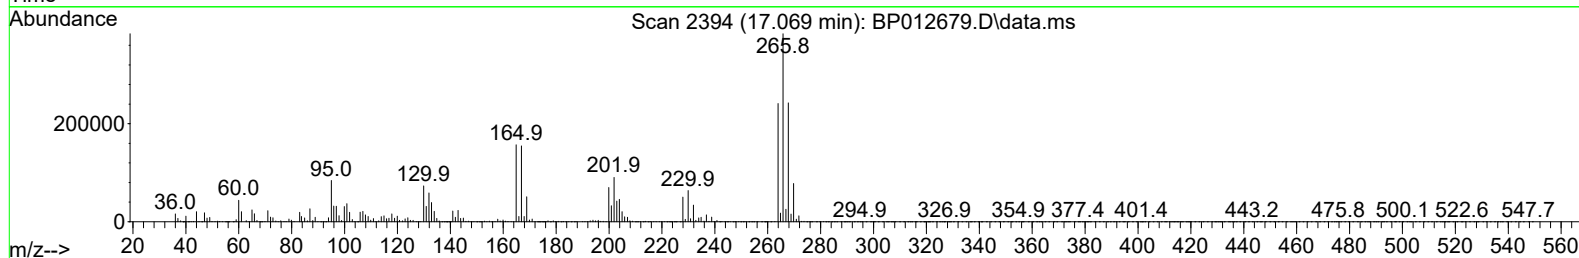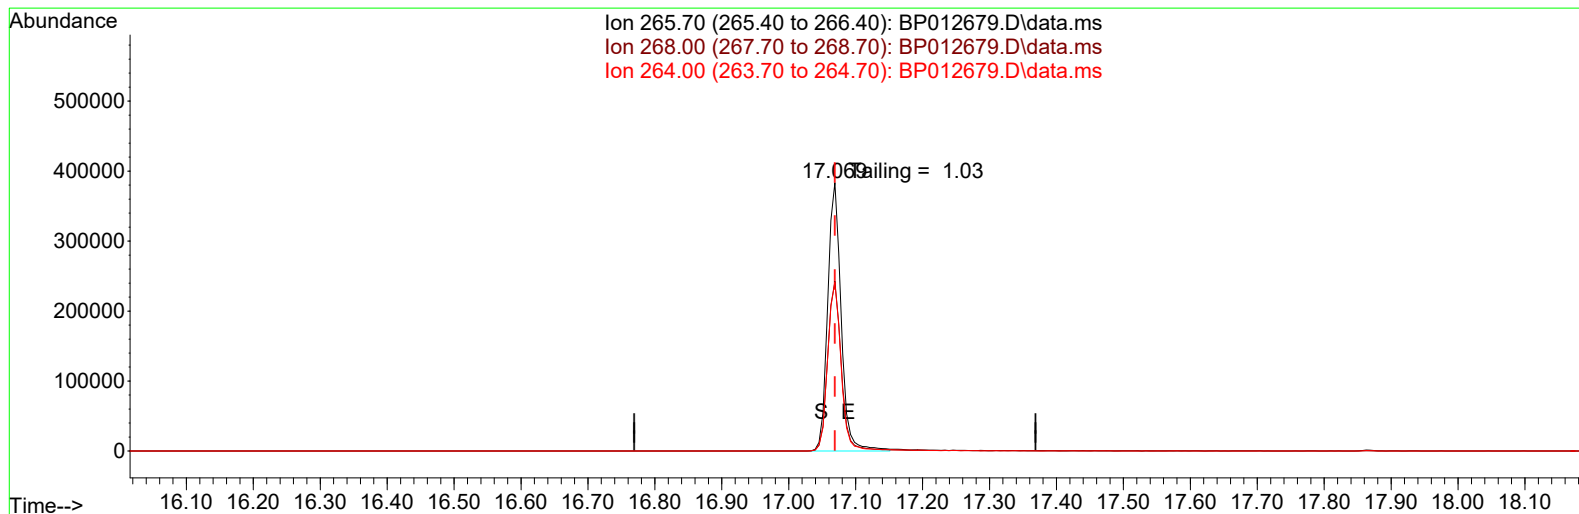

TIC: BP012679.D\data.ms

(70) Pentachlorophenol (C)

17.069min (-0.000) 911759.91 ng




response 540282

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	63.22
264.00	63.00	62.86
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112122\
 Data File : BP012679.D
 Acq On : 21 Nov 2022 09:41
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Nov 22 05:57:14 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 21 23:51:17 2022
 Response via : Initial Calibration

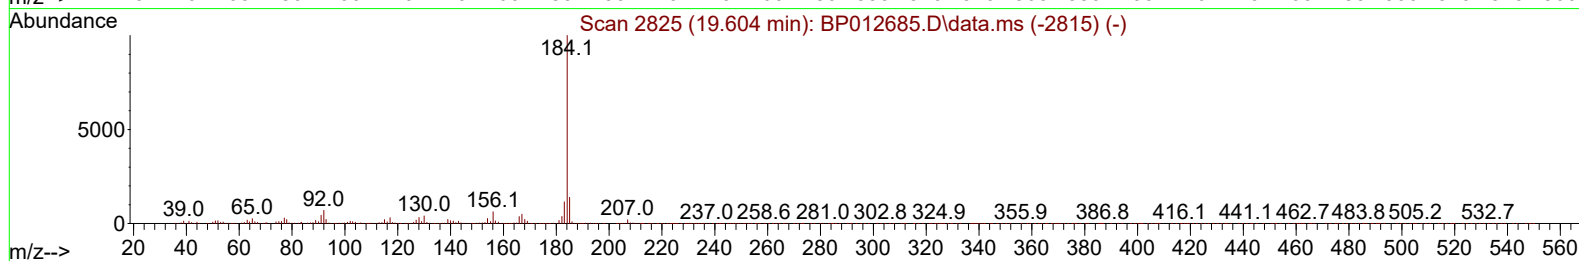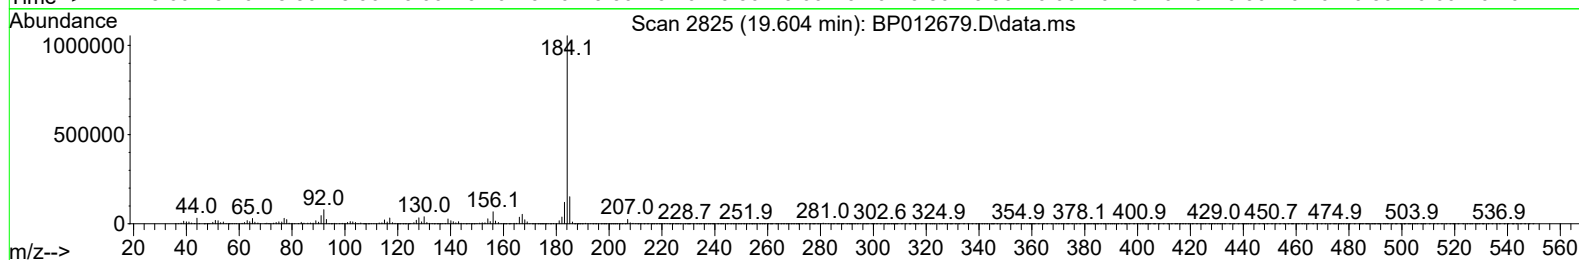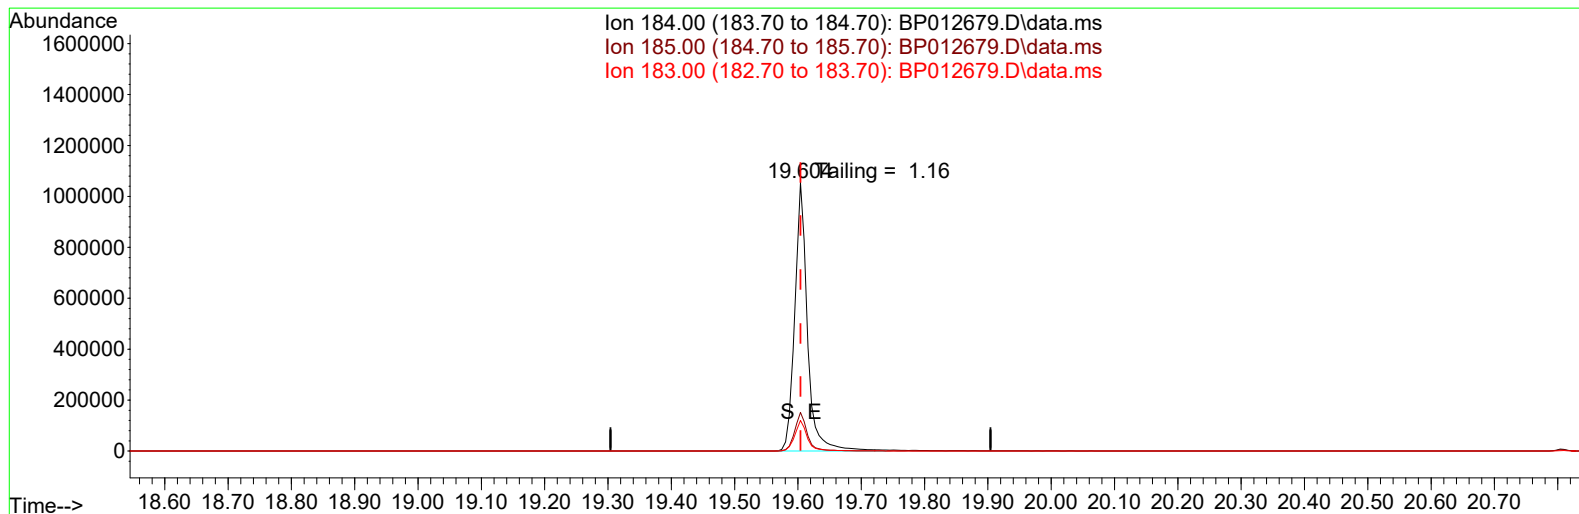

TIC: BP012679.D\data.ms

(77) Benzidine

19.604min (-0.000) 1440216.72 ng

response 1484394

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	14.41
183.00	11.50	11.42
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/21/2022	BNA_P	<u>BP012679.D</u>
Compound Name	Response	Retention Time
DDT	989750	20.81
DDD	15554	20.374
DDE	1284	19.88
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
16838	1006588	1.67

Instrument :
BNA_P
ClientSampleId :
DFTPP