
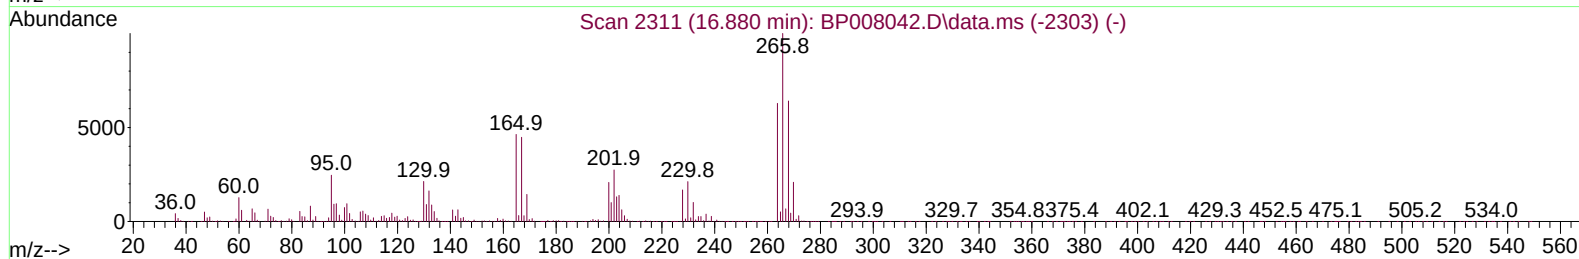
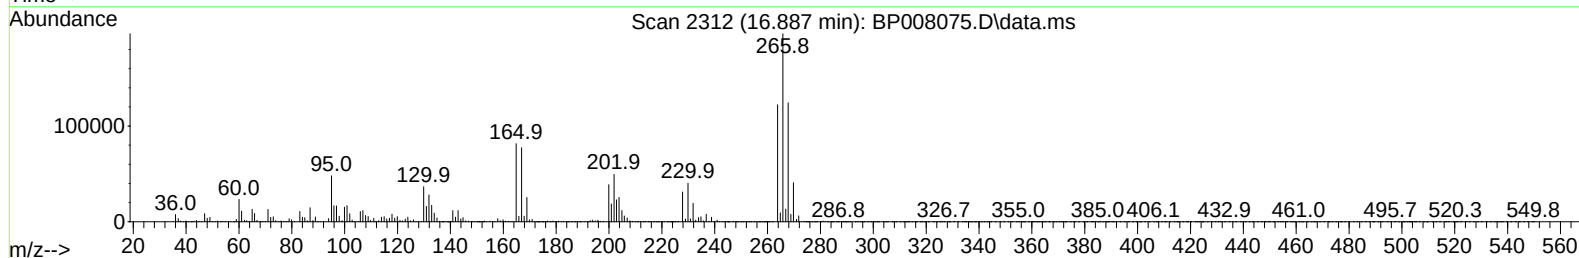


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112221\
Data File : BP008075.D
Acq On : 22 Nov 2021 10:36
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 23 03:03:25 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 20 00:21:11 2021
Response via : Initial Calibration

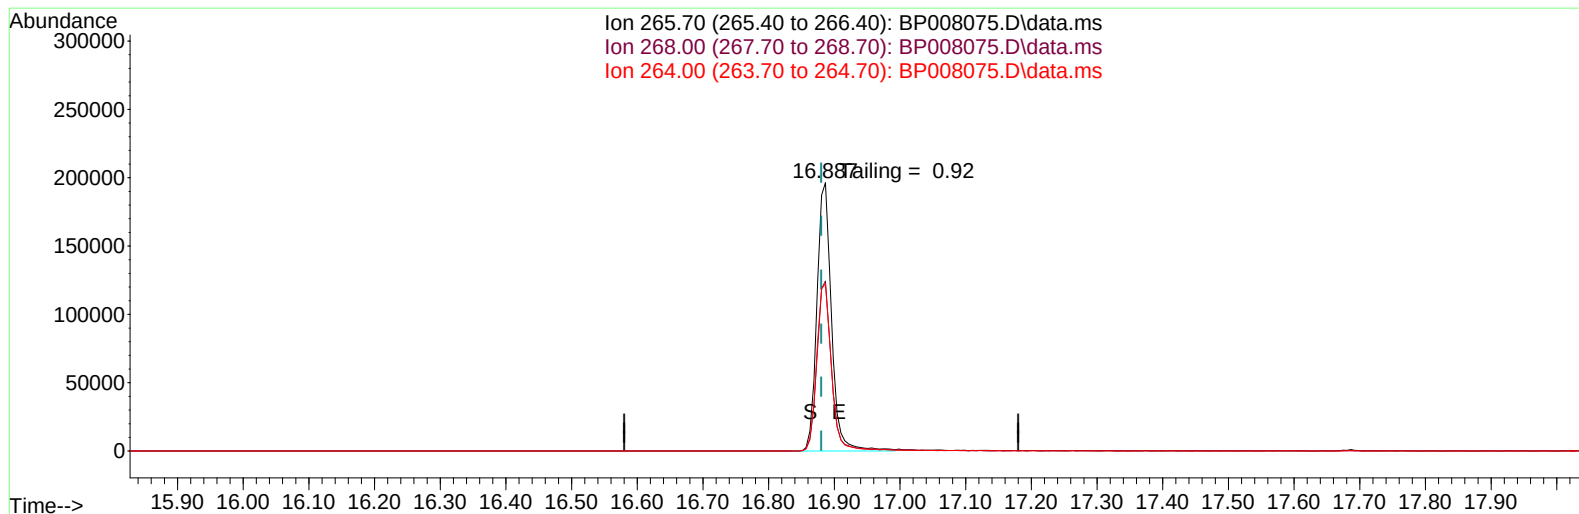

TIC: BP008075.D\data.ms

(70) Pentachlorophenol (C)




16.887min (+ 0.007) 70755.13 ng

response 305644

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.10	63.31
264.00	62.80	62.25
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112221\
 Data File : BP008075.D
 Acq On : 22 Nov 2021 10:36
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 23 03:03:25 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111921.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Nov 20 00:21:11 2021
 Response via : Initial Calibration

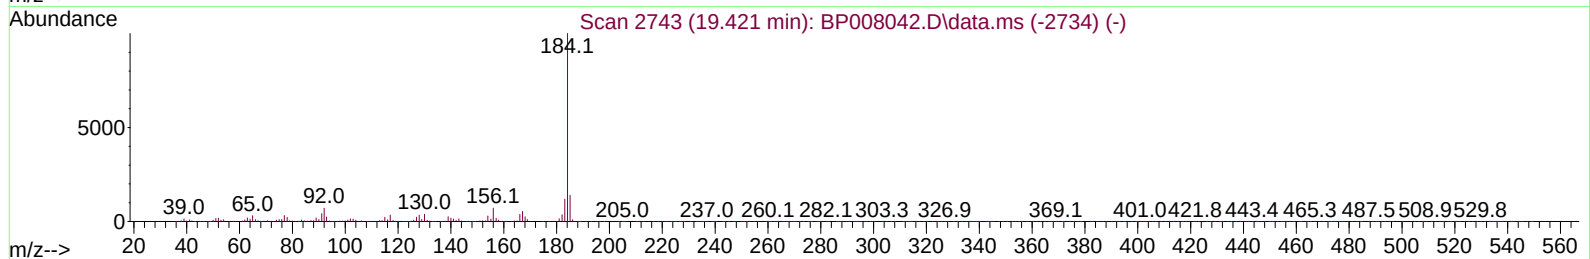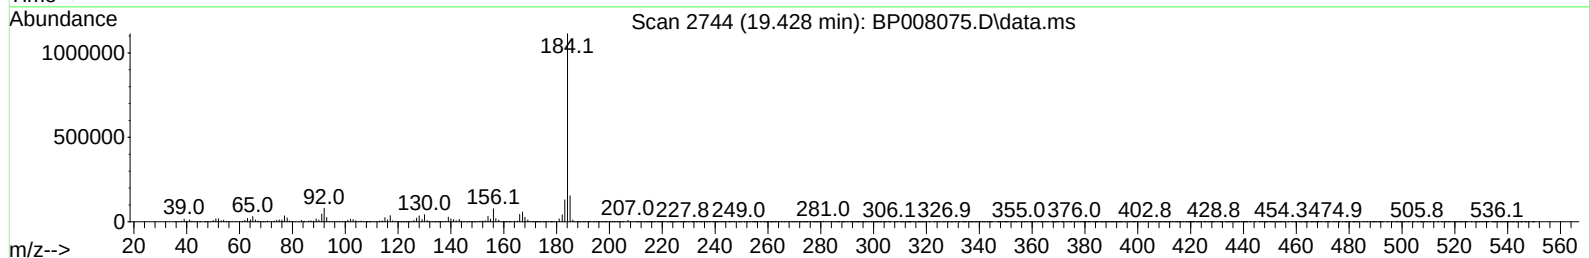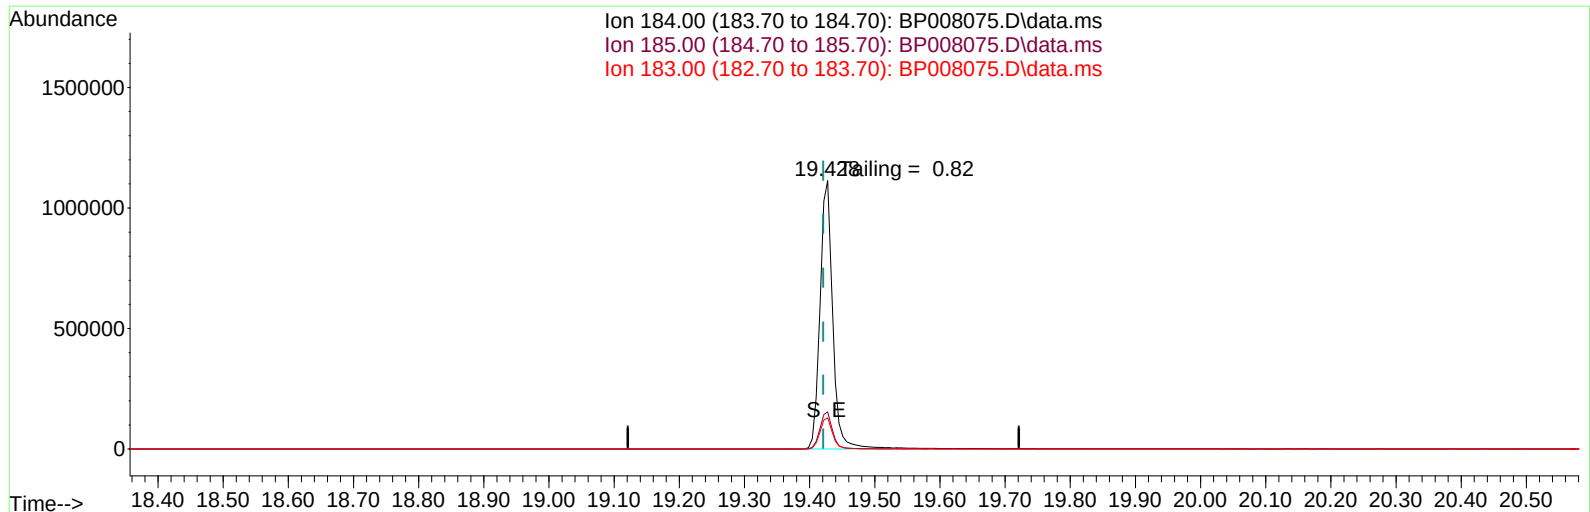

TIC: BP008075.D\data.ms

(77) Benzidine**19.428min (+ 0.007) 63822.61 ng****response 1515959**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	13.83
183.00	11.80	11.62
0.00	0.00	0.00