
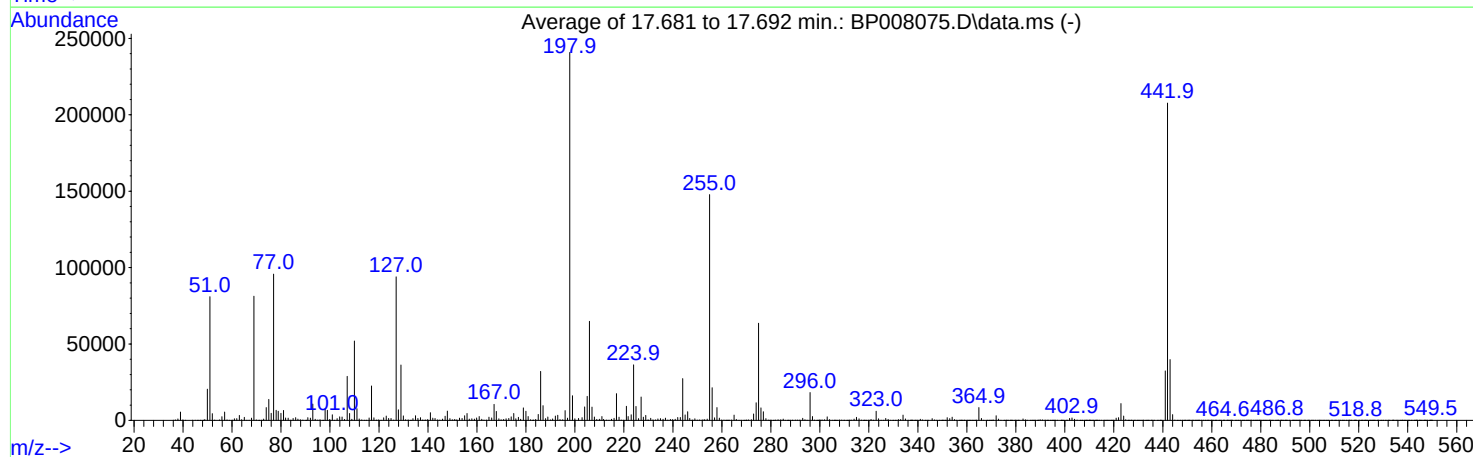


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112221\
 Data File : BP008075.D
 Acq On : 22 Nov 2021 10:36
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111921.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Nov 20 00:21:11 2021

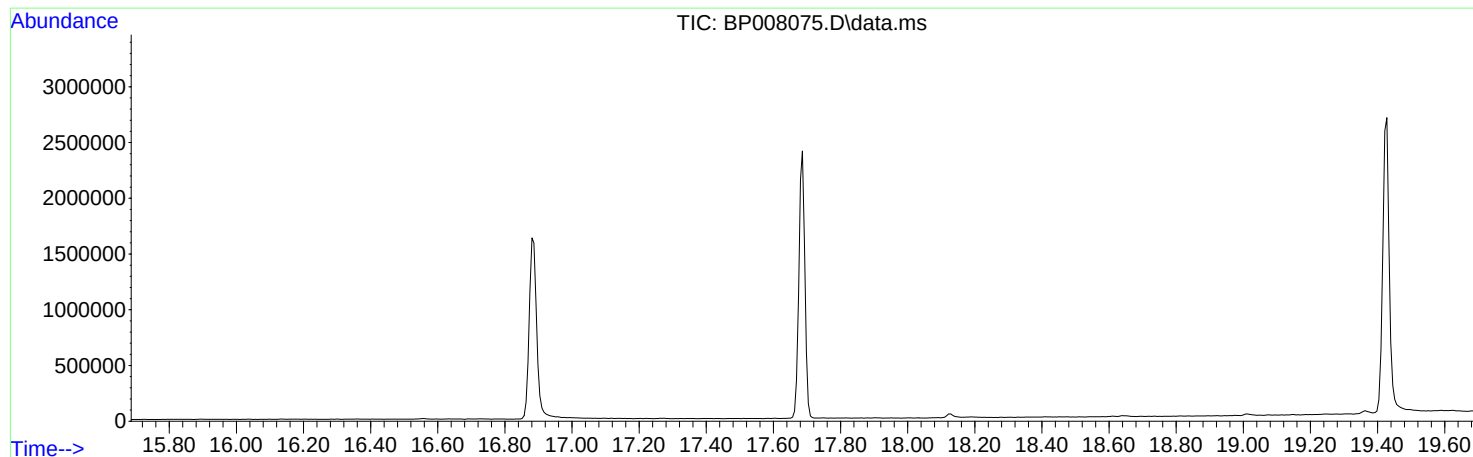




AutoFind: Scans 2447, 2448, 2449; Background Corrected with Scan 2439

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.6	80989	PASS
68	69	0.00	2	1.8	1430	PASS
69	198	0.00	100	33.8	81303	PASS
70	69	0.00	2	0.4	341	PASS
127	198	10	80	39.0	93988	PASS
197	198	0.00	2	0.6	1497	PASS
198	198	100	100	100.0	240748	PASS
199	198	5	9	6.7	16173	PASS
275	198	10	60	26.4	63599	PASS
365	198	1	100	3.5	8380	PASS
441	198	0.01	100	13.4	32320	PASS
442	442	100	100	100.0	207675	PASS
443	442	15	24	19.2	39821	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112221\
 Data File : BP008075.D
 Acq On : 22 Nov 2021 10:36
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Nov 23 03:03:25 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111921.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Nov 20 00:21:11 2021
 Response via : Initial Calibration

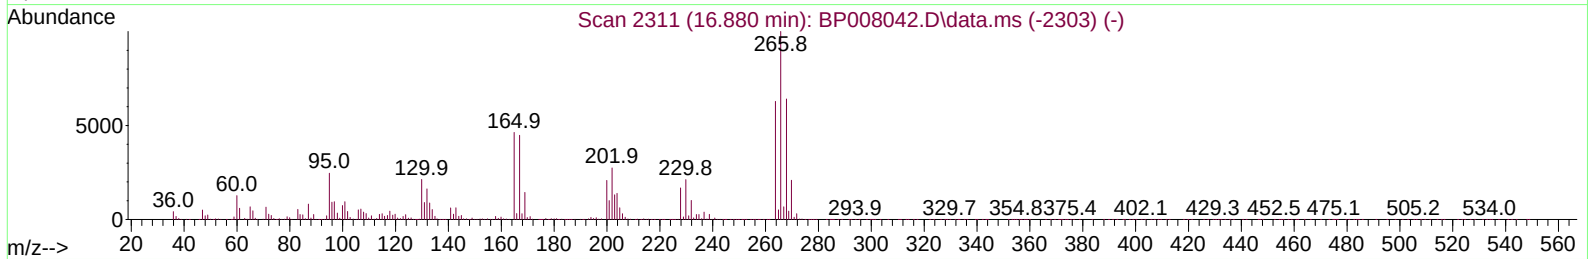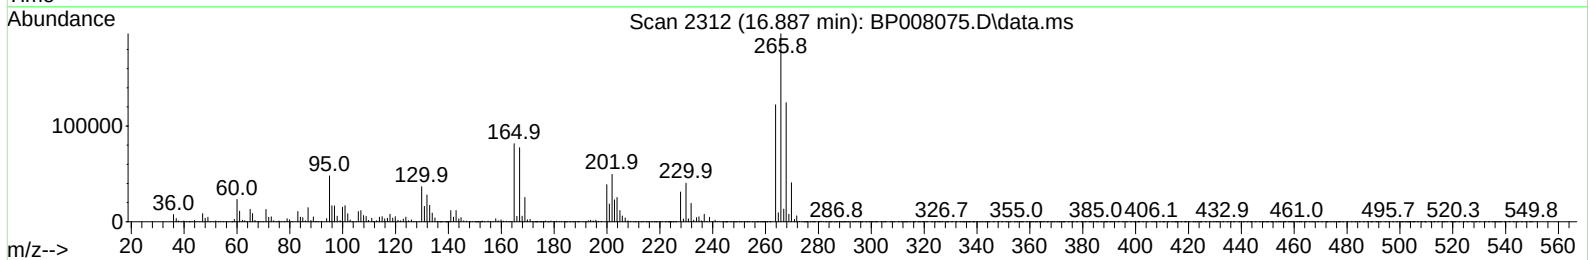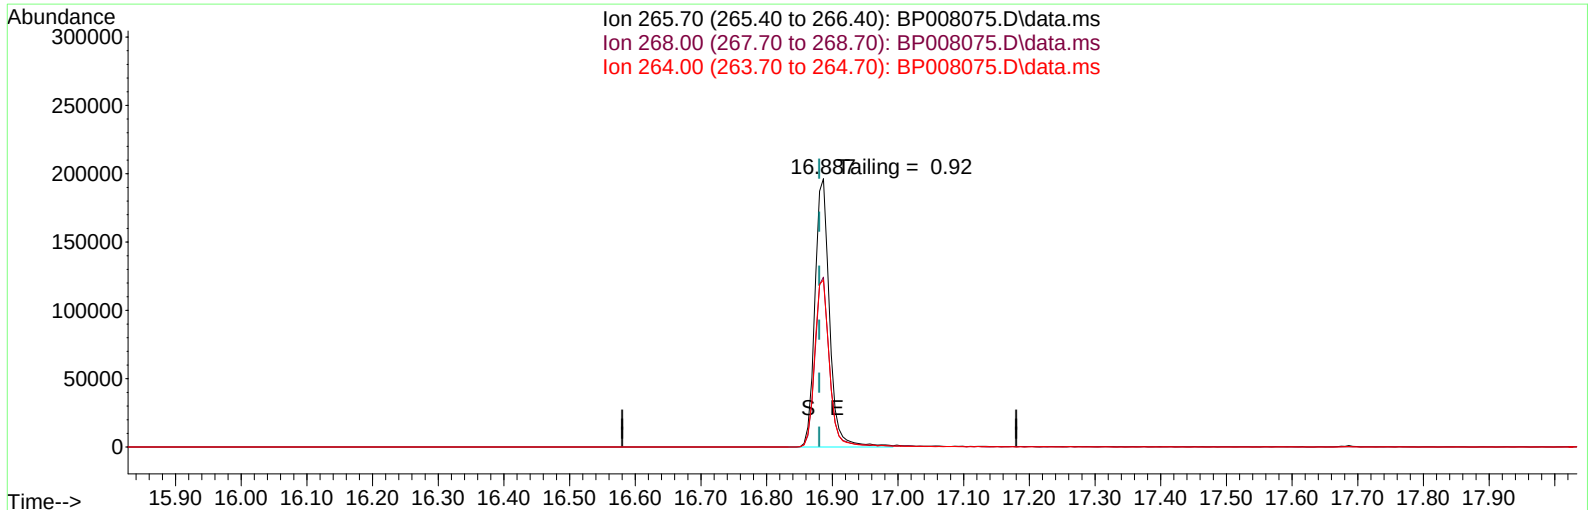

TIC: BP008075.D\data.ms

(70) Pentachlorophenol (C)

16.887min (+ 0.007) 70755.13 ng




response 305644

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.10	63.31
264.00	62.80	62.25
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112221\
 Data File : BP008075.D
 Acq On : 22 Nov 2021 10:36
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Nov 23 03:03:25 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111921.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Nov 20 00:21:11 2021
 Response via : Initial Calibration

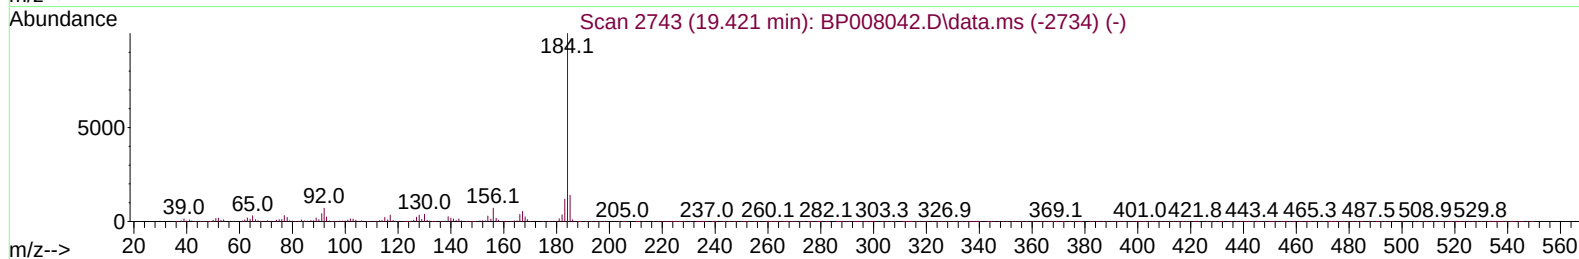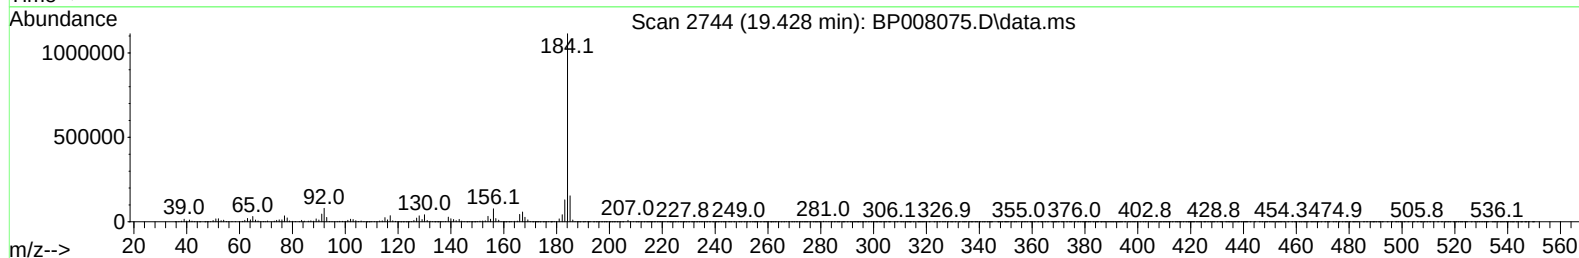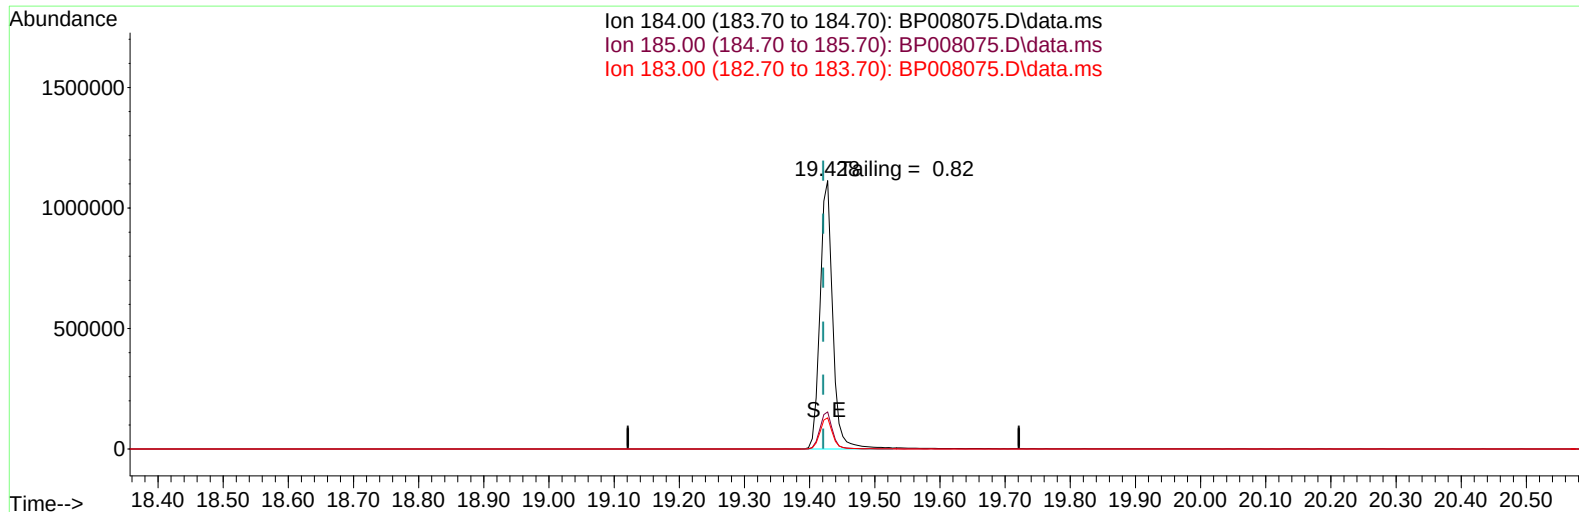

TIC: BP008075.D\data.ms

(77) Benzidine

19.428min (+ 0.007) 63822.61 ng

response 1515959

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	13.83
183.00	11.80	11.62
0.00	0.00	0.00

Instrument :
BNA_P
ClientSampleId :
DFTPP

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/22/2021	BNA_P	BP008075.D
Compound Name	Response	Retention Time
DDT	778621	20.633
DDD	9582	20.204
DDE	760	19.73
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10342	788963	1.31