
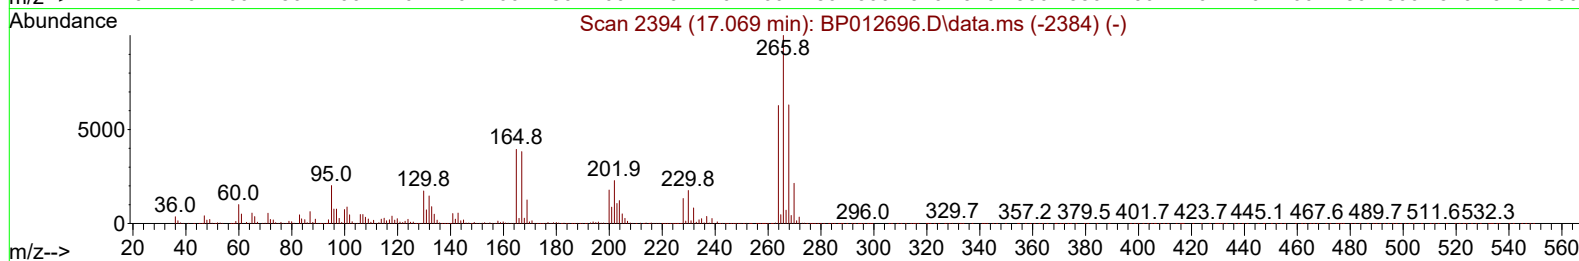
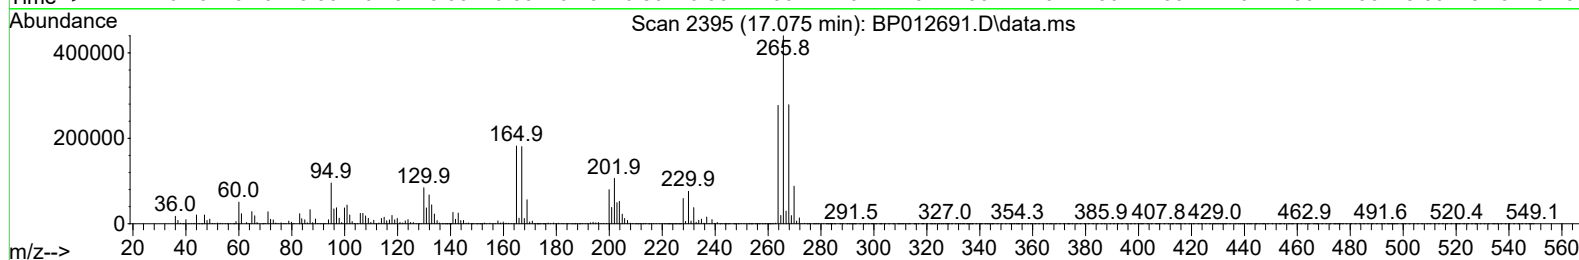


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112222\
Data File : BP012691.D
Acq On : 22 Nov 2022 08:54
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 23 06:37:22 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 23 00:38:14 2022
Response via : Initial Calibration

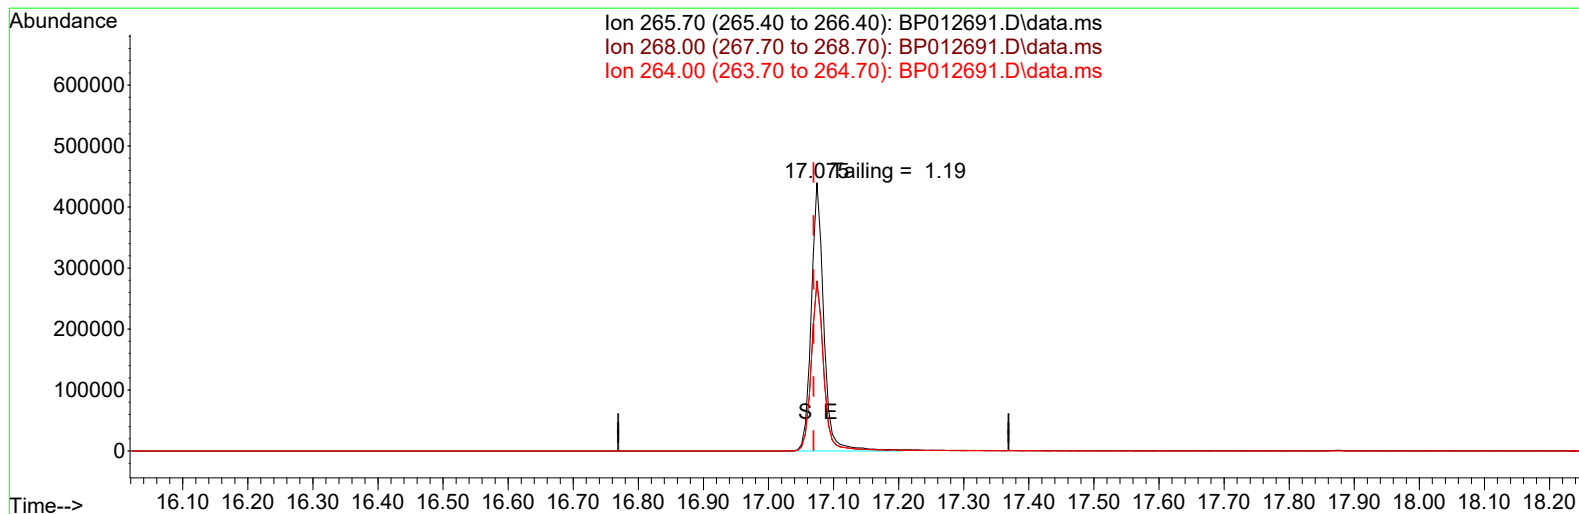

TIC: BP012691.D\data.ms

(70) Pentachlorophenol (C)




17.075min (+ 0.006) 214588.50 ng

response 595927

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	63.35
264.00	62.70	63.02
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112222\
Data File : BP012691.D
Acq On : 22 Nov 2022 08:54
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 23 06:37:22 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 23 00:38:14 2022
Response via : Initial Calibration

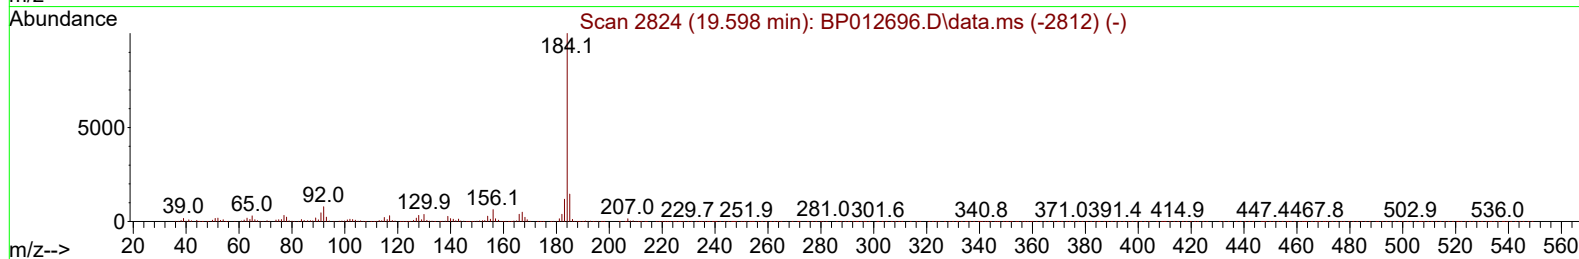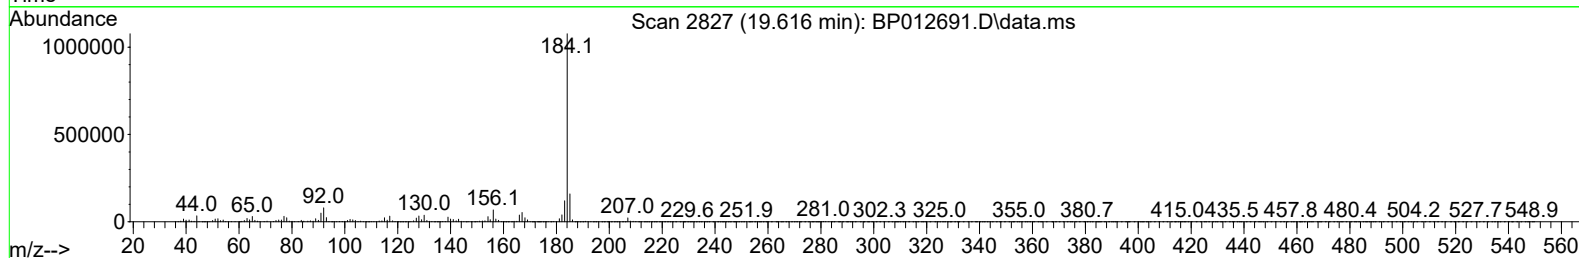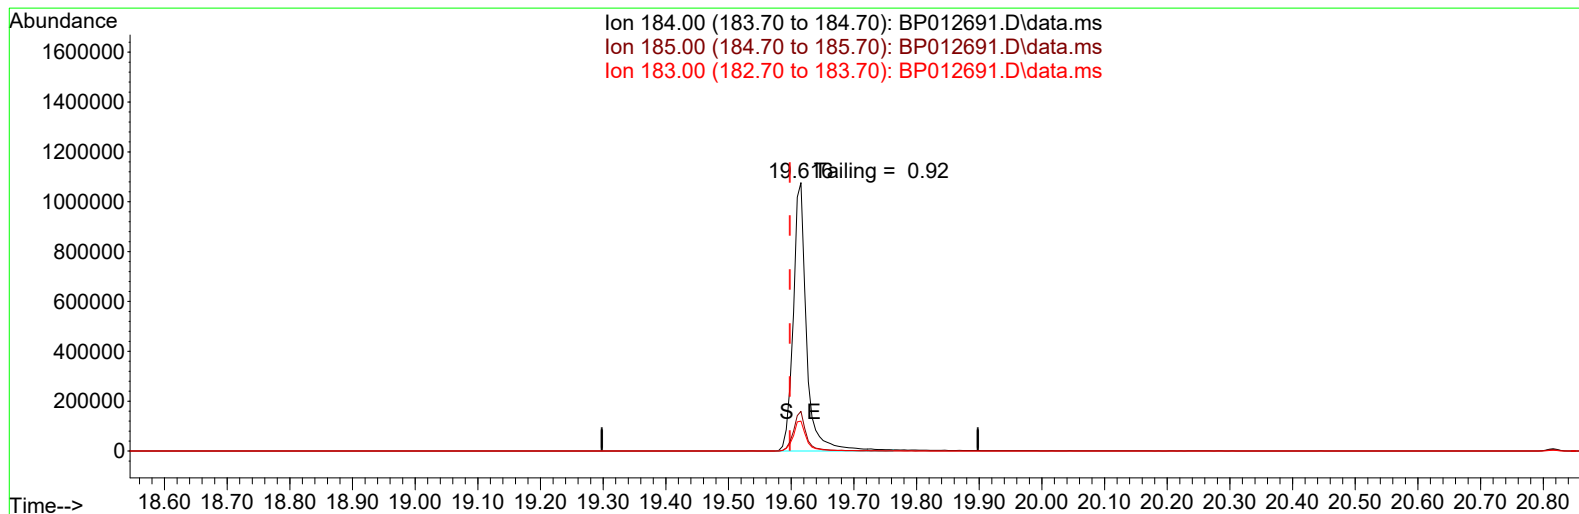

TIC: BP012691.D\data.ms

(77) Benzidine**19.616min (+ 0.018) 93885.37 ng****response 1612084**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.82
183.00	11.80	11.14
0.00	0.00	0.00