
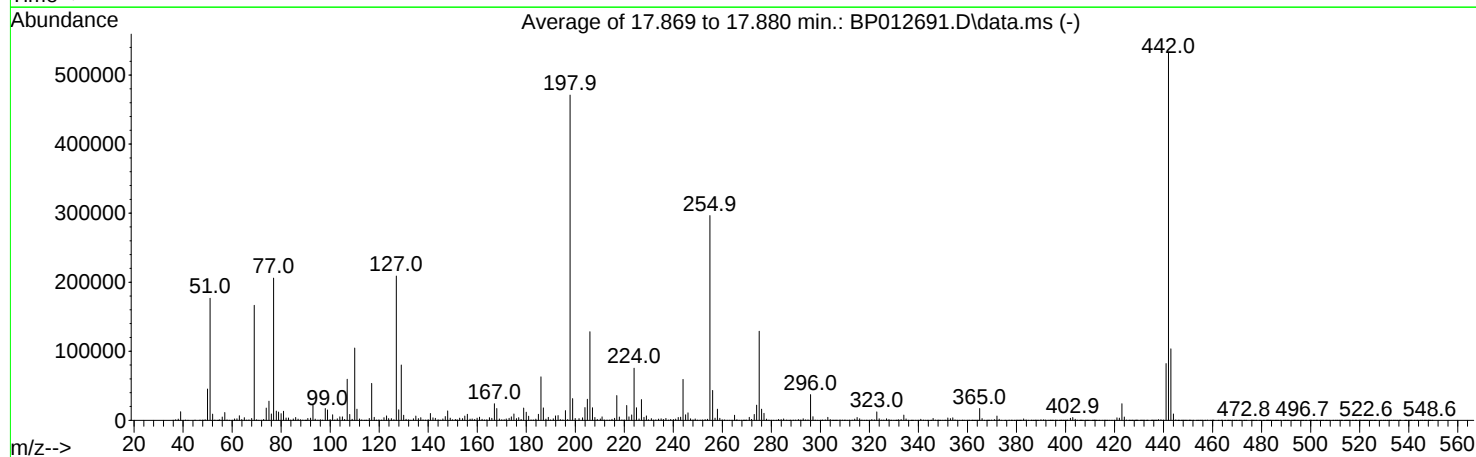


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112222\
 Data File : BP012691.D
 Acq On : 22 Nov 2022 08:54
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112222.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Nov 23 00:38:14 2022

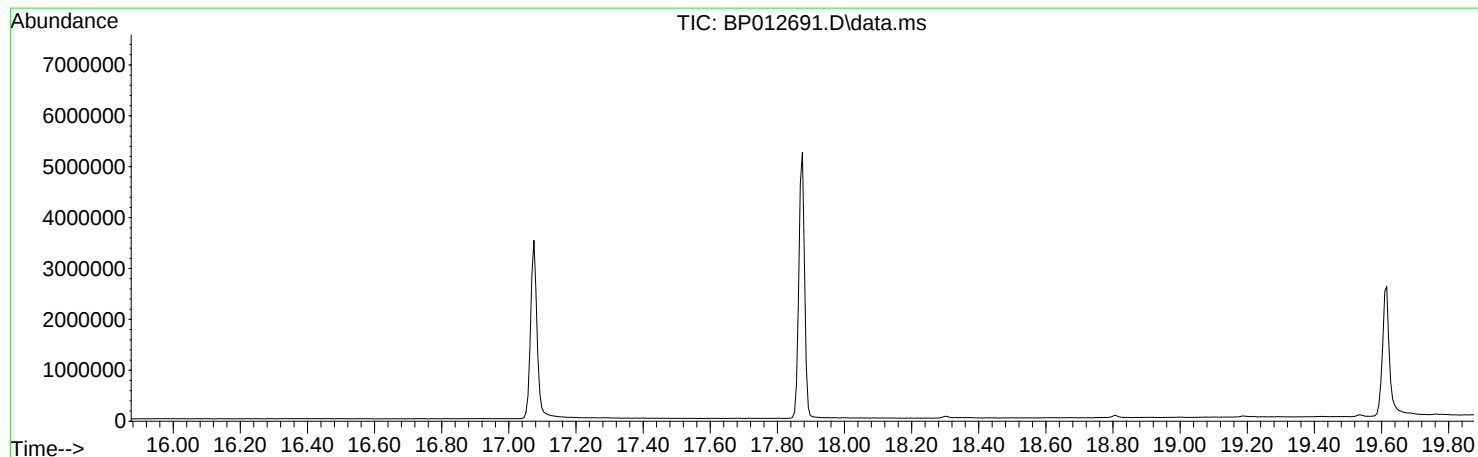




AutoFind: Scans 2530, 2531, 2532; Background Corrected with Scan 2519

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.5	176694	PASS
68	69	0.00	2	1.6	2654	PASS
69	198	0.00	100	35.4	166528	PASS
70	69	0.00	2	0.5	785	PASS
127	198	10	80	44.4	208896	PASS
197	198	0.00	2	0.2	1043	PASS
198	198	100	100	100.0	470985	PASS
199	198	5	9	6.7	31460	PASS
275	198	10	60	27.4	128909	PASS
365	198	1	100	3.6	17105	PASS
441	198	0.01	100	17.5	82264	PASS
442	442	100	100	100.0	532801	PASS
443	442	15	24	19.4	103520	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112222\
Data File : BP012691.D
Acq On : 22 Nov 2022 08:54
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Nov 23 06:37:22 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 23 00:38:14 2022
Response via : Initial Calibration

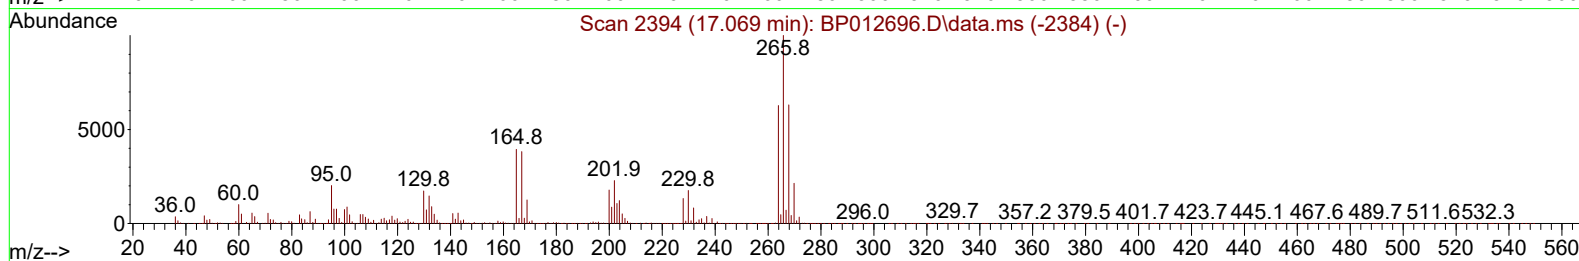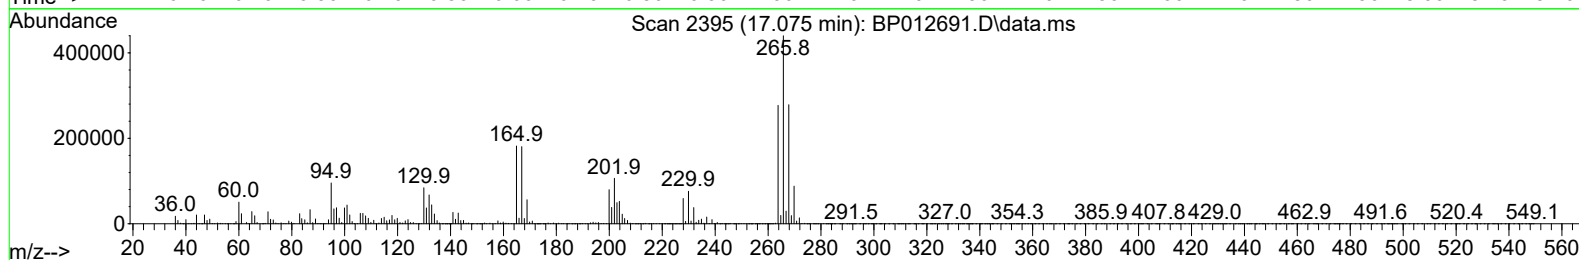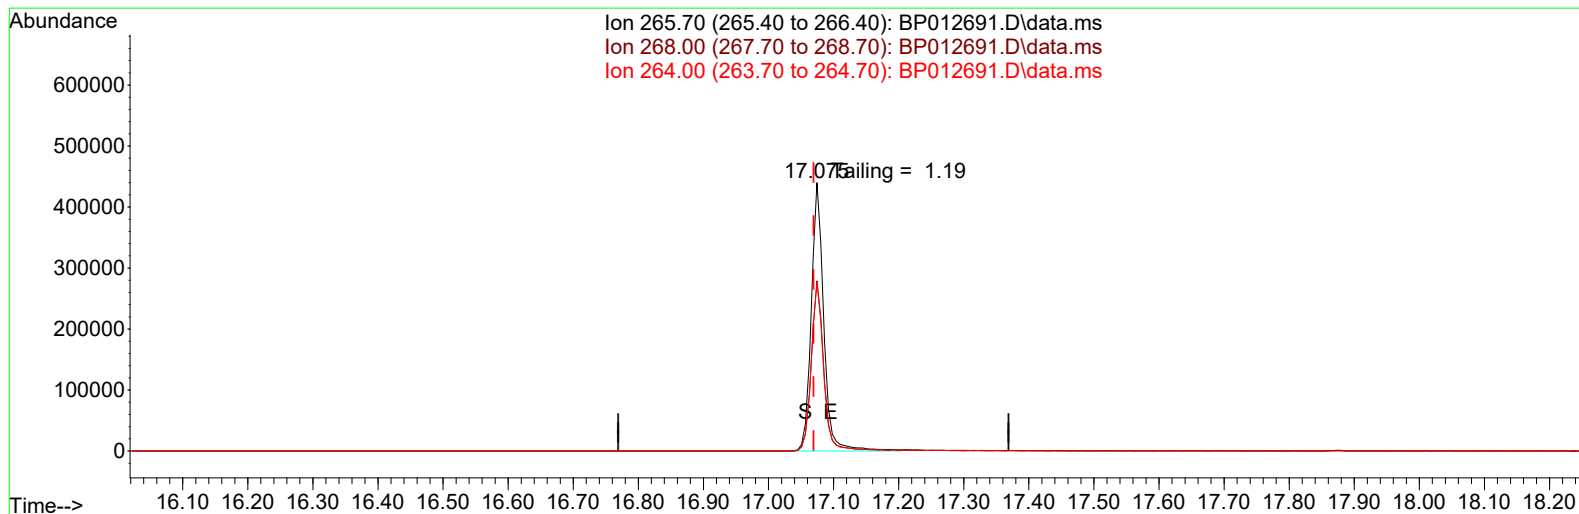

TIC: BP012691.D\data.ms

(70) Pentachlorophenol (C)

17.075min (+ 0.006) 214588.50 ng




response 595927

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	63.35
264.00	62.70	63.02
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112222\
Data File : BP012691.D
Acq On : 22 Nov 2022 08:54
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Nov 23 06:37:22 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 23 00:38:14 2022
Response via : Initial Calibration

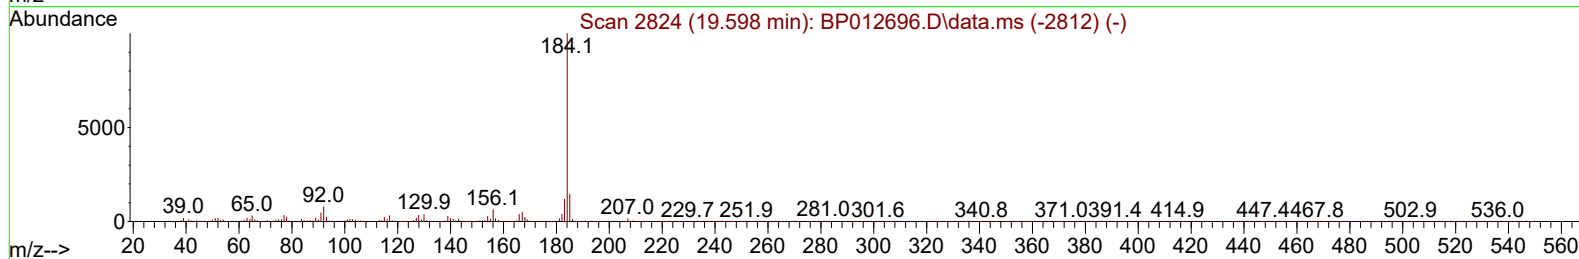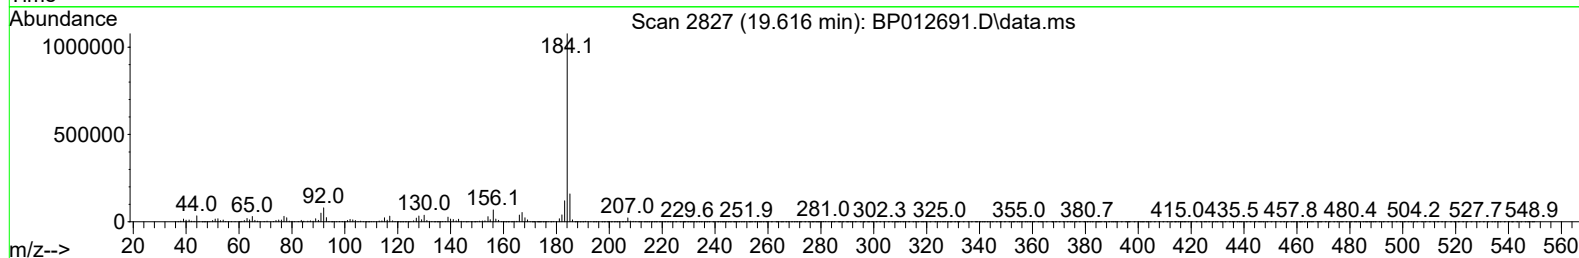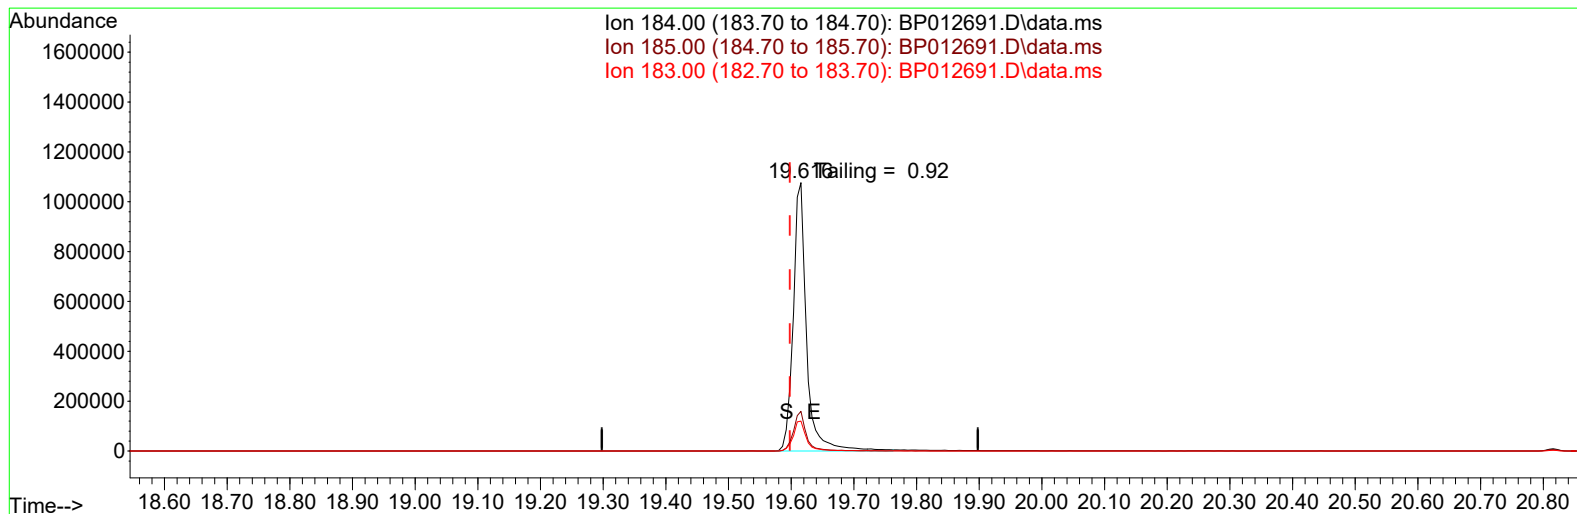

TIC: BP012691.D\data.ms

(77) Benzidine

19.616min (+ 0.018) 93885.37 ng

response 1612084

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.82
183.00	11.80	11.14
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/22/2022	BNA_P	<u>BP012691.D</u>
Compound Name	Response	Retention Time
DDT	1194972	20.815
DDD	20303	20.386
DDE	1414	19.892
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
21717	1216689	1.78

Instrument :
BNA_P
ClientSampleId :
DFTPP